

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111418\
 Data File : BG038008.D
 Acq On : 14 Nov 2018 22:15
 Operator : JU/SJ
 Sample : J5889-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WALL-D

Quant Time: Nov 15 03:01:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	53414	20.00	ng	0.00
21) Naphthalene-d8	10.90	136	233982	20.00	ng	0.00
39) Acenaphthene-d10	14.72	164	147560	20.00	ng	0.00
64) Phenanthrene-d10	17.47	188	351409	20.00	ng	0.00
76) Chrysene-d12	21.75	240	323833	20.00	ng	0.00
87) Perylene-d12	25.06	264	330127	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	341103	110.26	ng	0.00
7) Phenol-d6	7.23	99	489751	110.90	ng	0.00
23) Nitrobenzene-d5	9.26	82	294295	67.33	ng	0.00
42) 2,4,6-Tribromophenol	16.21	330	167399	99.47	ng	0.00
45) 2-Fluorobiphenyl	13.34	172	662266	65.39	ng	0.00
79) Terphenyl-d14	20.07	244	938548	68.20	ng	0.00
Target Compounds						
10) Phenol	7.25	94	31904	6.821	ng	92
50) Dimethylphthalate	14.16	163	83760	7.160	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG111418\
Data File : BG038008.D
Acq On : 14 Nov 2018 22:15
Operator : JU/SJ
Sample : J5889-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WALL-D

Quant Time: Nov 15 03:01:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

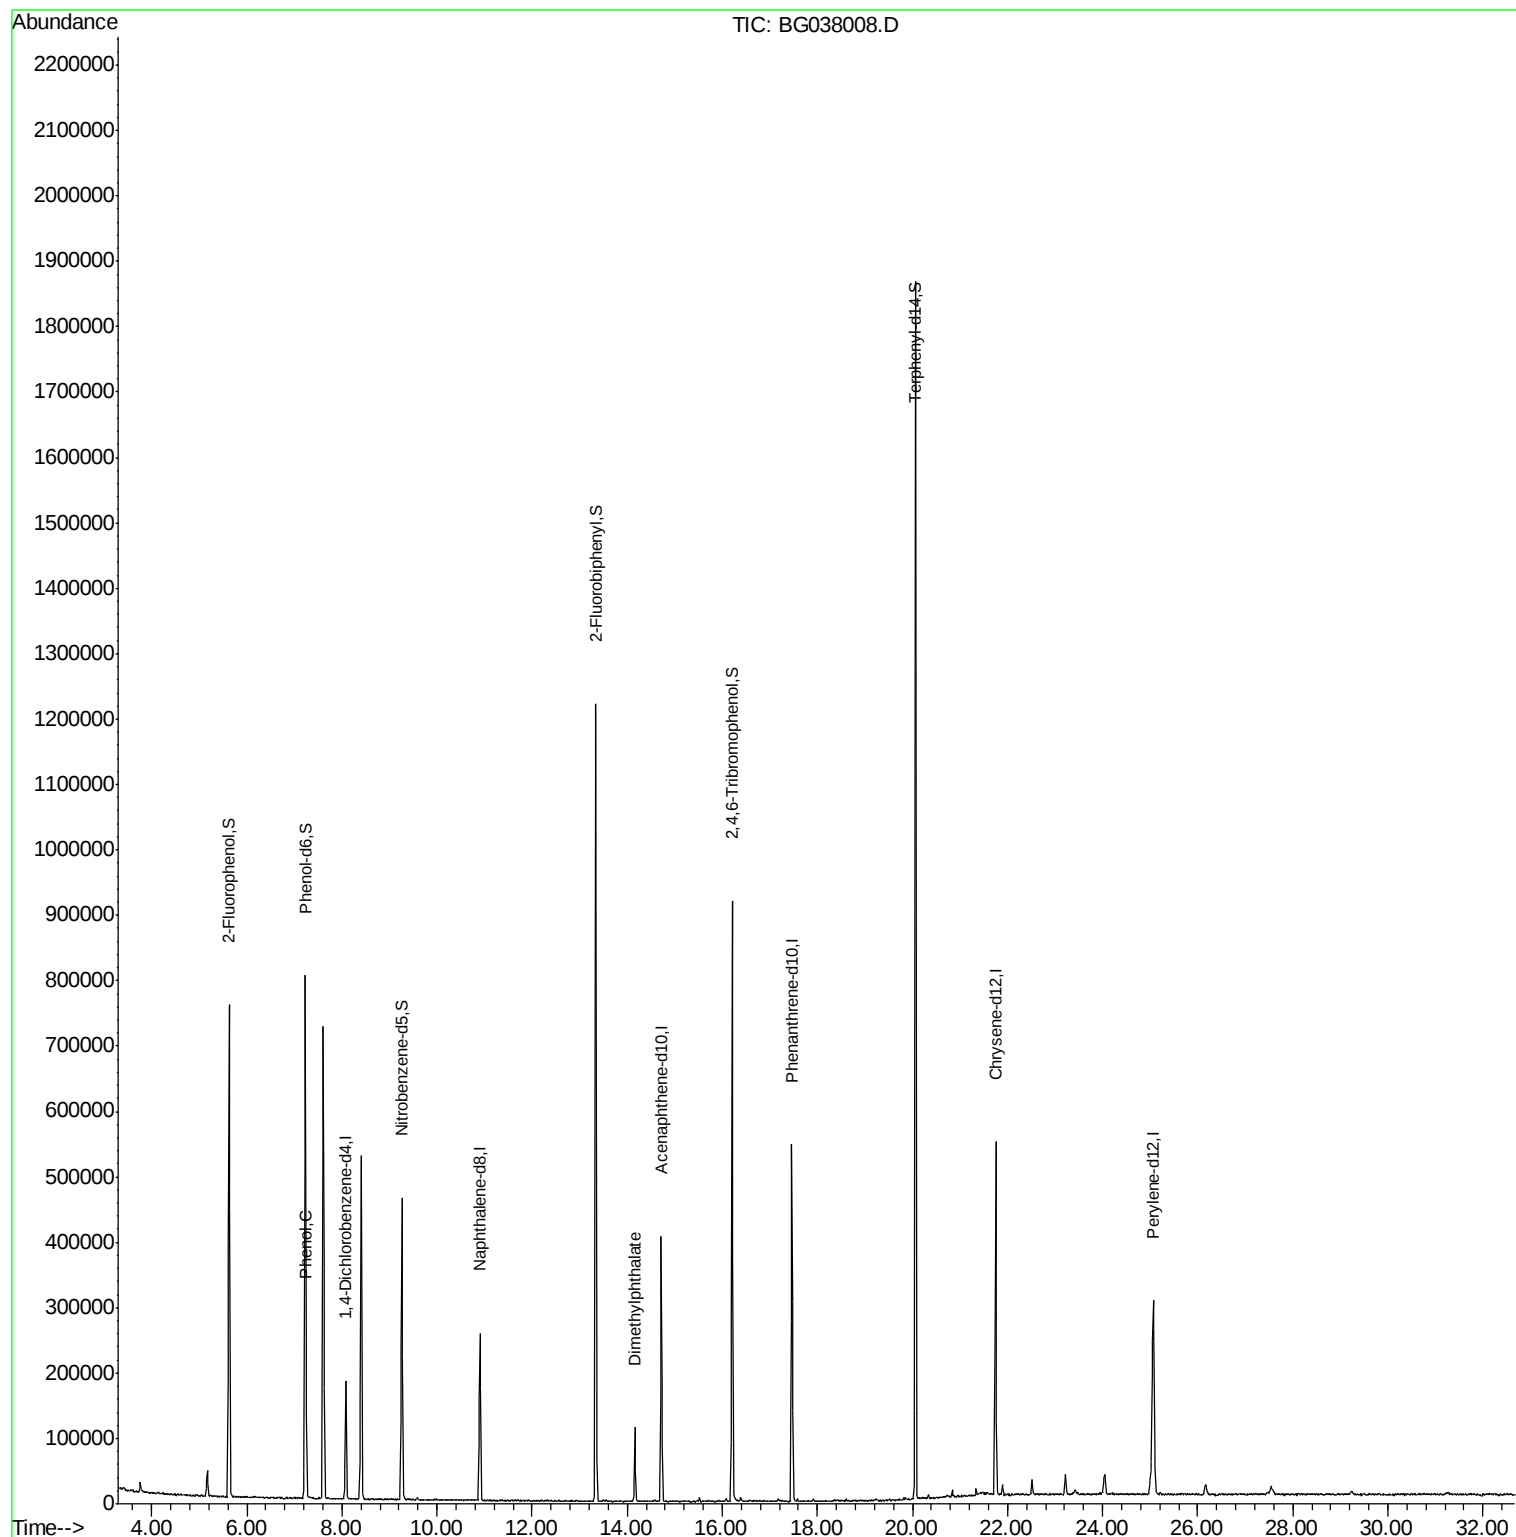

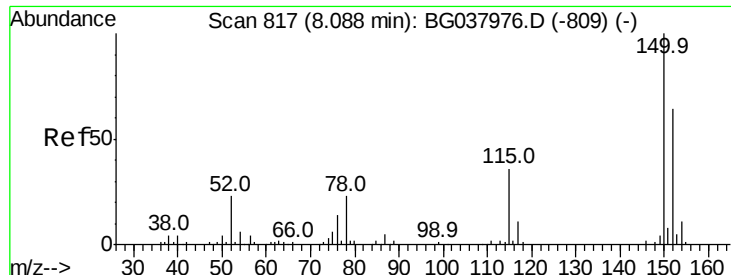


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.08 min Scan# 816
Delta R.T. -0.01 min
Lab File: BG038008.D
Acq: 14 Nov 2018 22:15

Instrument :
BNA_G
ClientSampleId :
WALL-D

Tot Ion:152 Resp: 53414
Ion Ratio Lower Upper
152 100
150 152.6 126.0 189.0
115 54.2 45.5 68.3

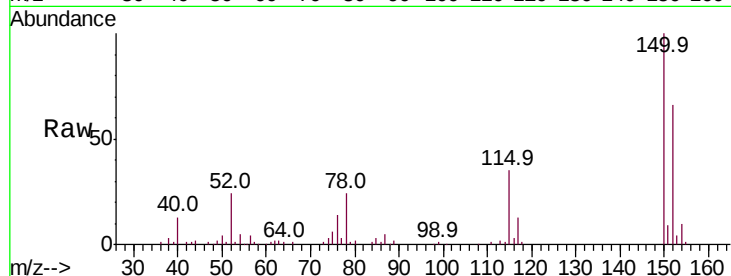


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

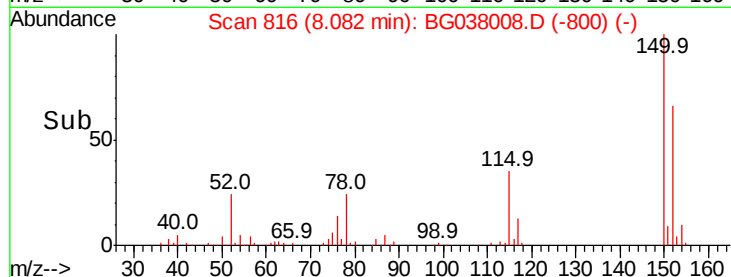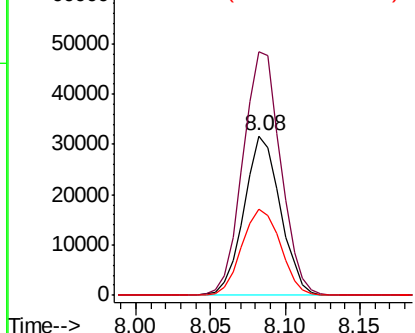



#5


2-Fluorophenol
Concen: 110.259 ng
RT: 5.63 min Scan# 398
Delta R.T. -0.01 min
Lab File: BG038008.D
Acq: 14 Nov 2018 22:15

Tgt Ion:112 Resp: 341103
Ion Ratio Lower Upper
112 100
64 65.8 53.1 79.7
63 35.0 27.3 40.9

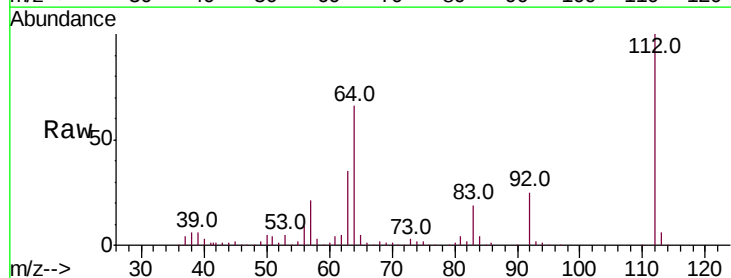

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

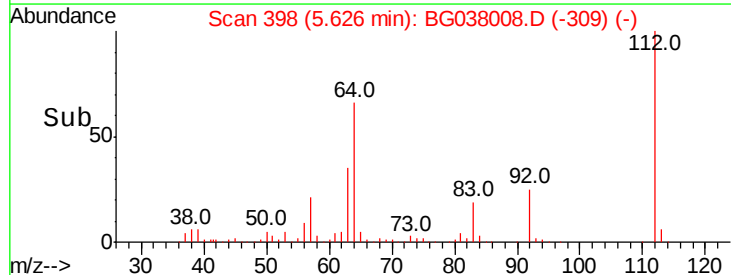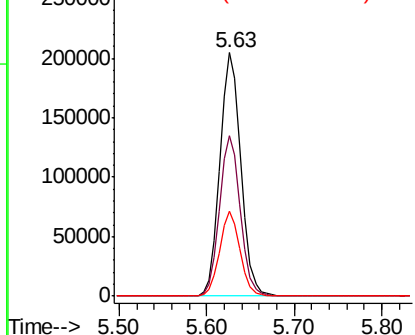

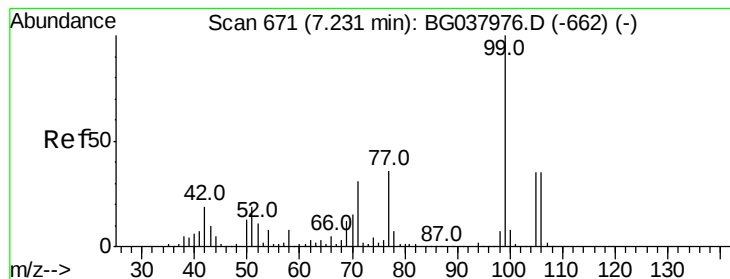

#7

Phenol-d6

Concen: 110.904 ng

RT: 7.23 min Scan# 671

Delta R.T. -0.00 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15

Instrument :

BNA_G

ClientSampleId :

WALL-D


Tot Ion: 99 Resp: 489751

Ion Ratio Lower Upper




99 100

42 18.4 15.0 22.4

71 31.3 25.5 38.3

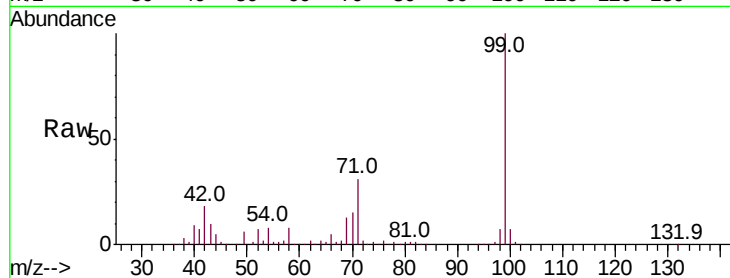

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

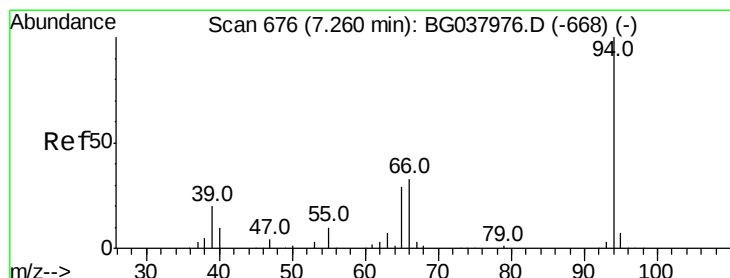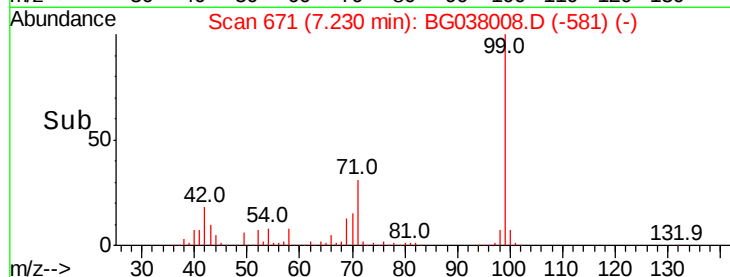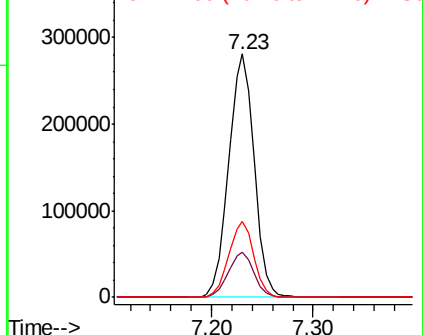

#10

Phenol

Concen: 6.821 ng

RT: 7.25 min Scan# 675

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15


Tgt Ion: 94 Resp: 31904

Ion Ratio Lower Upper



94 100


65 33.3 9.7 49.7

66 41.5 15.9 55.9

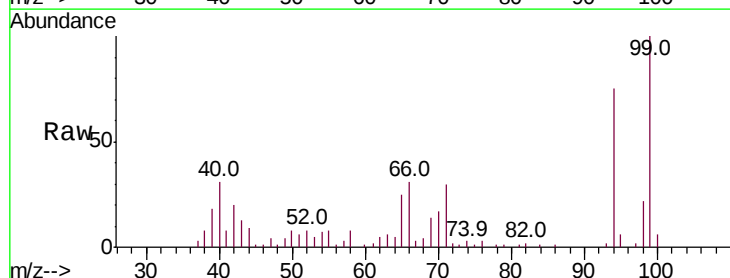

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

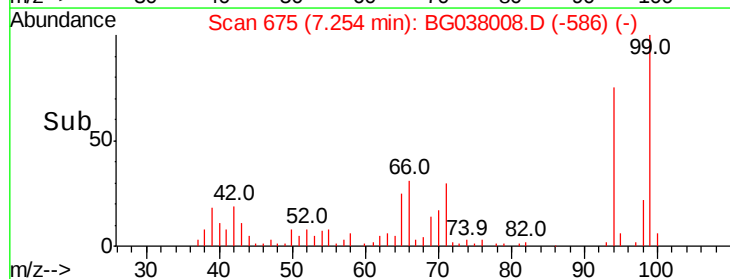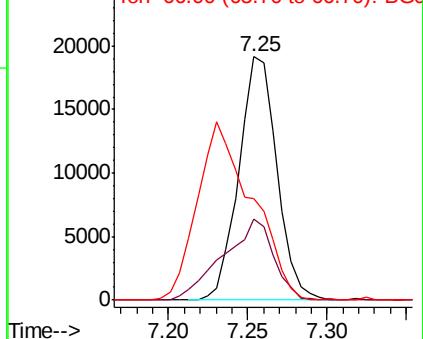

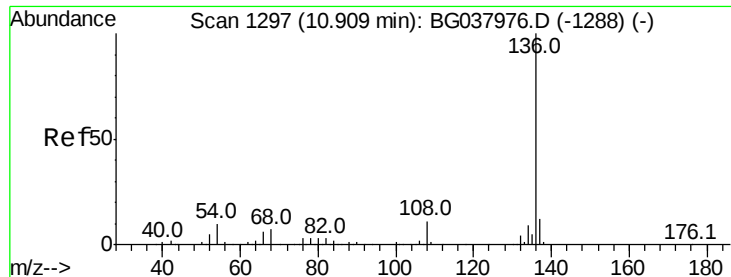

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.90 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15

Instrument :

BNA_G

ClientSampleId :

WALL-D

Tot Ion:136 Resp: 233982



Ion Ratio Lower Upper

136 100

137 11.8 9.6 14.4

54 9.7 7.9 11.9

68 6.6 4.8 7.2

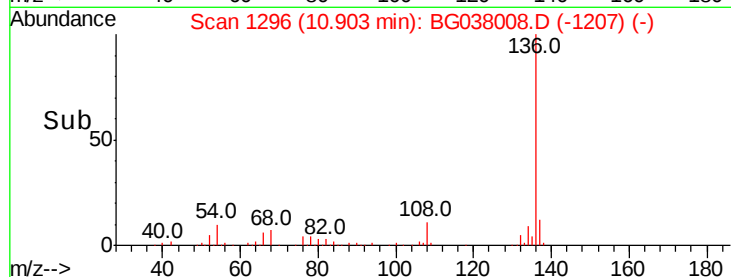
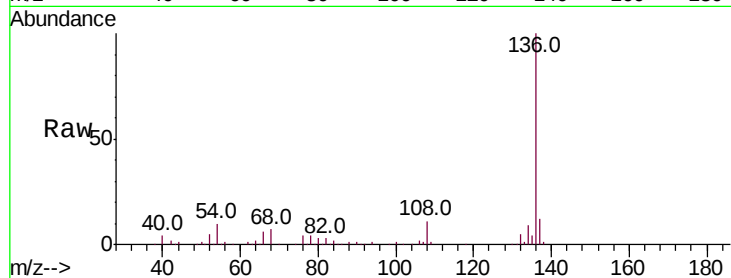


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

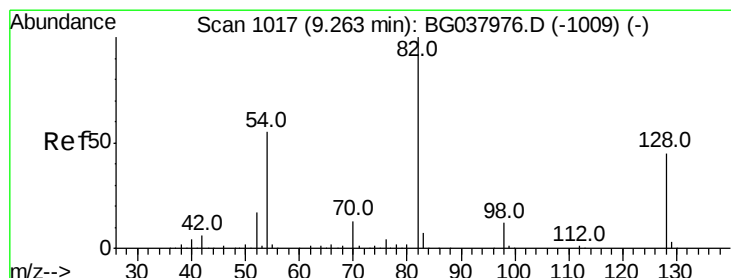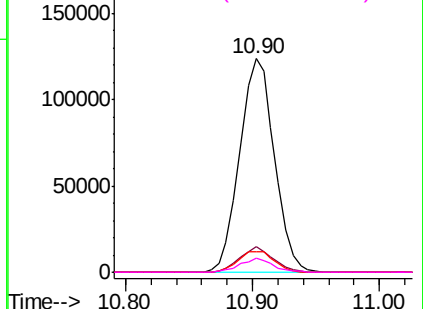

#23

Nitrobenzene-d5

Concen: 67.329 ng

RT: 9.26 min Scan# 1016

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15



Tgt Ion: 82 Resp: 294295

Ion Ratio Lower Upper

82 100

128 44.9 34.6 51.8


54 55.3 45.3 67.9

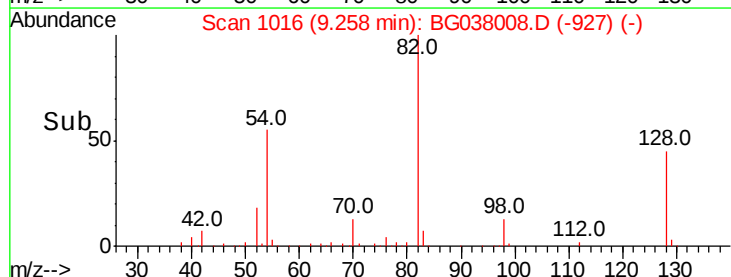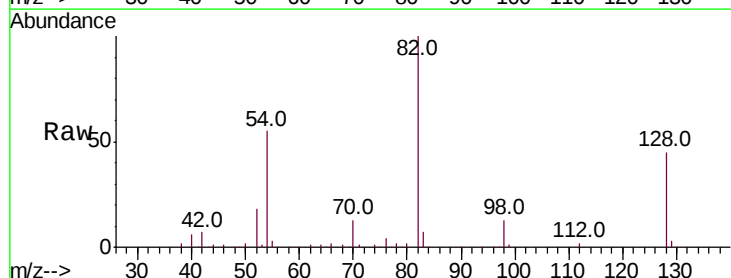

Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BGC

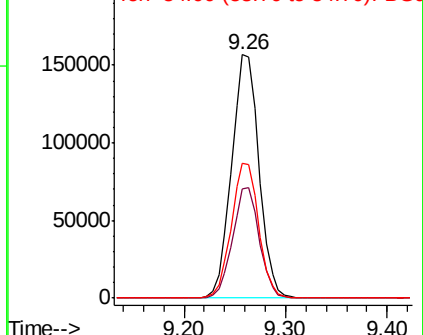



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.72 min Scan# 1945

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15

Instrument :

BNA_G

ClientSampleId :

WALL-D


Tot Ion:164 Resp: 147560

Ion Ratio Lower Upper

164 100

162 103.0 81.3 121.9




160 45.3 36.3 54.5

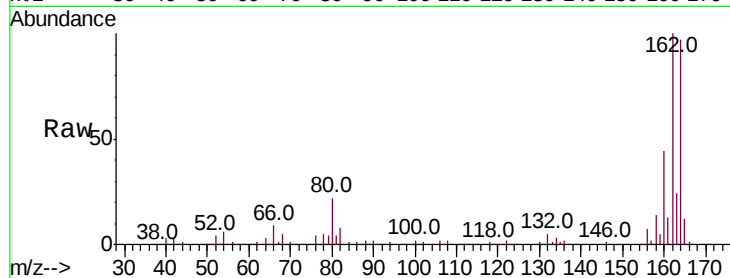

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

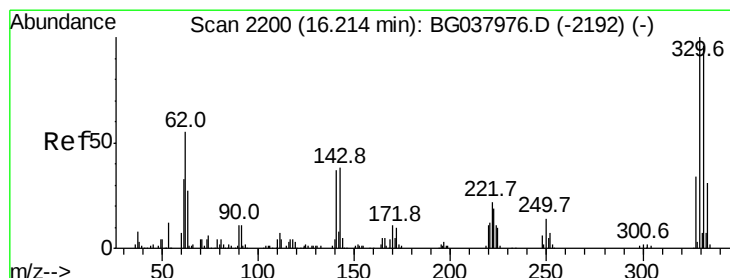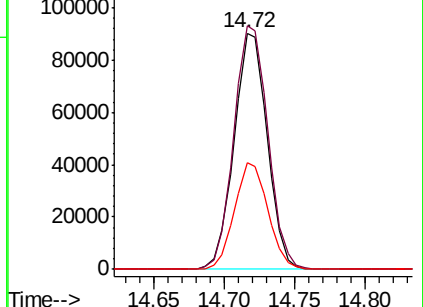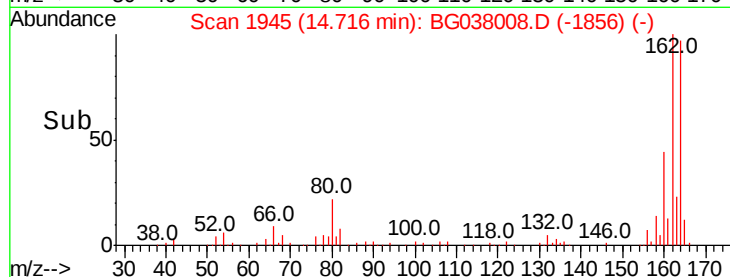

#42

2,4,6-Tribromophenol

Concen: 99.471 ng

RT: 16.21 min Scan# 2199

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15


Tgt Ion:330 Resp: 167399

Ion Ratio Lower Upper

330 100

332 97.0 78.4 117.6



141 39.7 32.2 48.2

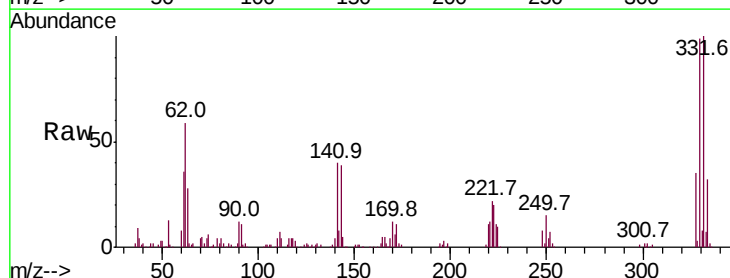


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

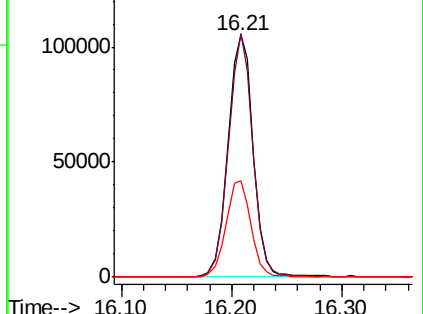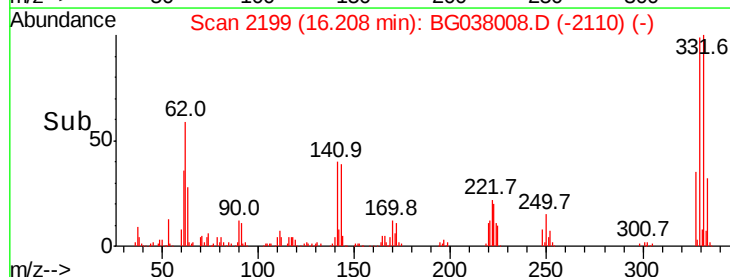

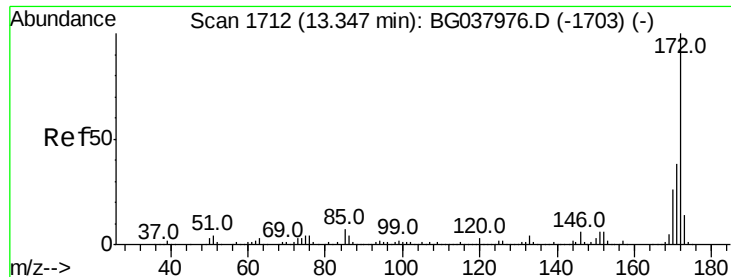

#45

2-Fluorobiphenyl

Concen: 65.385 ng

RT: 13.34 min Scan# 1711

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15

Instrument :


BNA_G

ClientSampled :

WALL-D

Tot Ion:172 Resp: 662266

Ion	Ratio	Lower	Upper
172	100		
171	38.0	31.0	46.4
170	24.3	20.2	30.2



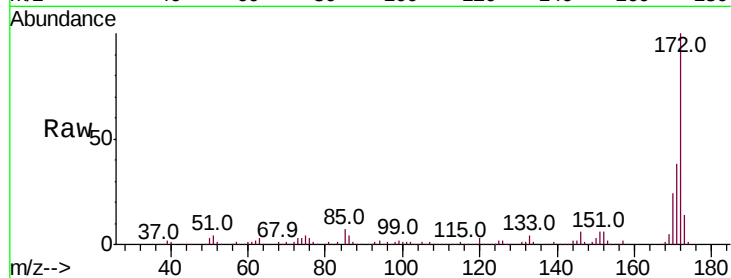


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

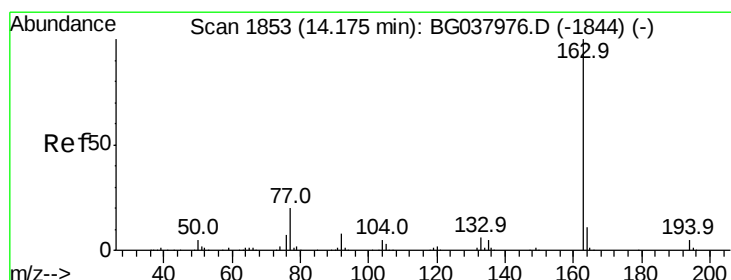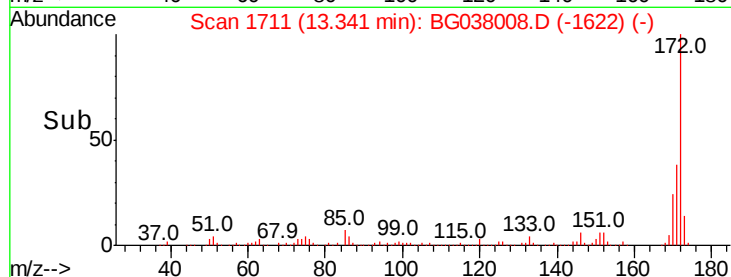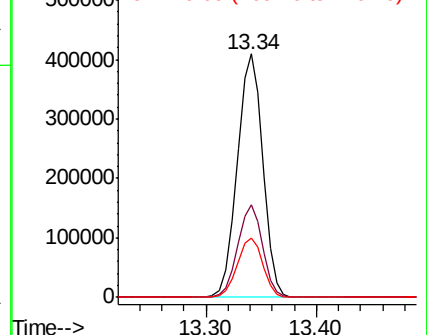

#50

Dimethylphthalate

Concen: 7.160 ng

RT: 14.16 min Scan# 1851


Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15

Tgt Ion:163 Resp: 83760

Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.5	5.3
164	10.1	8.5	12.7


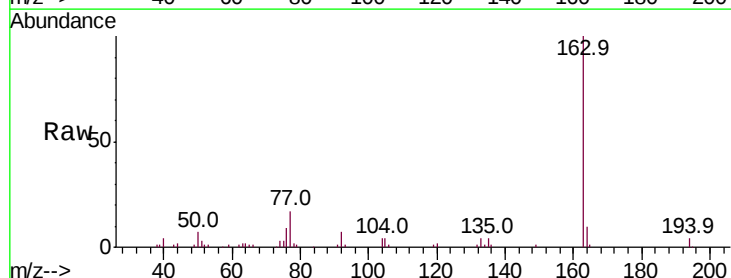



Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

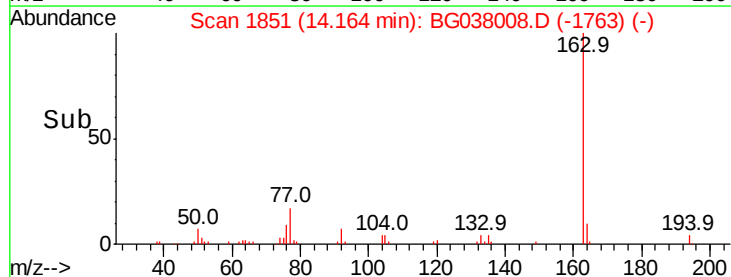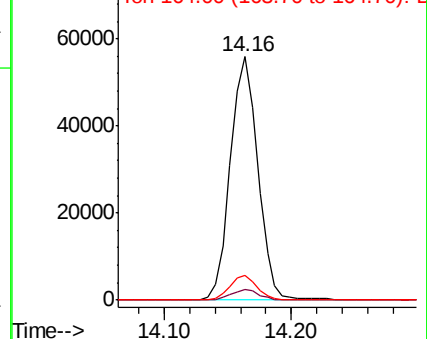

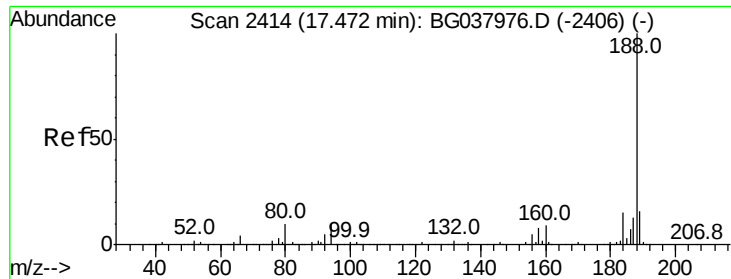

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.47 min Scan# 2413

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15

Instrument :

BNA_G

ClientSampleId :

WALL-D


Tot Ion:188 Resp: 351409

Ion Ratio Lower Upper

188 100

94 9.1 7.2 10.8




80 10.0 7.7 11.5

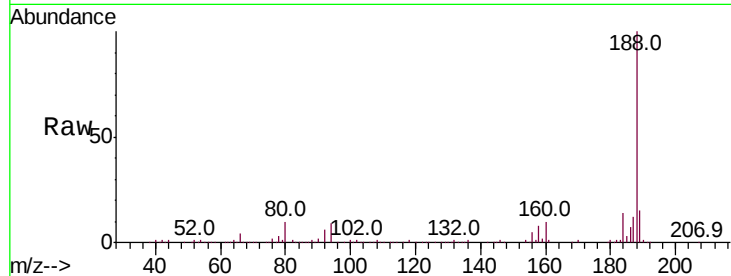

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

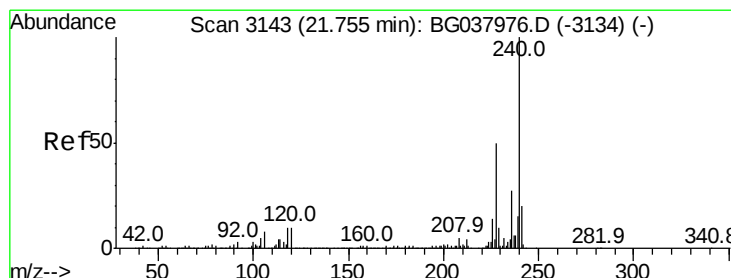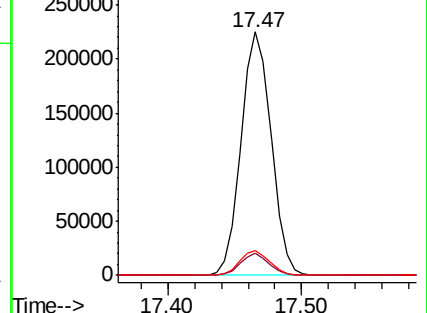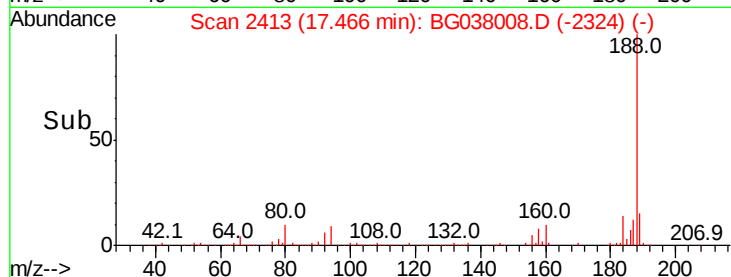

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.75 min Scan# 3142

Delta R.T. -0.01 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15


Tgt Ion:240 Resp: 323833

Ion Ratio Lower Upper

240 100

120 10.7 8.1 12.1



236 27.7 21.4 32.0

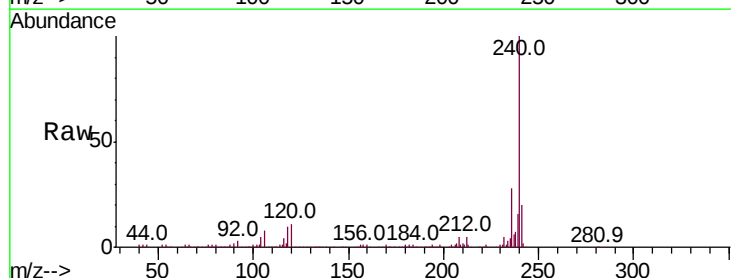


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

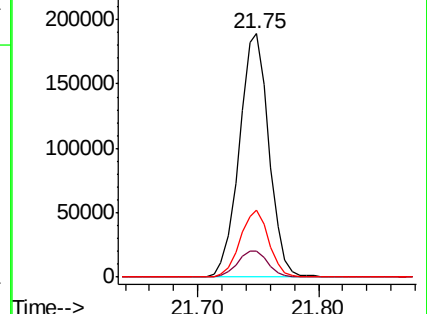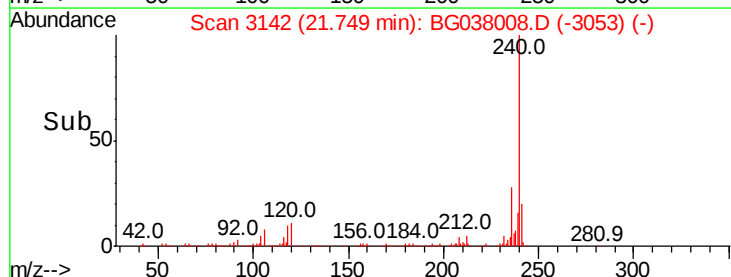

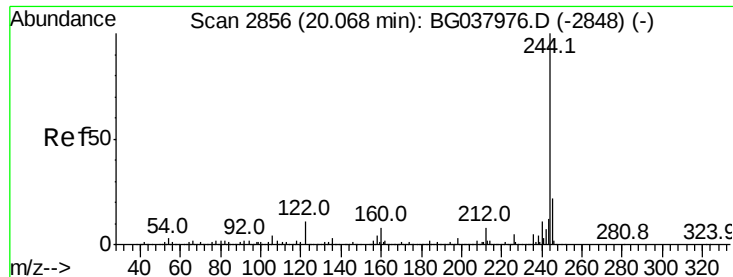

#79

Terphenyl-d14

Concen: 68.196 ng

RT: 20.07 min Scan# 2856

Delta R.T. 0.00 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15

Instrument :

BNA_G

ClientSampleId :

WALL-D


Tot Ion:244 Resp: 938548

Ion Ratio Lower Upper

244 100

212 7.9 6.5 9.7




122 10.6 9.0 13.4

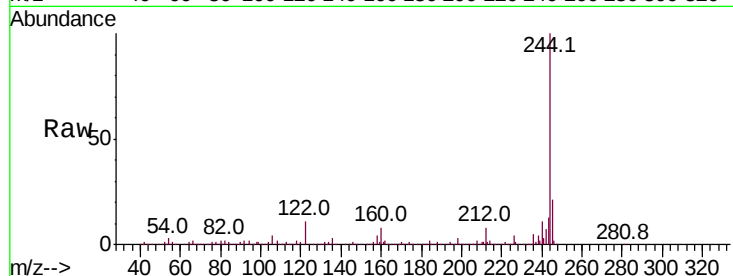

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

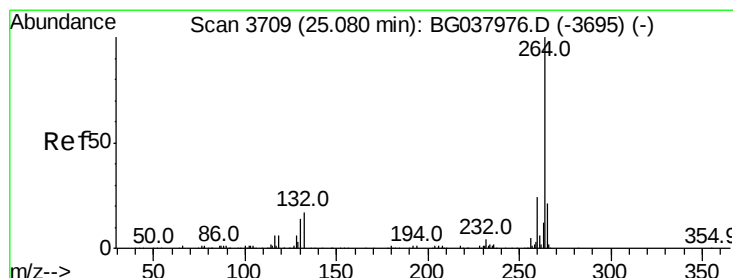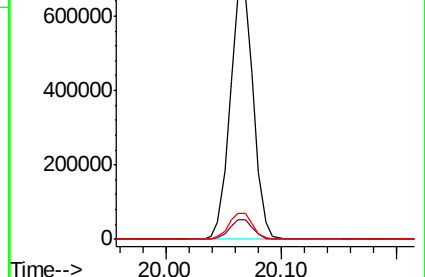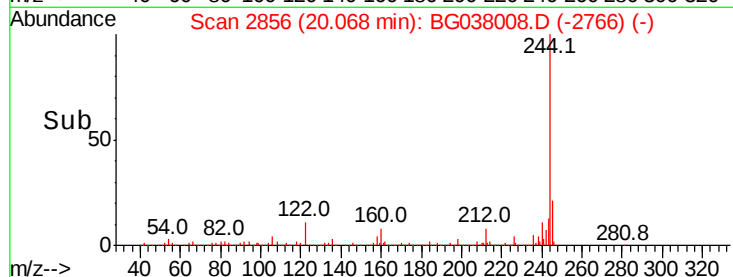

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.06 min Scan# 3706

Delta R.T. -0.02 min

Lab File: BG038008.D

Acq: 14 Nov 2018 22:15


Tgt Ion:264 Resp: 330127

Ion Ratio Lower Upper

264 100

260 23.8 18.2 27.4

265 21.0 17.9 26.9

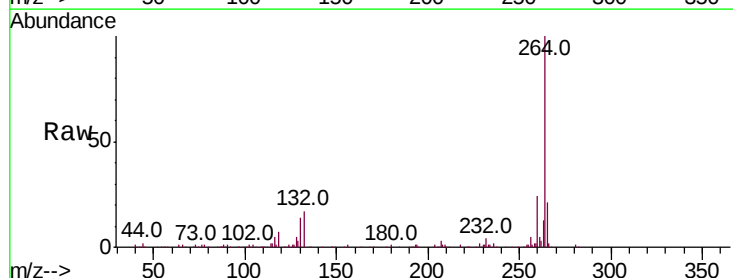

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

