
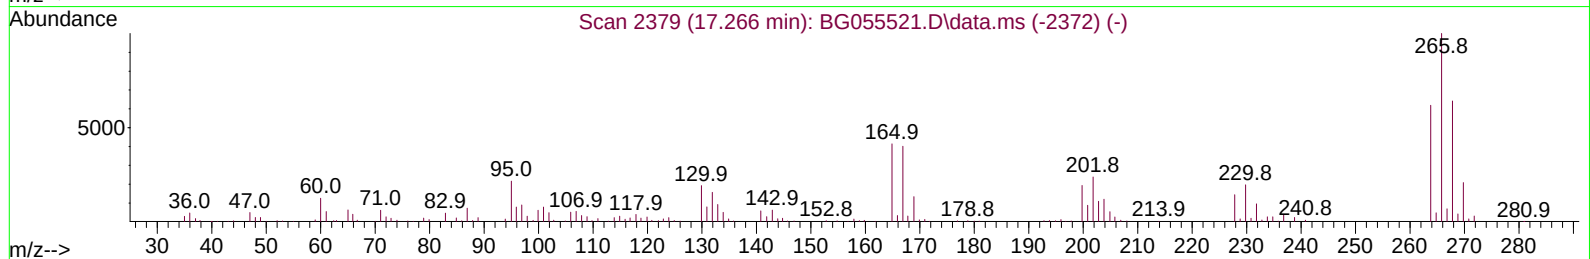
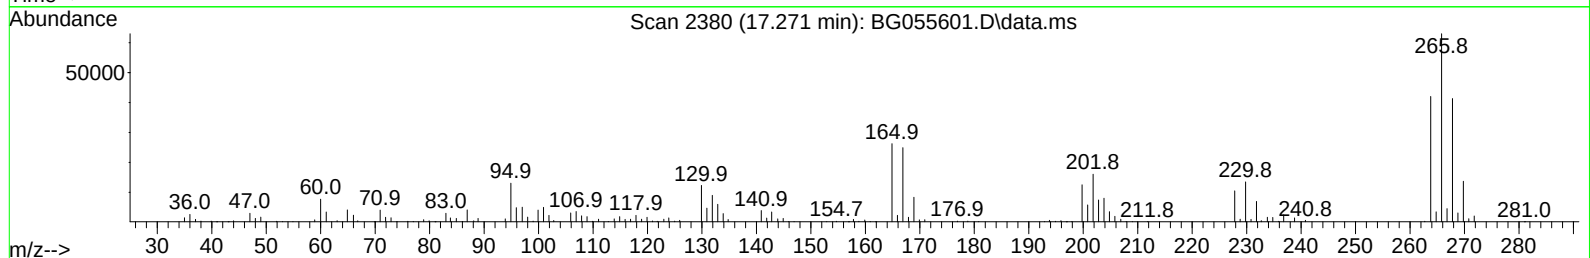


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111422\
Data File : BG055601.D
Acq On : 14 Nov 2022 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 15:59:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

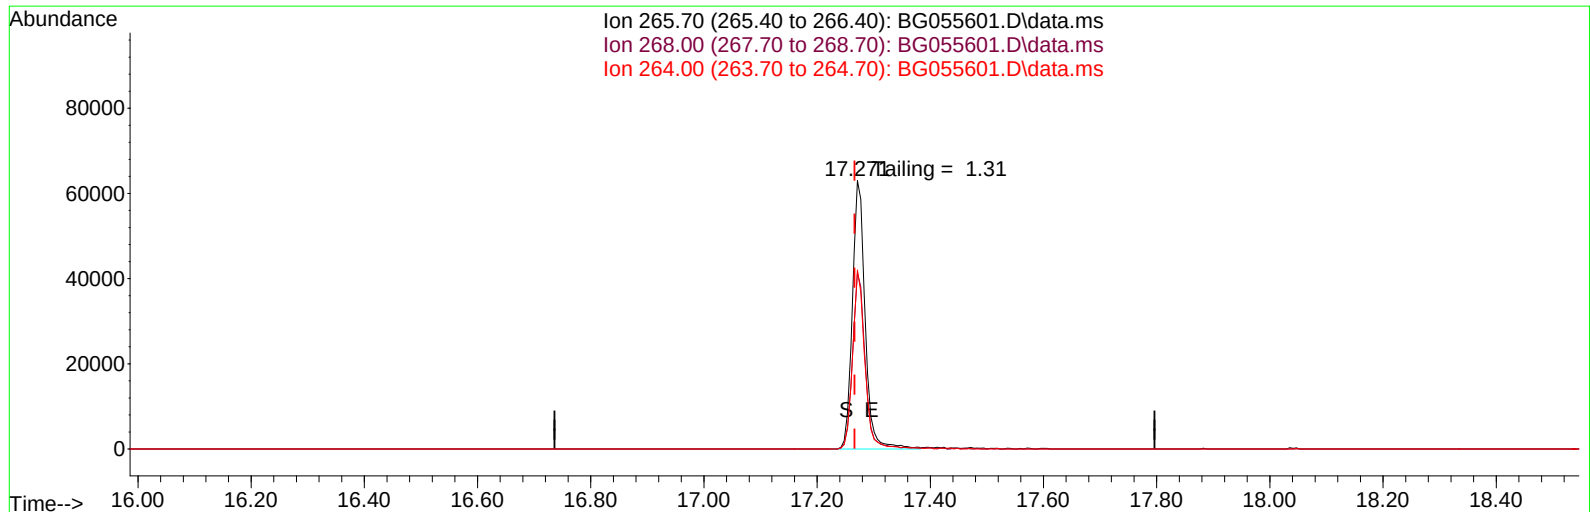

TIC: BG055601.D\data.ms

(70) Pentachlorophenol (C)




17.271min (+ 0.005) 27084.52 ng

response 98801

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	65.63
264.00	61.90	66.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111422\
 Data File : BG055601.D
 Acq On : 14 Nov 2022 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 15:59:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 10 03:39:46 2022
 Response via : Initial Calibration

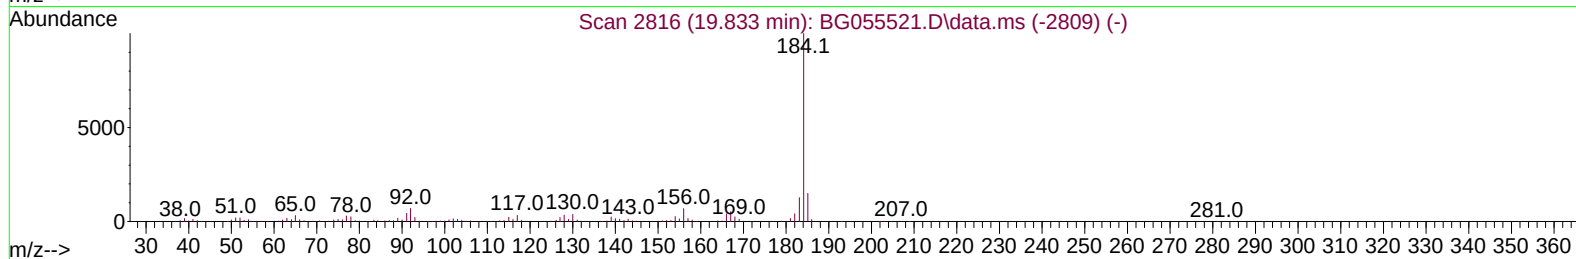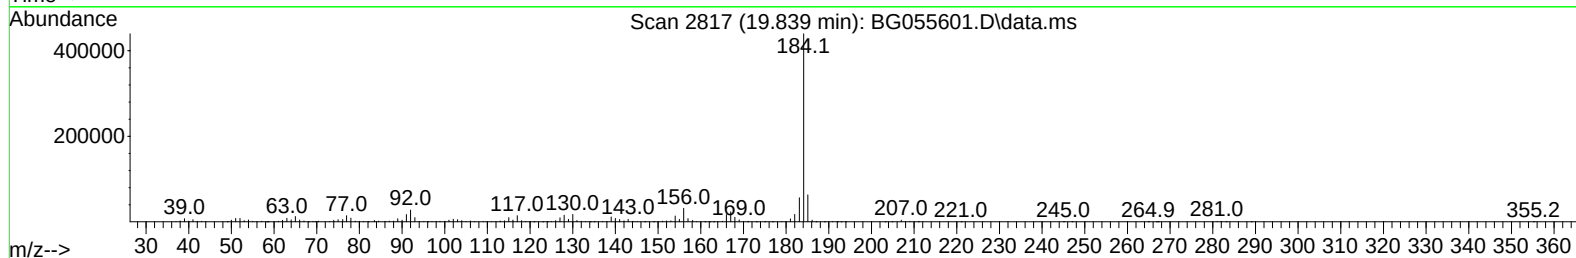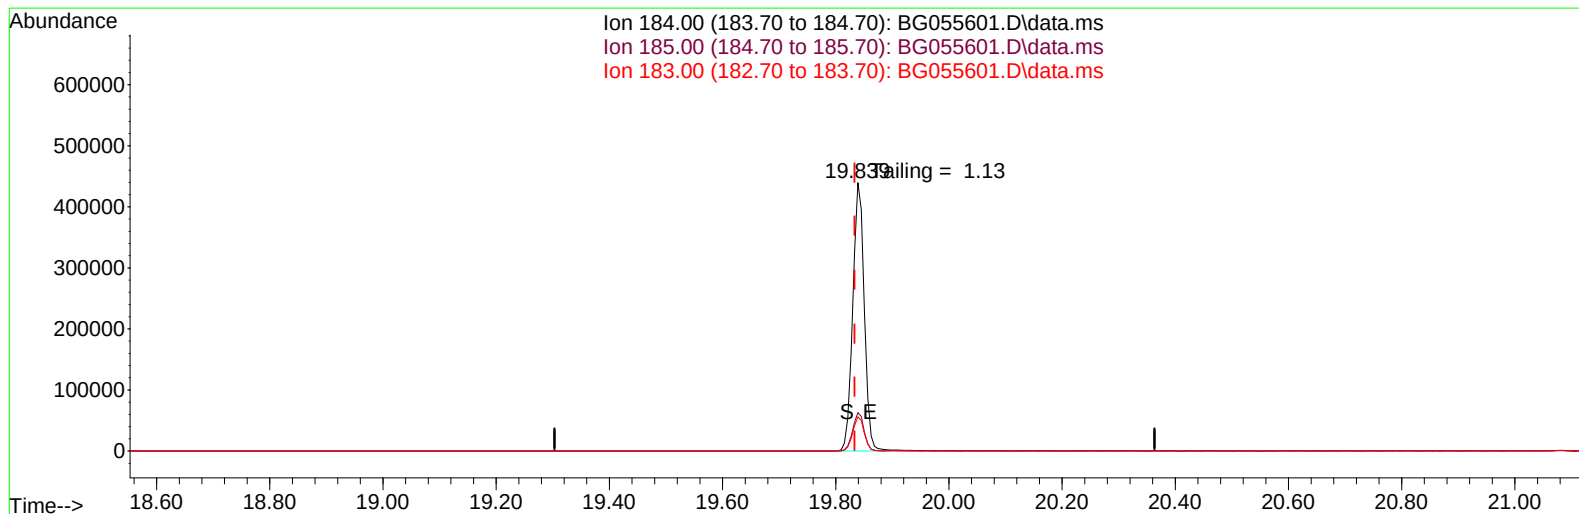

TIC: BG055601.D\data.ms

(77) Benzidine**19.839min (+ 0.006) 210903.62 ng****response 621932**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.31
183.00	12.70	12.76
0.00	0.00	0.00