
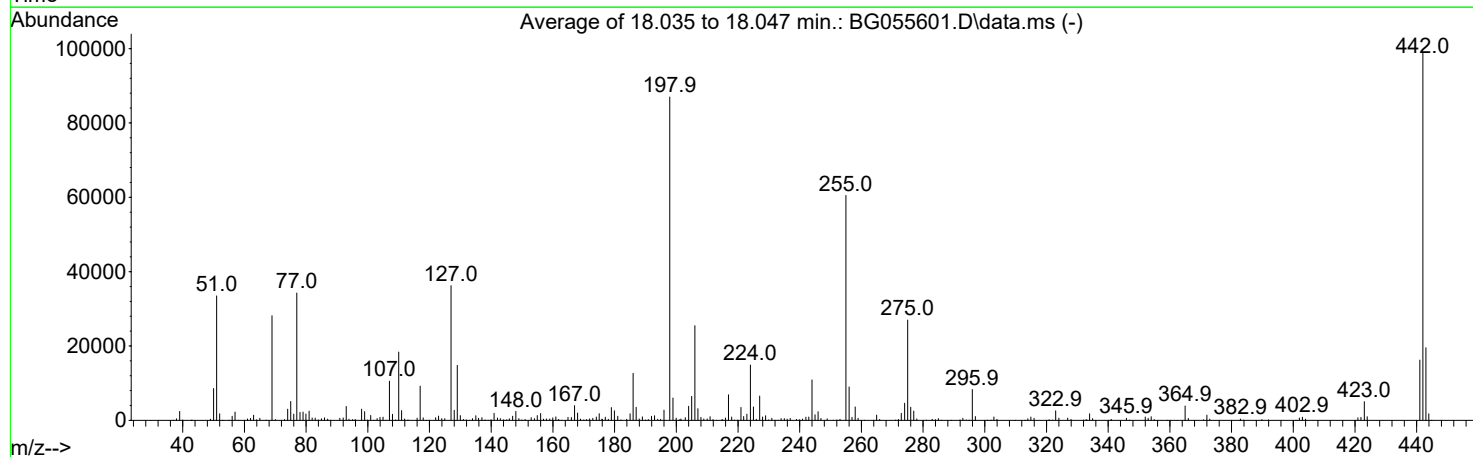


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111422\
 Data File : BG055601.D
 Acq On : 14 Nov 2022 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 03:39:46 2022

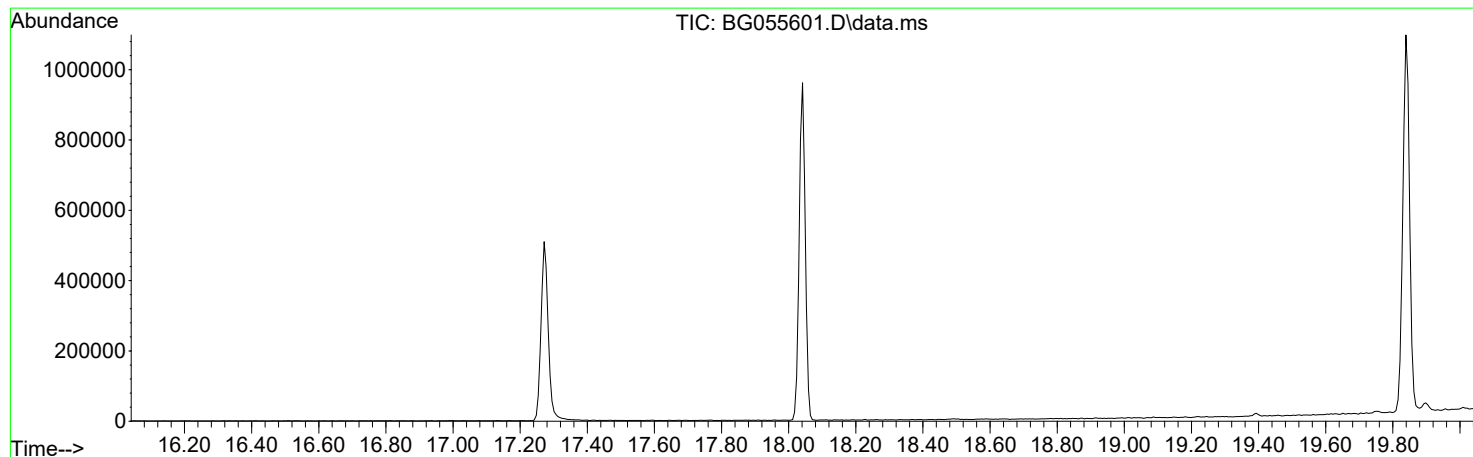

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	33499	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.4	28157	PASS
70	69	0.00	2	0.8	213	PASS
127	198	10	80	41.7	36229	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86981	PASS
199	198	5	9	6.9	6025	PASS
275	198	10	60	31.0	26997	PASS
365	198	1	100	4.5	3875	PASS
441	198	0.01	100	18.7	16223	PASS
442	442	50	100	100.0	98949	PASS
443	442	15	24	19.8	19552	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/14/2022	BNA_G	BG055601.D
Compound Name	Response	Retention Time
DDT	256347	21.085
DDD	7245	20.626
DDE	528	20.127
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7773	264120	2.94

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111422\
Data File : BG055601.D
Acq On : 14 Nov 2022 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 14 15:59:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

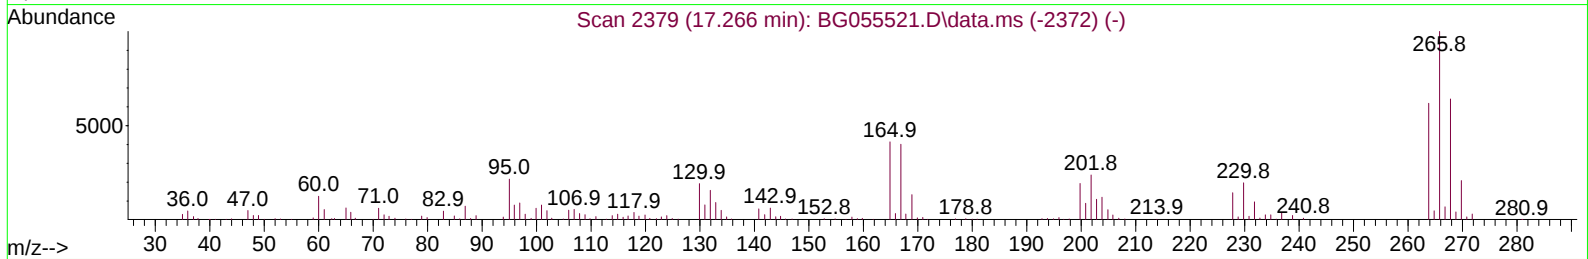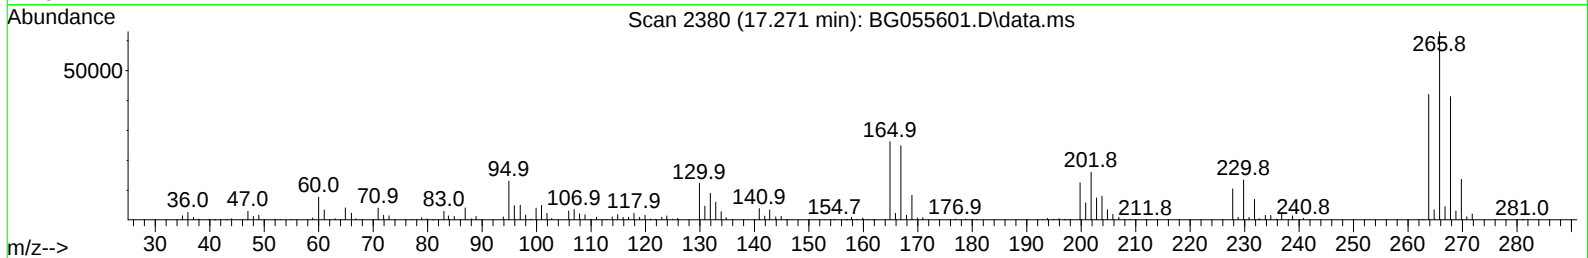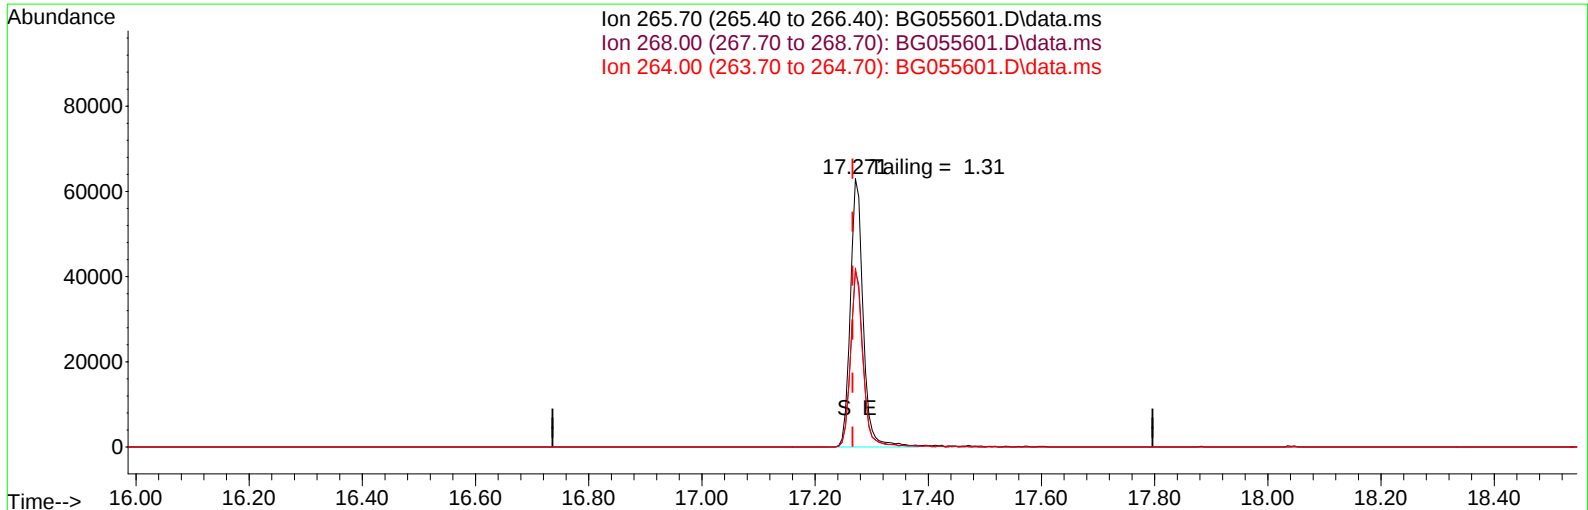

TIC: BG055601.D\data.ms

(70) Pentachlorophenol (C)

17.271min (+ 0.005) 27084.52 ng




response 98801

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	65.63
264.00	61.90	66.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111422\
Data File : BG055601.D
Acq On : 14 Nov 2022 10:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 14 15:59:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

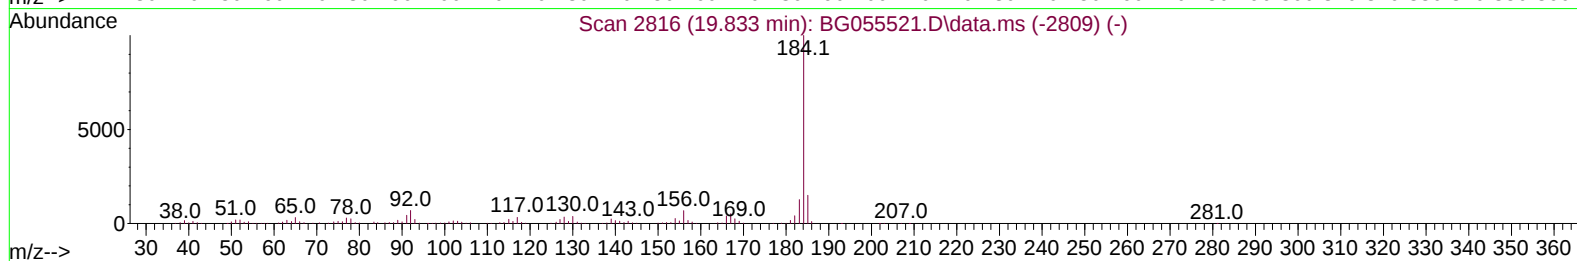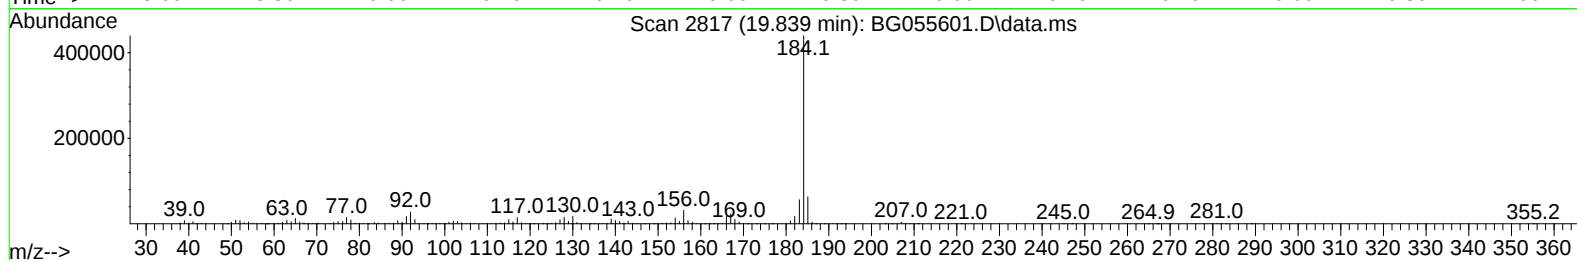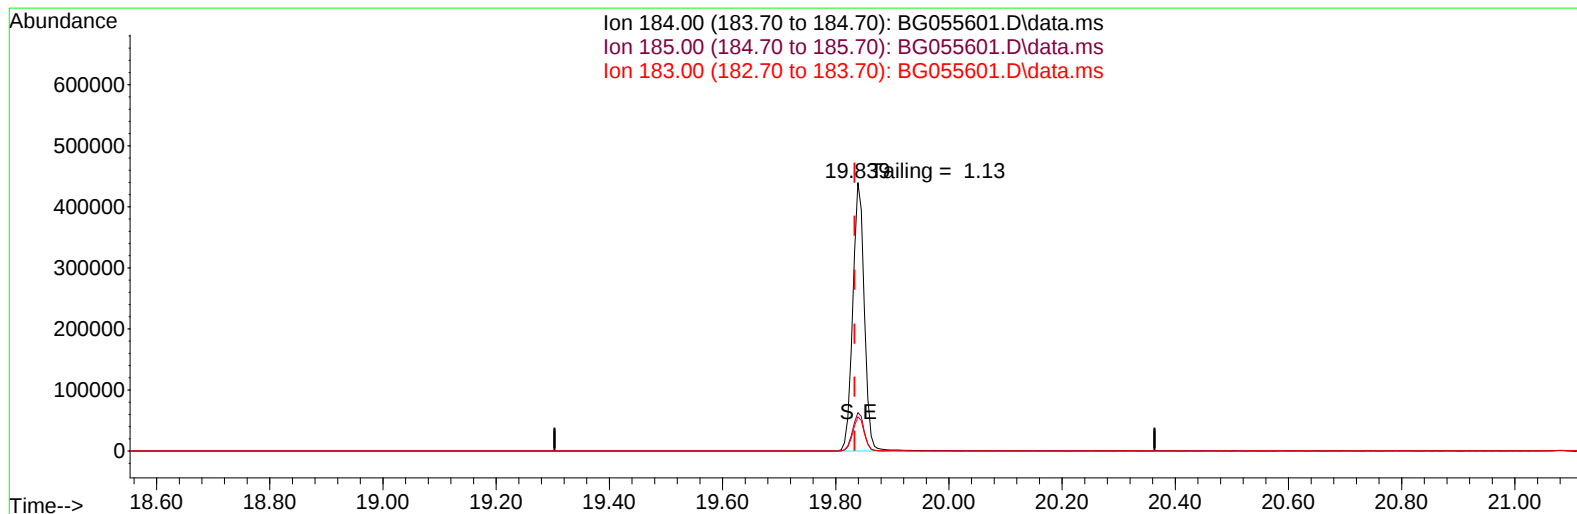

TIC: BG055601.D\data.ms

(77) Benzidine

19.839min (+ 0.006) 210903.62 ng

response 621932

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.31
183.00	12.70	12.76
0.00	0.00	0.00