

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111515\
 Data File : BG019630.D
 Acq On : 16 Nov 2015 1:05
 Operator : UM/NP
 Sample : G4309-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 16 03:15:33 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 03:12:59 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	31210	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	125305	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.79	164	98233	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.53	188	270181	20.00	ng/ul	0.00
78) Chrysene-d12	21.80	240	332941	20.00	ng/ul	0.00
86) Perylene-d12	25.13	264	317460	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.46	96	3608	5.54	ng/uL	0.00
5) Phenol-d5	7.30	99	85410	29.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	59977	33.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	54855	30.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	70628	30.95	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	29650	32.20	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	34010	31.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	68411	28.85	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	73726	30.73	ng/ul	0.00
44) Dimethylphthalate-d6	14.18	166	247317	30.54	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	271352	30.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	36477	28.35	ng/ul	0.00
58) Fluorene-d10	15.78	176	222081	29.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.89	200	42447	24.27	ng/ul	0.00
71) Anthracene-d10	17.63	188	376397	30.56	ng/ul	0.00
79) Pyrene-d10	19.90	212	460445	31.60	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.90	264	497878	31.25	ng/ul	0.00

Target Compounds


						Ovalue
6) Phenol	7.33	94	5442	1.78	ng/ul	97
15) N-Nitroso-di-n-propylamine	8.86	70	2589	1.03	ng/ul#	1
45) Dimethylphthalate	14.23	163	150386	18.16	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111515\
Data File : BG019630.D
Acq On : 16 Nov 2015 1:05
Operator : UM/NP
Sample : G4309-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 16 03:15:33 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 16 03:12:59 2015
Response via : Initial Calibration

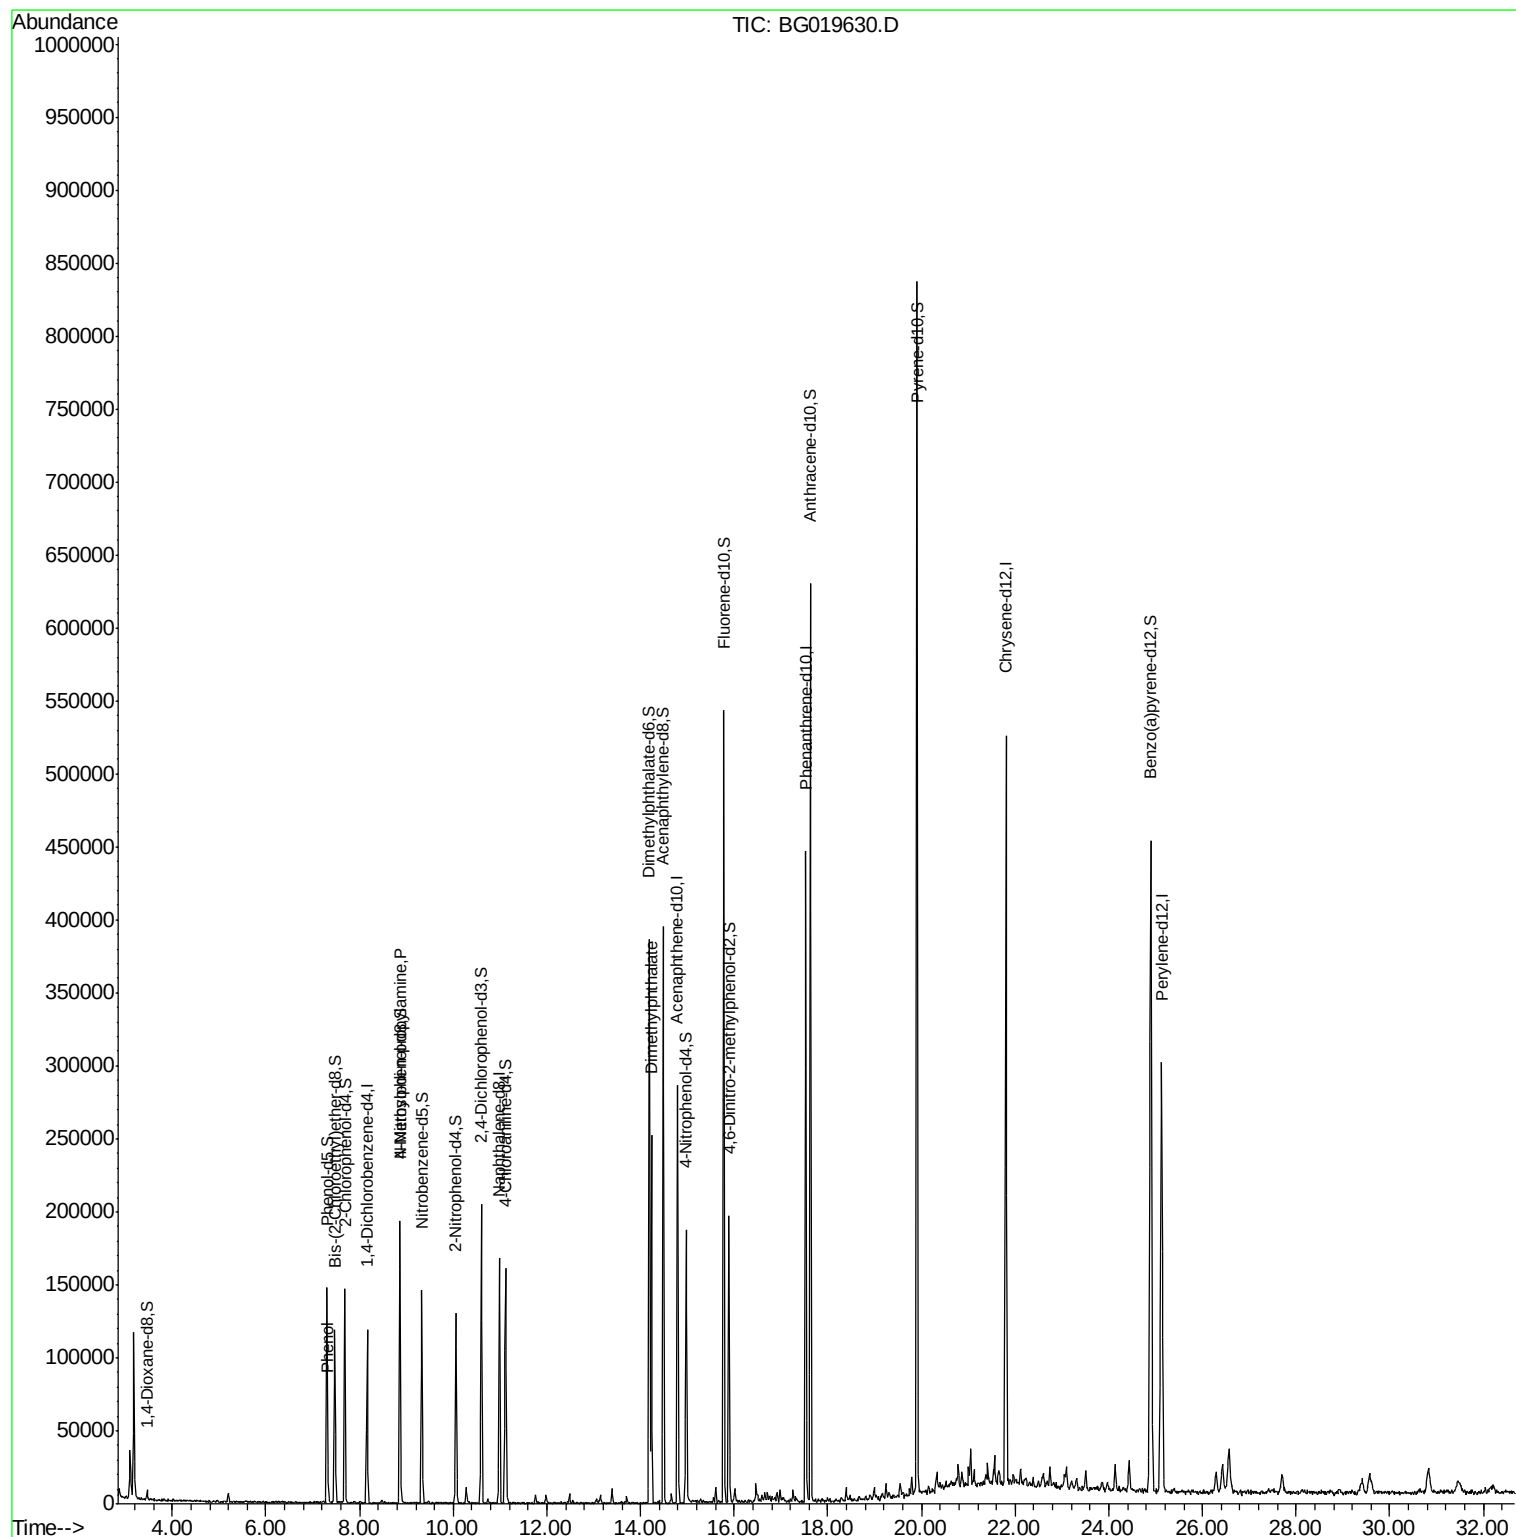

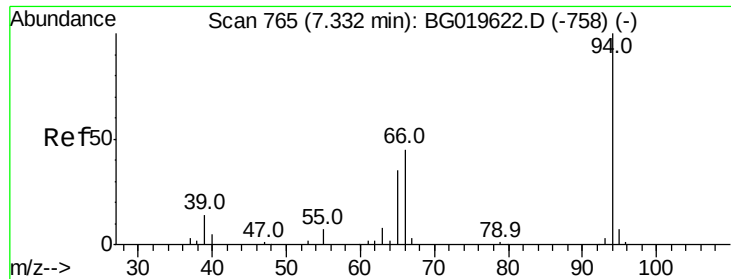

#6

Phenol

Concen: 1.78 ng/ul

RT: 7.33 min Scan# 764

Delta R.T. -0.01 min

Lab File: BG019630.D

Acq: 16 Nov 2015 1:05

Instrument :

BNA_G

ClientSampled :


Tot Ion: 94 Resp: 5442

Ion Ratio Lower Upper




94 100

65 34.7 29.3 43.9

66 54.0 45.0 67.6

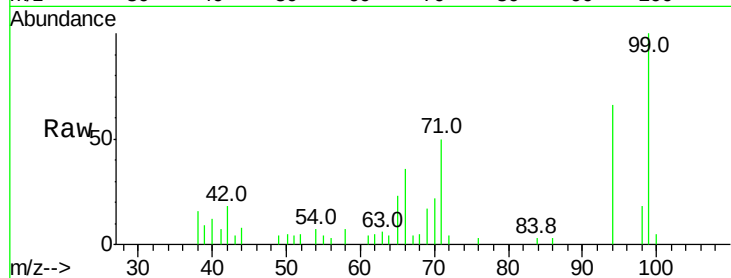

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

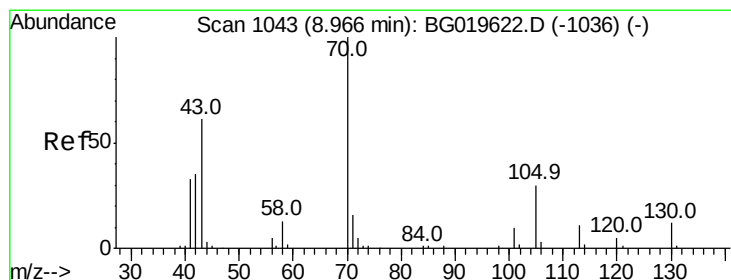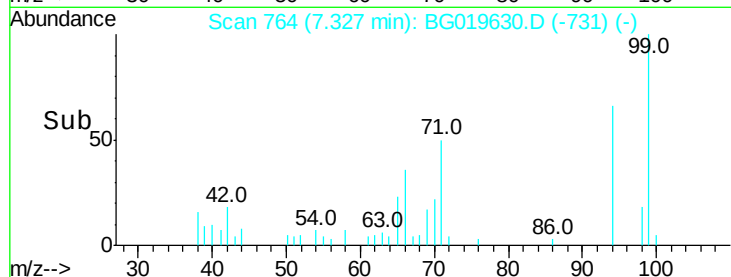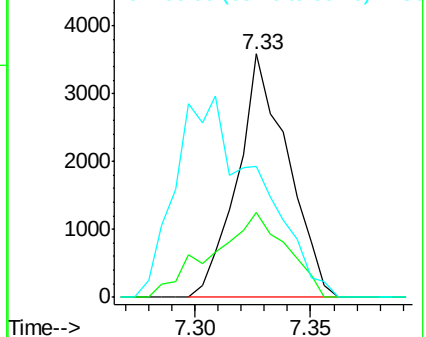

#15

N-Nitroso-di-n-propylamine

Concen: 1.03 ng/ul

RT: 8.86 min Scan# 1025

Delta R.T. -0.11 min

Lab File: BG019630.D

Acq: 16 Nov 2015 1:05

Tgt Ion: 70 Resp: 2589


Ion Ratio Lower Upper

70 100



42 175.6 36.6 55.0#


101 0.0 5.8 8.8#

130 0.0 14.6 22.0#

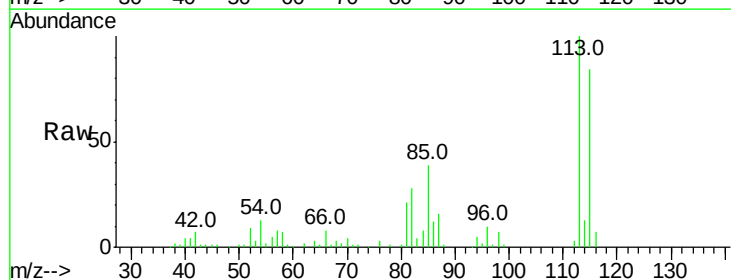

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

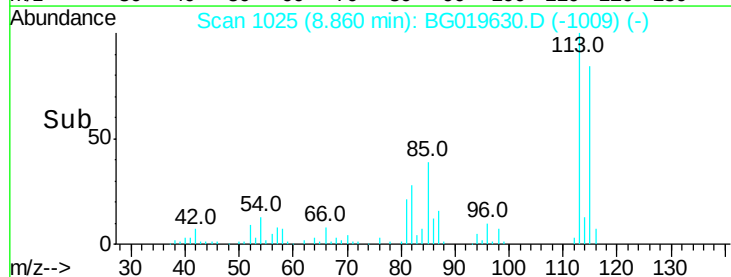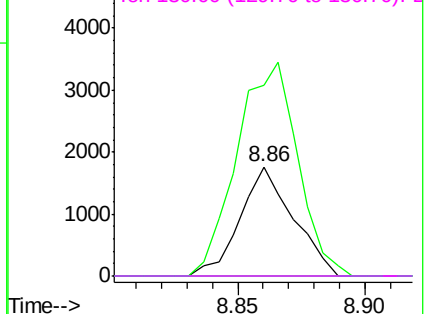

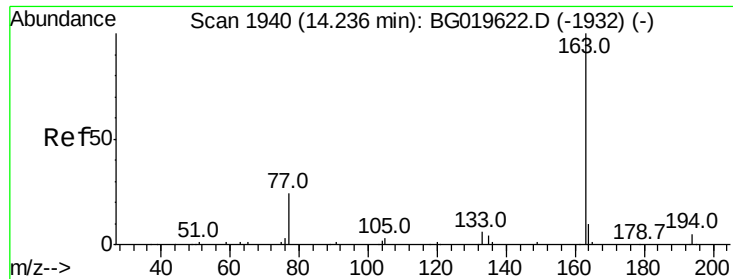

#45

Dimethylphthalate

Concen: 18.16 ng/ul

RT: 14.23 min Scan# 1939

Delta R.T. -0.01 min

Lab File: BG019630.D

Acq: 16 Nov 2015 1:05

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 150386

Ion Ratio Lower Upper

163 100

194 3.9 4.3 6.5#

164 9.9 7.5 11.3

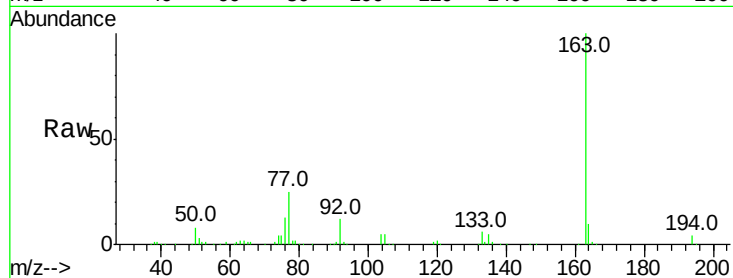

Abundance Ion 163.00 (162.70 to 163.70): E
150000
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

