

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111515\
 Data File : BG019635.D
 Acq On : 16 Nov 2015 4:16
 Operator : UM/NP
 Sample : G4309-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KQ8

Quant Time: Nov 16 06:16:00 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Nov 16 03:12:59 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	31552	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	125632	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.79	164	98940	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.53	188	271370	20.00	ng/ul	0.00
78) Chrysene-d12	21.80	240	331744	20.00	ng/ul	0.00
86) Perylene-d12	25.13	264	317113	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.46	96	2767	4.20	ng/uL	0.00
5) Phenol-d5	7.30	99	69068	23.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	46576	25.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	43214	23.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	52753	22.87	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	23448	25.40	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	25606	23.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	55172	23.20	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	58833	24.46	ng/ul	0.00
44) Dimethylphthalate-d6	14.18	166	200115	24.53	ng/ul	0.00
47) Acenaphthylene-d8	14.49	160	220963	24.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.98	143	30648	23.65	ng/ul	0.00
58) Fluorene-d10	15.77	176	178135	23.60	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.89	200	33802	19.24	ng/ul	0.00
71) Anthracene-d10	17.63	188	305243	24.68	ng/ul	0.00
79) Pyrene-d10	19.90	212	370891	25.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.89	264	394035	24.76	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.23	163	122660	14.70	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111515\
Data File : BG019635.D
Acq On : 16 Nov 2015 4:16
Operator : UM/NP
Sample : G4309-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KQ8

Quant Time: Nov 16 06:16:00 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102815.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Nov 16 03:12:59 2015
Response via : Initial Calibration

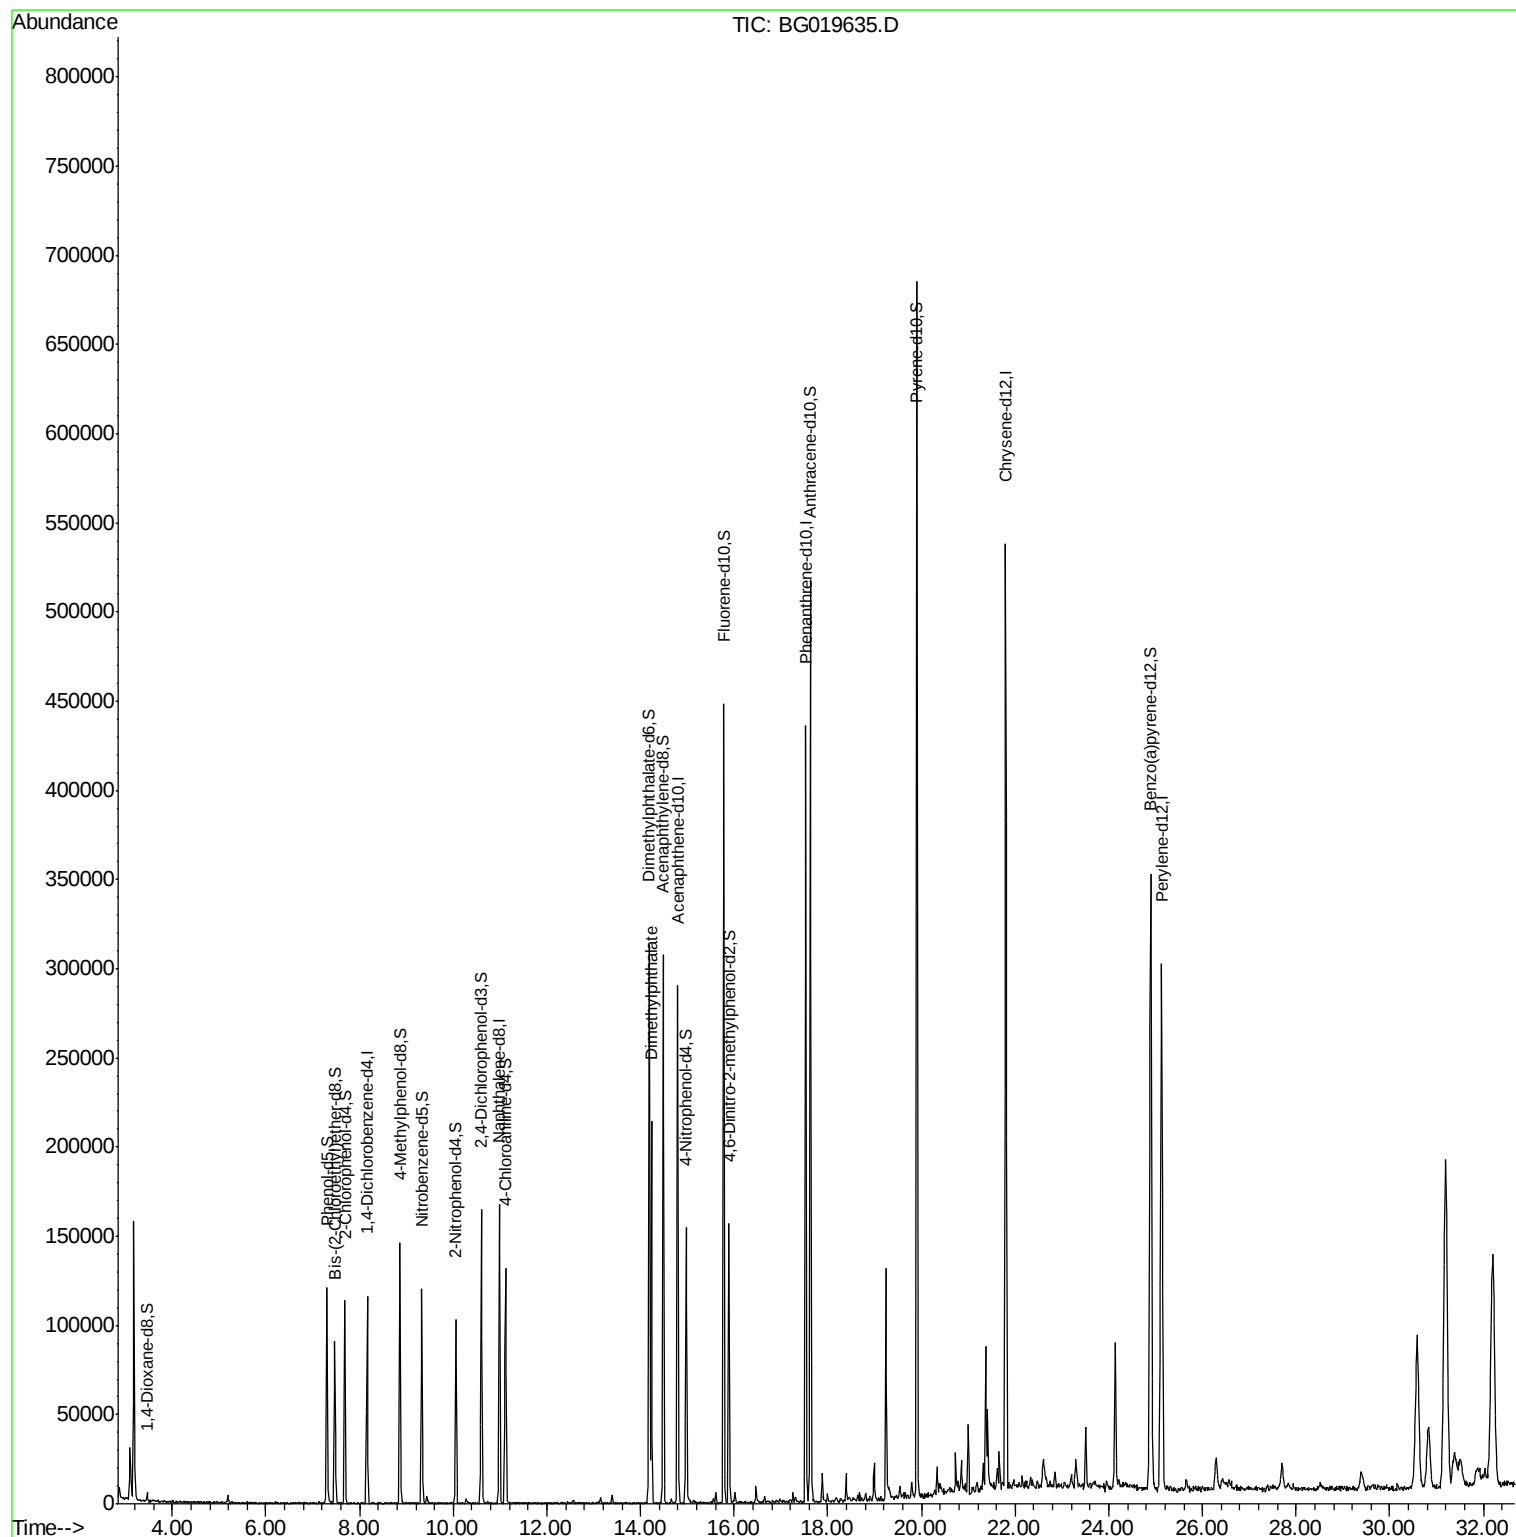

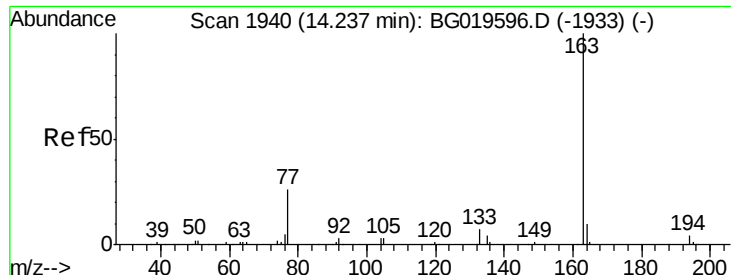

#45

Dimethylphthalate

Concen: 14.70 ng/ul

RT: 14.23 min Scan# 1939

Delta R.T. -0.01 min

Lab File: BG019635.D

Acq: 16 Nov 2015 4:16

Instrument :

BNA_G

ClientSampleId :

D9KQ8


Tgt Ion:163 Resp: 122660

Ion Ratio Lower Upper

163 100

194 5.1 4.3 6.5

164 10.8 7.5 11.3

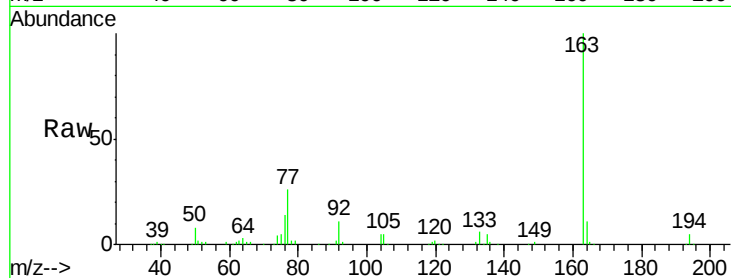

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

