
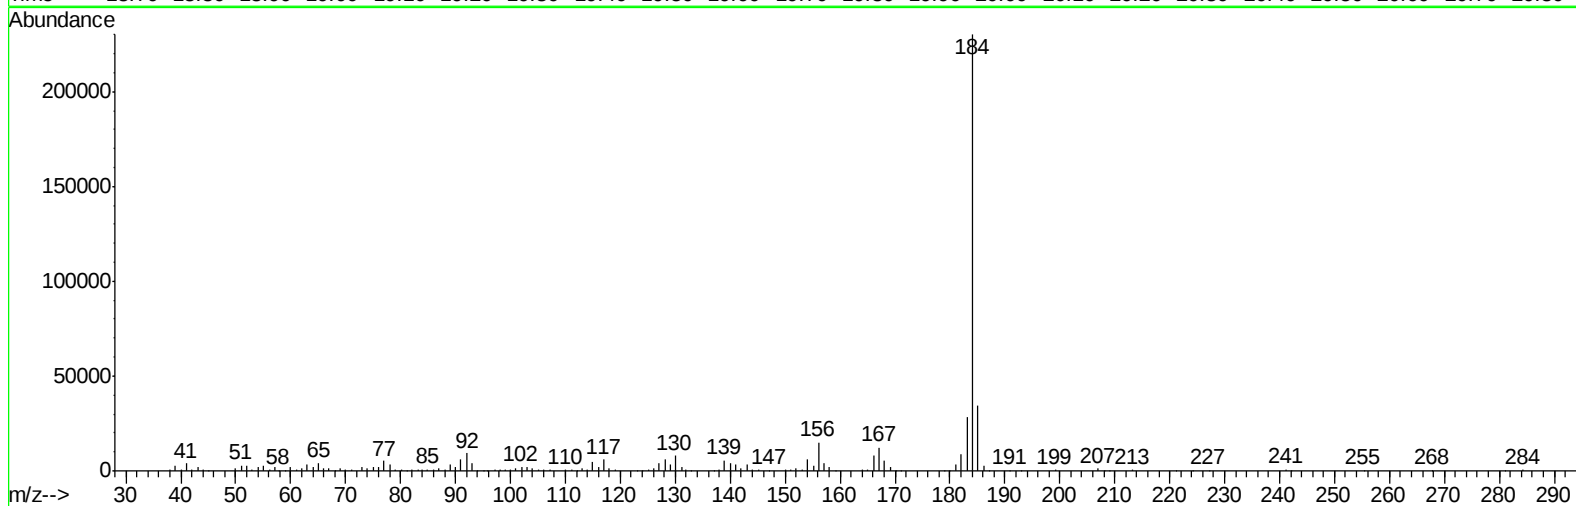


Data Path : Z:\HPCHEM1\BNA G\DATA\BG111517\
Data File : BG031006.D
Acq On : 15 Nov 2017 9:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 08:49:02 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

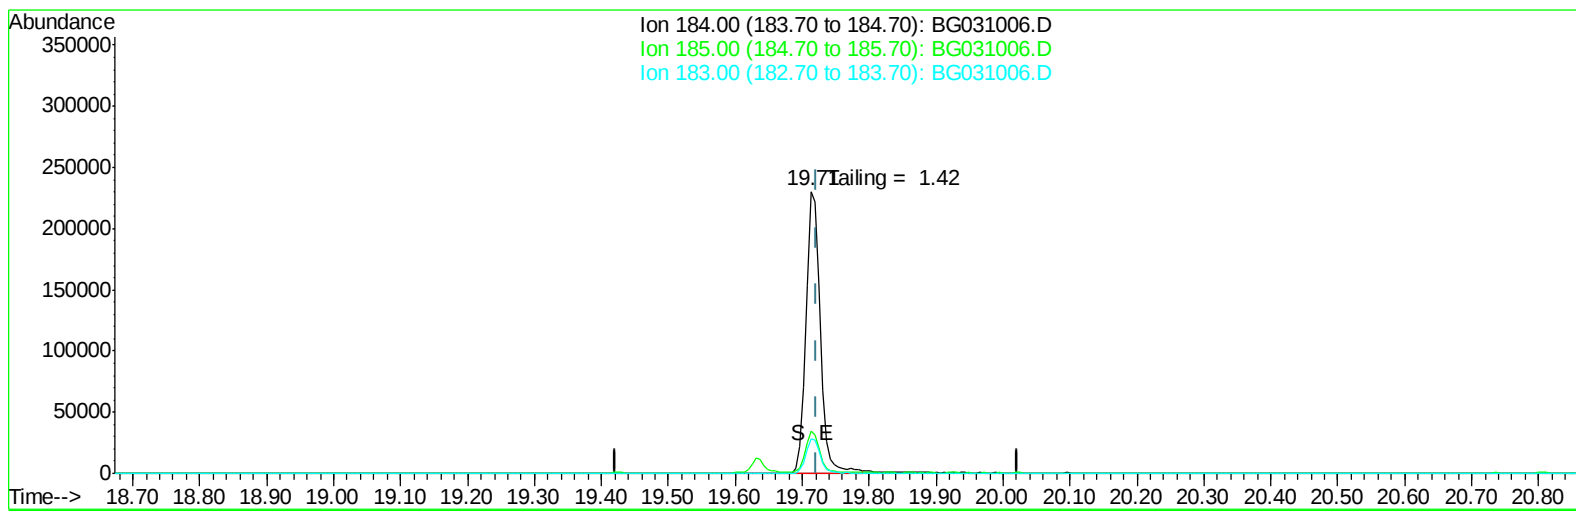

TIC: BG031006.D

(76) Benzidine



19.713min (-0.009) 39436.78ng

response 357235

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.10
183.00	13.30	12.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111517\
Data File : BG031006.D
Acq On : 15 Nov 2017 9:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 08:49:02 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

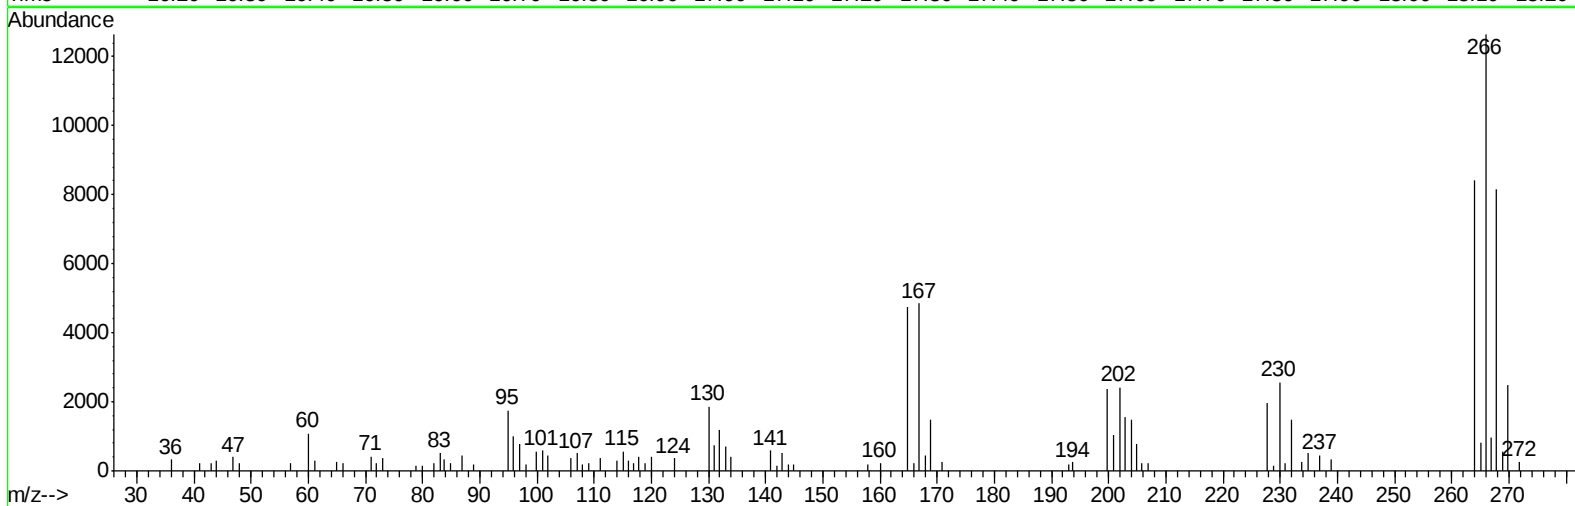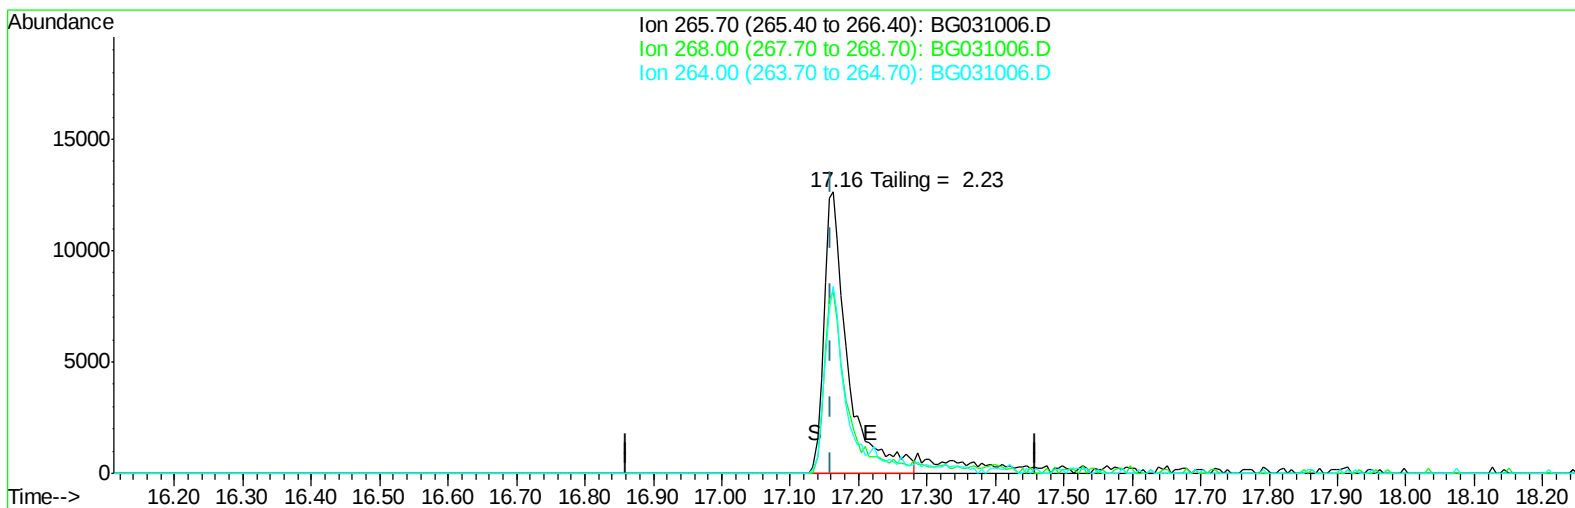

TIC: BG031006.D

(69) Pentachlorophenol (C)

17.163min (+0.003) 34311.40ng

response 29353

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.53
264.00	62.00	66.46
0.00	0.00	0.00