
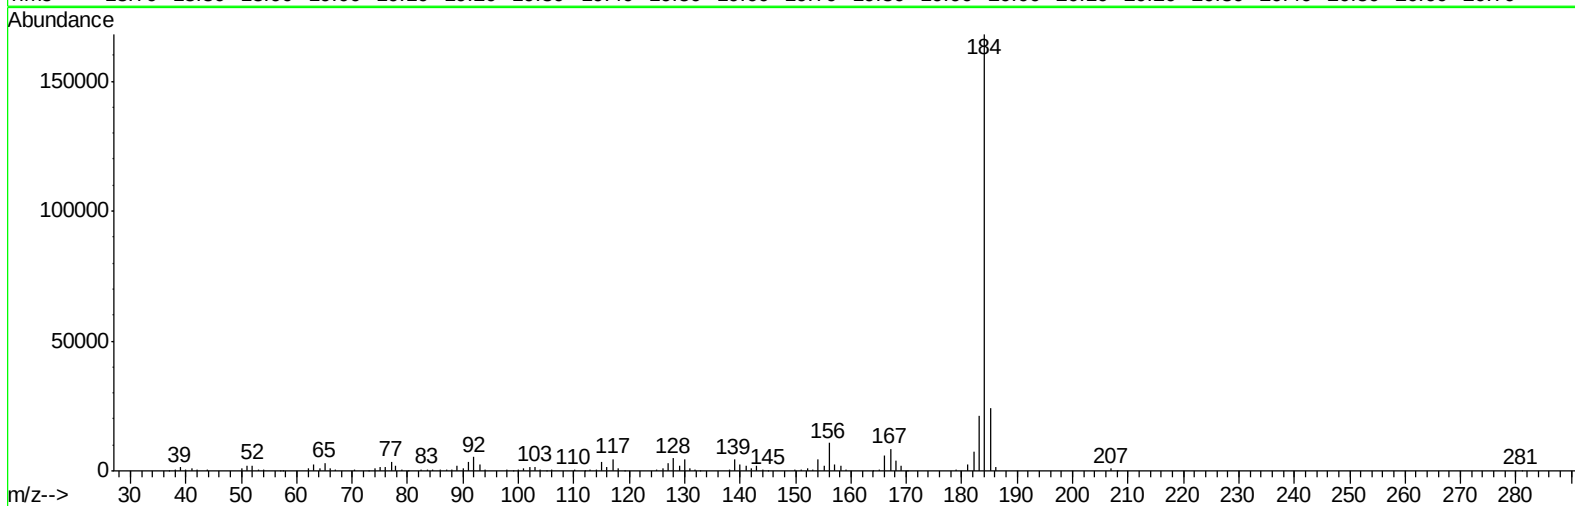


Data Path : Z:\HPCHEM1\BNA G\DATA\BG111517\
Data File : BG031025.D
Acq On : 15 Nov 2017 22:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 08:51:10 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

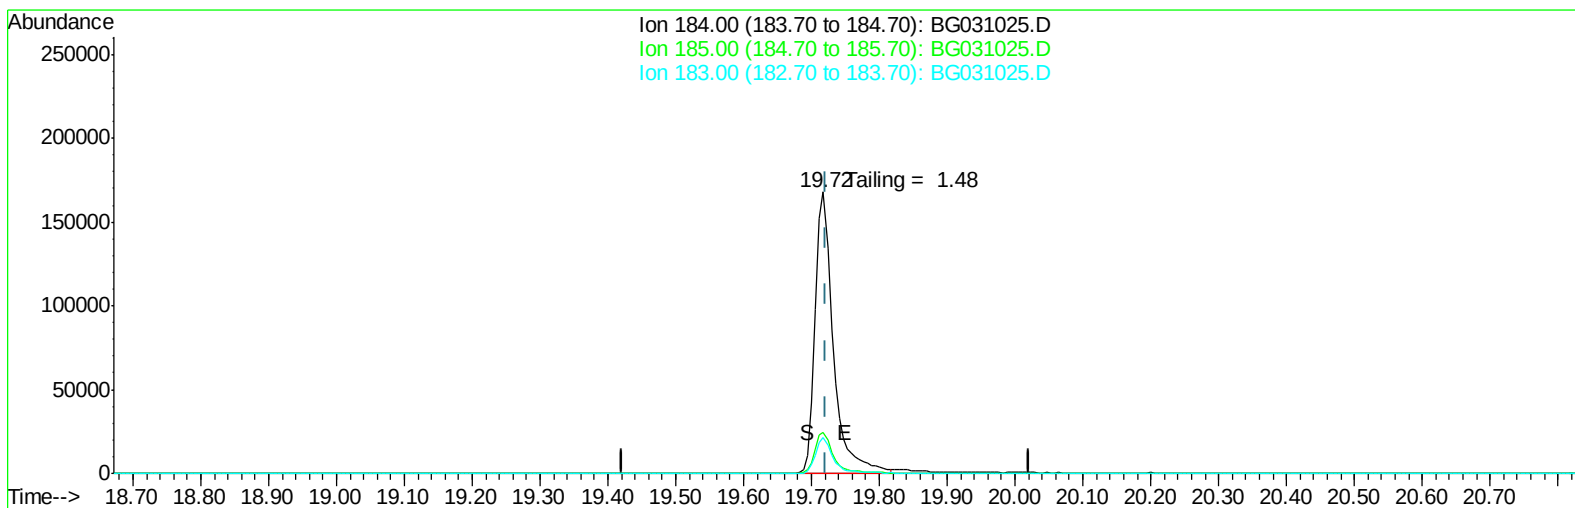

TIC: BG031025.D

(76) Benzidine



19.718min (-0.004) 0.00ng

response 311221

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.44
183.00	13.30	12.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111517\
Data File : BG031025.D
Acq On : 15 Nov 2017 22:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 08:51:10 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG111017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 10 15:38:25 2017
Response via : Initial Calibration

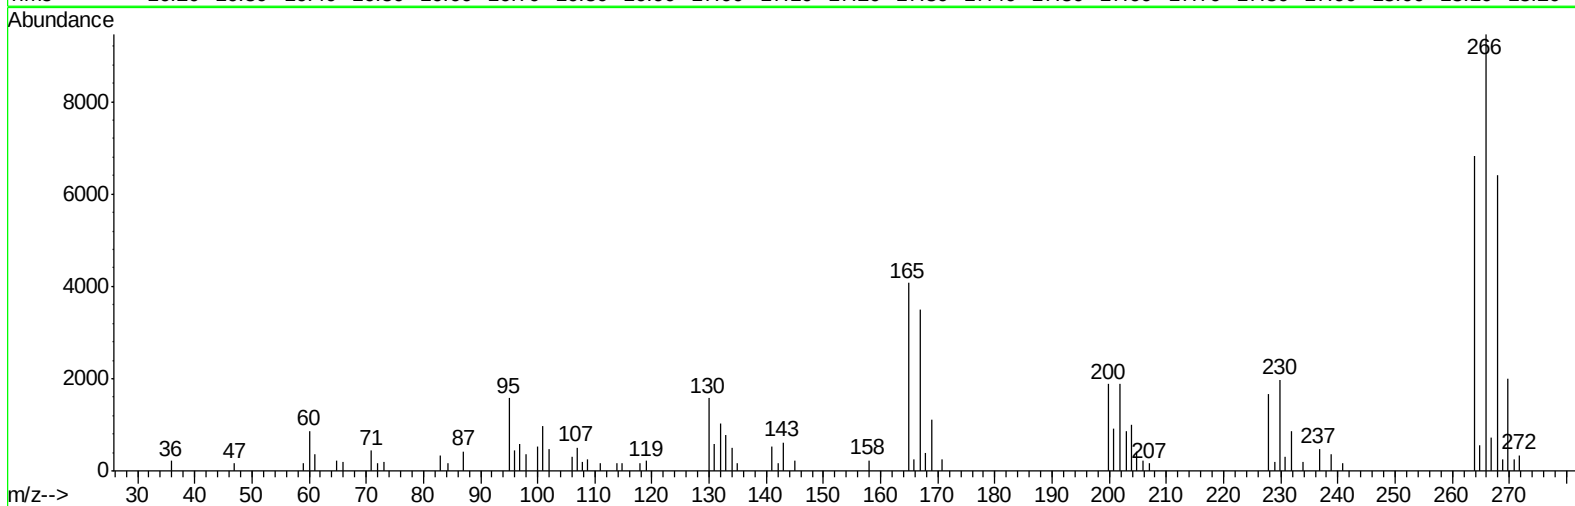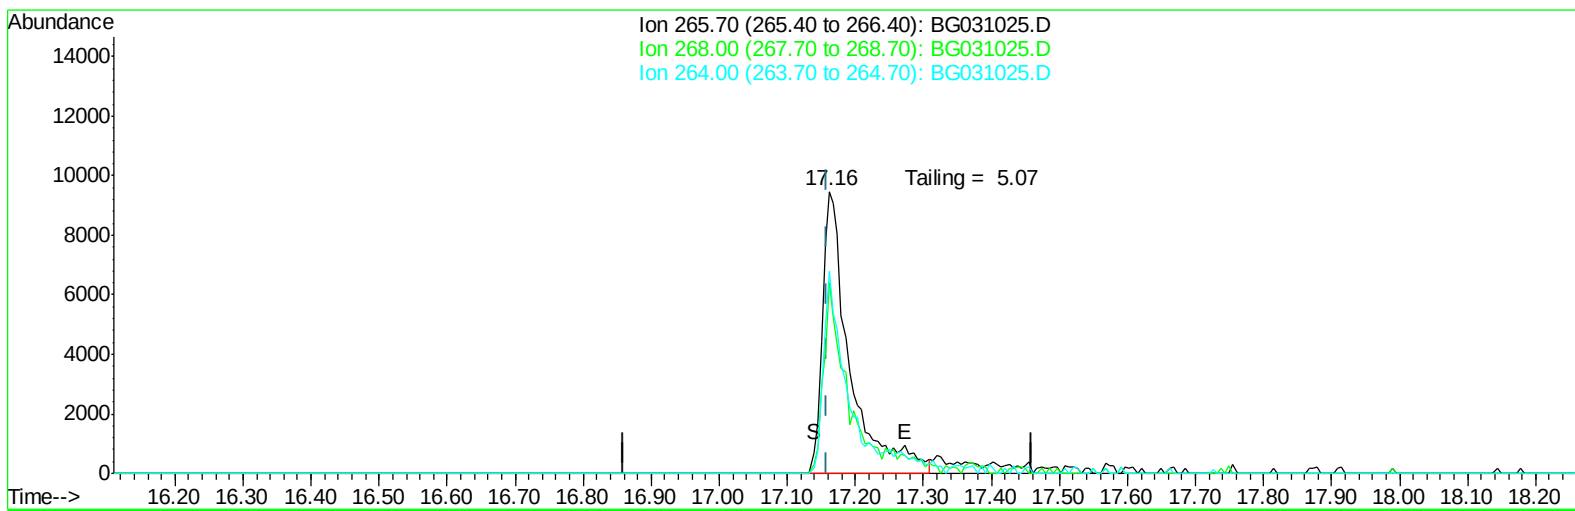

TIC: BG031025.D

(69) Pentachlorophenol (C)

17.162min (+0.002) 0.00ng

response 24854

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.65
264.00	62.00	72.01
0.00	0.00	0.00