


Data Path : Z:\HPCHEM1\BNA_G\Data\BG111517\
 Data File : BG031025.D
 Acq On : 15 Nov 2017 22:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG111017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 10 15:38:25 2017

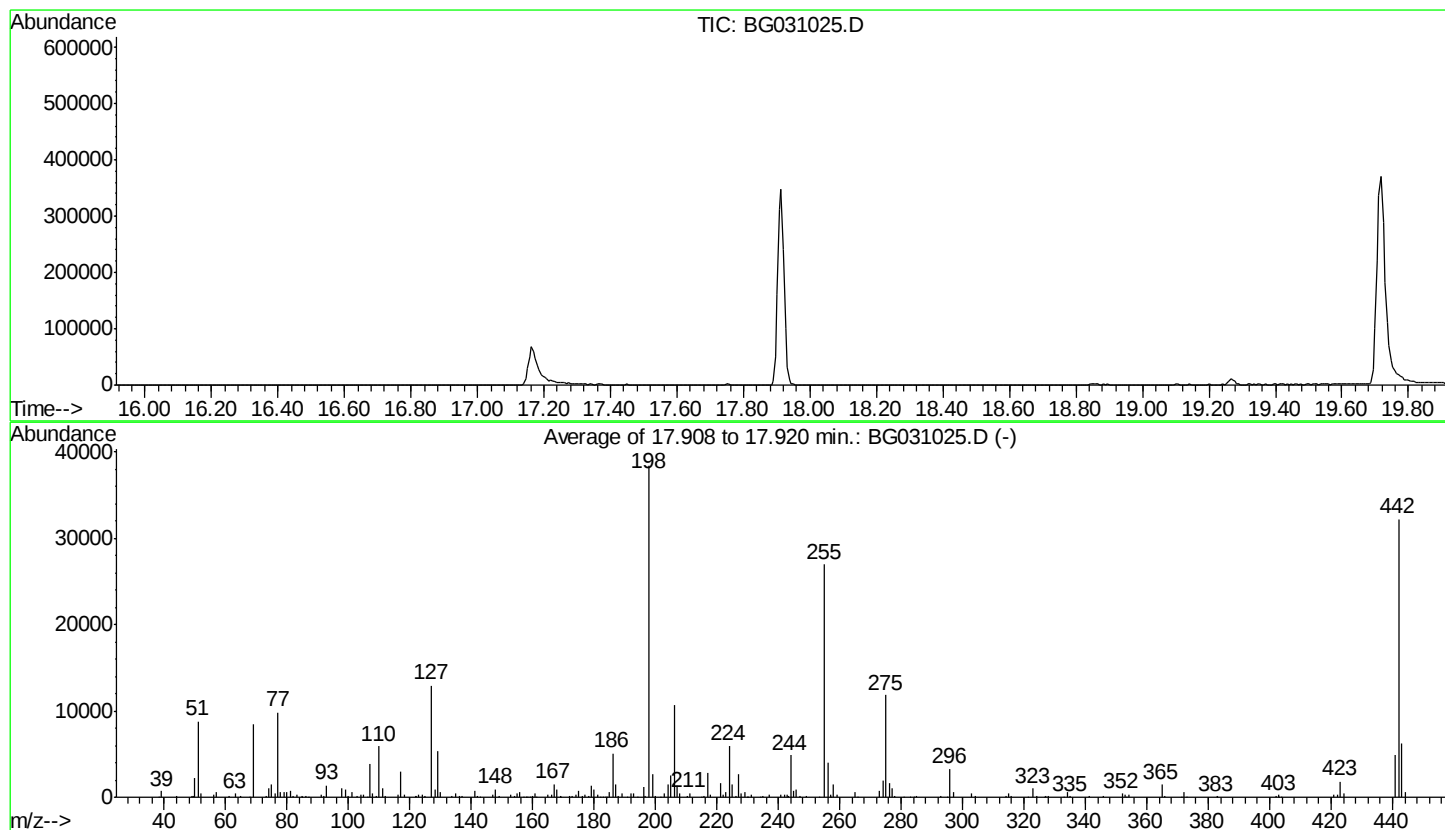

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.8	8763	PASS
68	69	0.00	2	0.9	73	PASS
69	198	0.00	100	22.1	8467	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.7	12933	PASS
197	198	0.00	2	0.3	120	PASS
198	198	100	100	100.0	38389	PASS
199	198	5	9	7.0	2692	PASS
275	198	10	60	30.9	11852	PASS
365	198	1	100	3.8	1476	PASS
441	442	0.01	24	15.2	4900	PASS
442	198	50	100	83.8	32170	PASS
443	442	15	24	19.5	6267	PASS