

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111521\
 Data File : BG051037.D
 Acq On : 15 Nov 2021 11:10
 Operator : CG/JU
 Sample : PB140632BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK632

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051037.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.578	10	15	23	rVB	9438	16196	1.61%	0.165%
2	3.648	25	27	28	rBV	1070	1005	0.10%	0.010%
3	4.006	84	88	103	rBV	115606	212183	21.14%	2.158%
4	4.347	143	146	150	rVB3	2119	2844	0.28%	0.029%
5	4.741	210	213	217	rVB2	1042	1320	0.13%	0.013%
6	5.117	275	277	280	rBV3	750	1031	0.10%	0.010%
7	5.182	283	288	290	rVB3	782	1079	0.11%	0.011%
8	6.750	548	555	558	rBV3	667	1311	0.13%	0.013%
9	7.162	622	625	627	rBV	883	1238	0.12%	0.013%
10	7.367	653	660	672	rBV	137605	242904	24.20%	2.471%
11	7.538	682	689	698	rBV	105609	183235	18.26%	1.864%
12	7.749	717	725	733	rBV	126949	226573	22.57%	2.304%
13	8.225	799	806	816	rVB	111199	191151	19.04%	1.944%
14	8.924	917	925	936	rBV	156458	285781	28.47%	2.907%
15	9.400	998	1006	1015	rBV	129185	230806	23.00%	2.348%
16	10.123	1123	1129	1137	rBV	107494	194416	19.37%	1.977%
17	10.663	1215	1221	1231	rBV	143020	270035	26.90%	2.747%
18	11.051	1279	1287	1295	rBV	156937	285782	28.47%	2.907%
19	11.186	1301	1310	1321	rBV	152087	299991	29.89%	3.051%
20	11.627	1382	1385	1388	rVB	857	1043	0.10%	0.011%
21	12.626	1551	1555	1559	rBV3	1900	2891	0.29%	0.029%
22	14.242	1824	1830	1841	rVB	312887	474530	47.28%	4.826%
23	14.547	1875	1882	1890	rBV	336068	543422	54.14%	5.527%
24	14.853	1927	1934	1941	rBV	256858	409068	40.76%	4.161%
25	15.041	1960	1966	1979	rBV	122187	233424	23.26%	2.374%
26	15.140	1982	1983	1986	rVB2	2094	1153	0.11%	0.012%
27	15.840	2094	2102	2111	rBV	436640	683948	68.14%	6.956%
28	15.957	2116	2122	2136	rBV	125500	200249	19.95%	2.037%
29	16.075	2139	2142	2147	rVB3	1301	1994	0.20%	0.020%
30	16.415	2195	2200	2203	rBV2	644	1034	0.10%	0.011%
31	16.885	2274	2280	2284	rBV2	554	1247	0.12%	0.013%
32	17.379	2361	2364	2370	rBV3	1015	1709	0.17%	0.017%
33	17.596	2394	2401	2408	rBV	348924	537719	53.57%	5.469%
34	17.696	2411	2418	2428	rVV	519727	807490	80.45%	8.213%
35	17.984	2465	2467	2471	rBV3	898	1113	0.11%	0.011%
36	18.460	2542	2548	2551	rBV3	921	1376	0.14%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111521\
 Data File : BG051037.D
 Acq On : 15 Nov 2021 11:10
 Operator : CG/JU
 Sample : PB140632BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK632

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
 Title : SVOA CALIBRATION

37	18.924	2625	2627	2630	rBV2	975	1114	0.11%	0.011%
38	19.242	2678	2681	2682	rBV3	1192	1213	0.12%	0.012%
39	19.336	2695	2697	2702	rVB4	1142	1101	0.11%	0.011%
40	19.406	2707	2709	2711	rVB2	1536	1121	0.11%	0.011%
41	19.535	2728	2731	2737	rBV5	7280	9490	0.95%	0.097%
42	19.612	2739	2744	2747	rBV2	7214	10680	1.06%	0.109%
43	19.976	2799	2806	2816	rBV	674664	1003722	100.00%	10.209%
44	20.375	2872	2874	2875	rBV2	1862	1290	0.13%	0.013%
45	20.558	2903	2905	2906	rVB2	2510	1077	0.11%	0.011%
46	21.897	3126	3133	3144	rVB	329001	578328	57.62%	5.882%
47	23.413	3388	3391	3398	rVB5	16249	27862	2.78%	0.283%
48	23.936	3478	3480	3481	rBV	4548	2215	0.22%	0.023%
49	24.259	3532	3535	3544	rVB5	21619	43162	4.30%	0.439%
50	25.064	3662	3672	3685	rVB2	308194	893741	89.04%	9.090%
51	25.299	3701	3712	3725	rVB3	189045	641449	63.91%	6.524%
52	26.468	3905	3911	3918	rVB9	21076	60375	6.02%	0.614%
53	26.756	3958	3960	3961	rBV	4179	1674	0.17%	0.017%




Sum of corrected areas: 9831905

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111521\
Data File : BG051037.D
Acq On : 15 Nov 2021 11:10
Operator : CG/JU
Sample : PB140632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

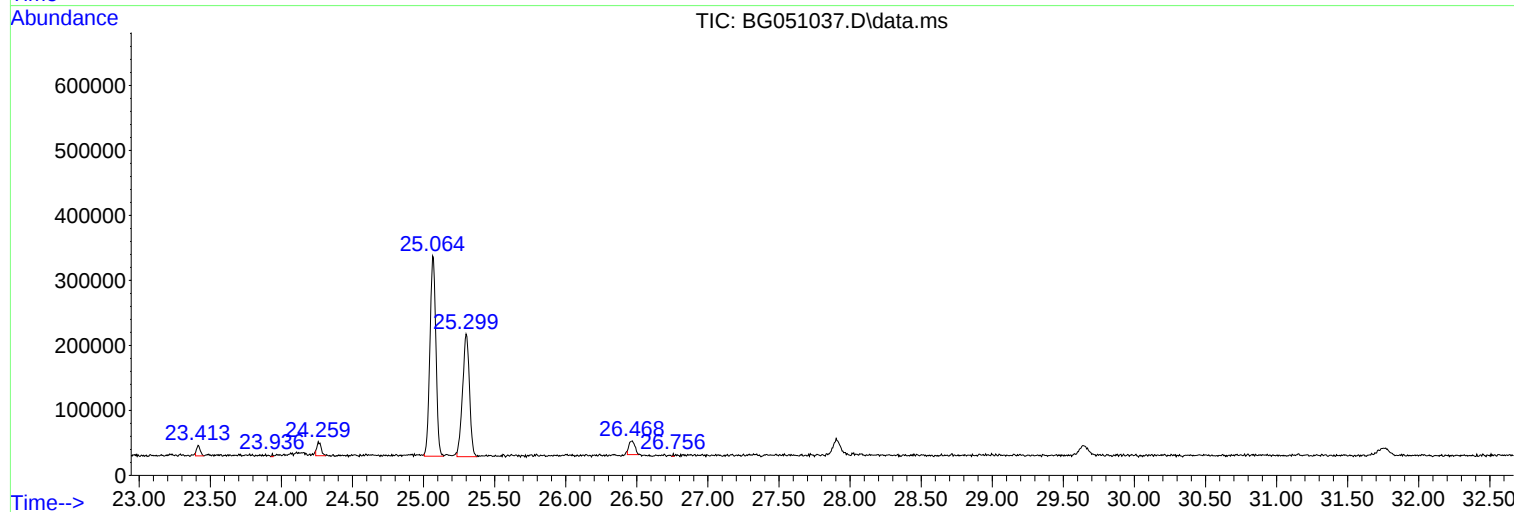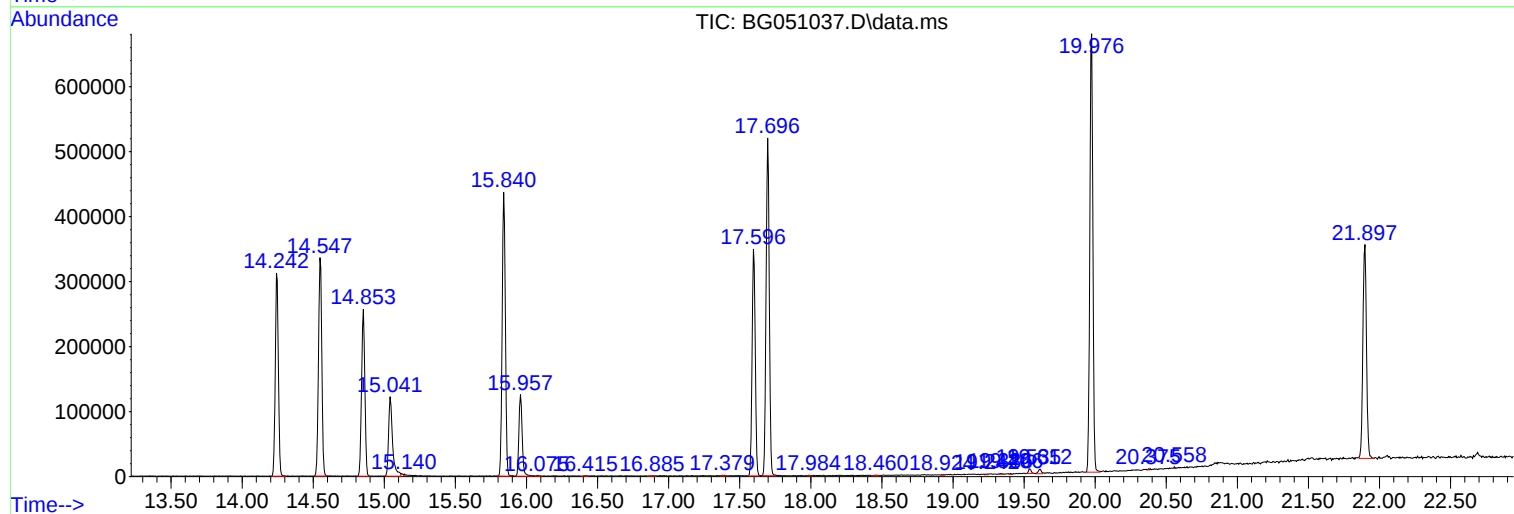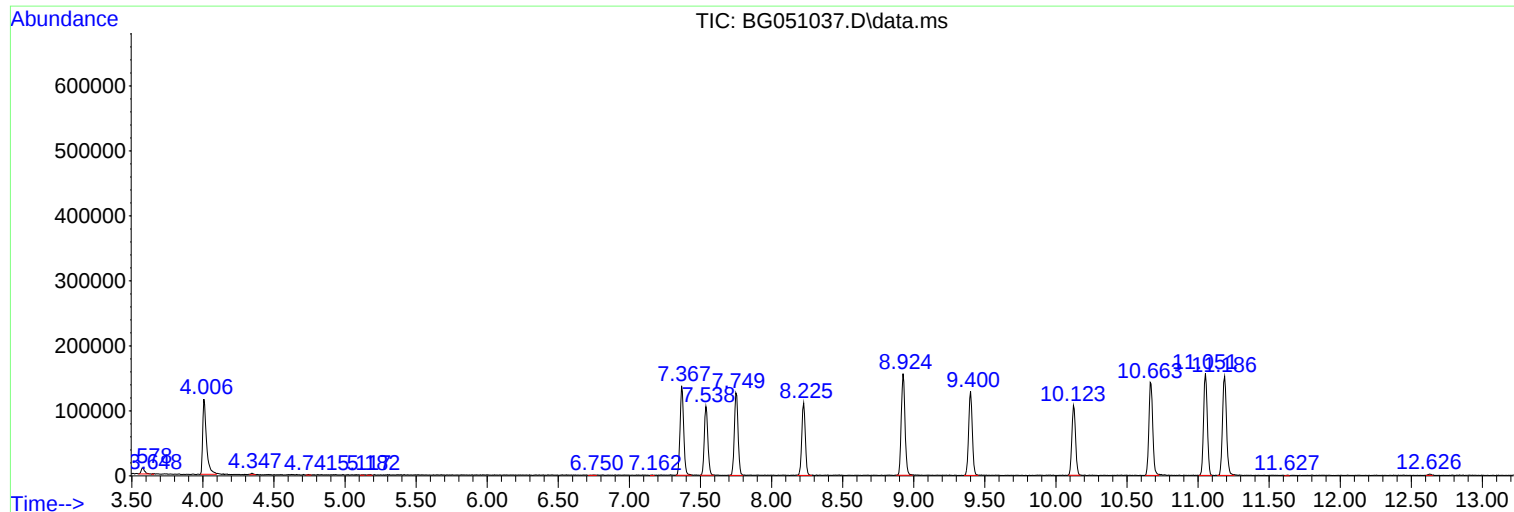

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111521\
Data File : BG051037.D
Acq On : 15 Nov 2021 11:10
Operator : CG/JU
Sample : PB140632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111521\
Data File : BG051037.D
Acq On : 15 Nov 2021 11:10
Operator : CG/JU
Sample : PB140632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG110321.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
