
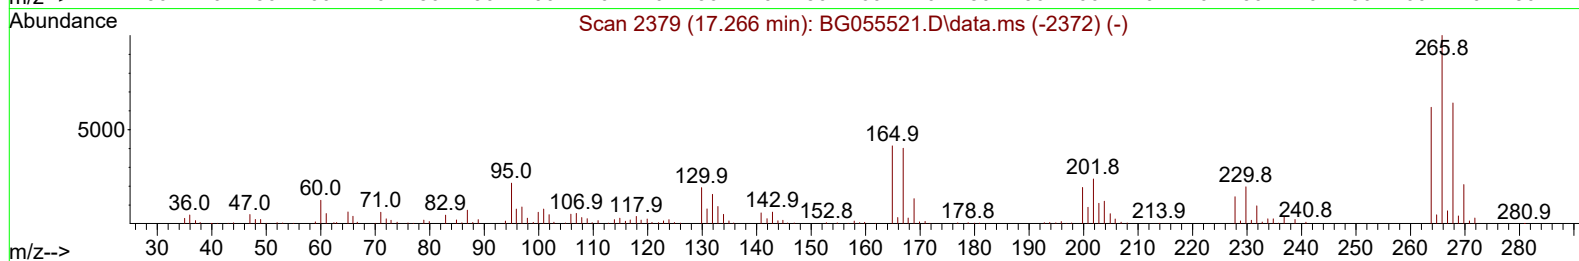
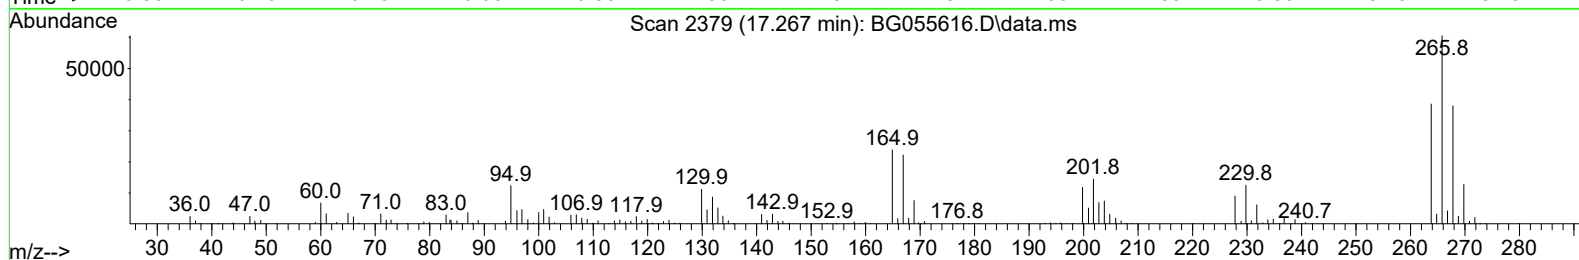


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111522\
Data File : BG055616.D
Acq On : 15 Nov 2022 9:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 04:11:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:36:26 2022
Response via : Initial Calibration

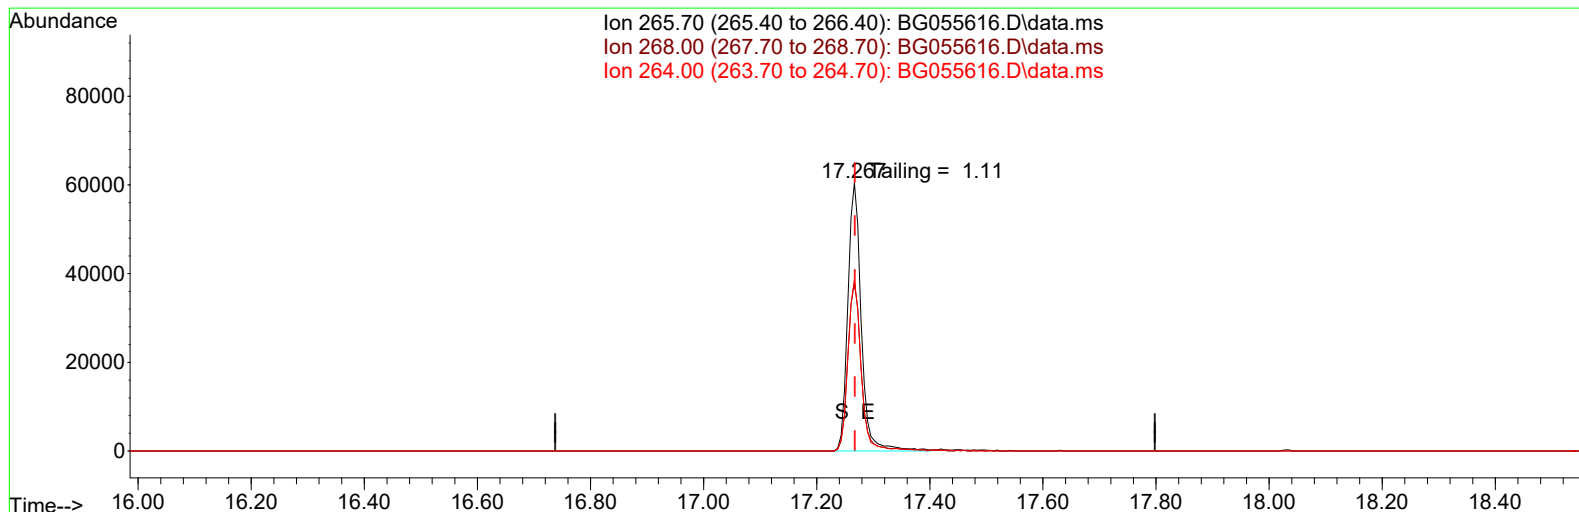

TIC: BG055616.D\data.ms

(70) Pentachlorophenol (C)




17.267min (-0.001) 24986.24 ng

response 100112

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	62.80
264.00	61.90	63.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111522\
Data File : BG055616.D
Acq On : 15 Nov 2022 9:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 04:11:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:36:26 2022
Response via : Initial Calibration

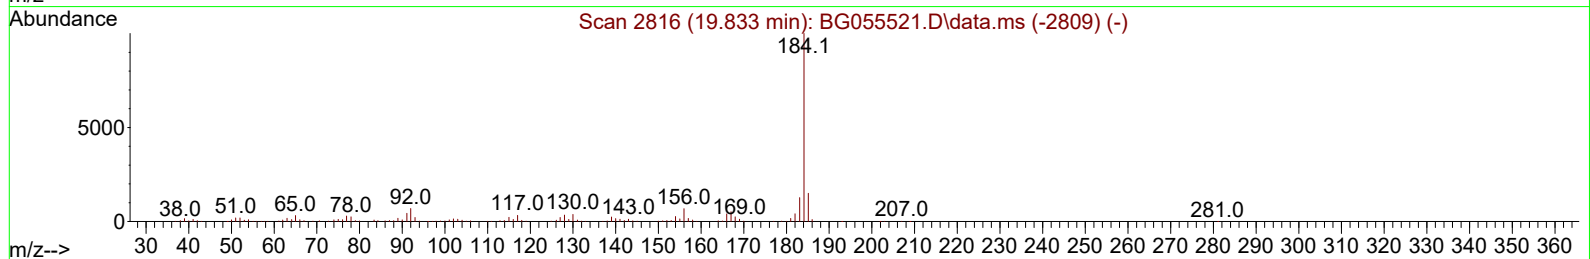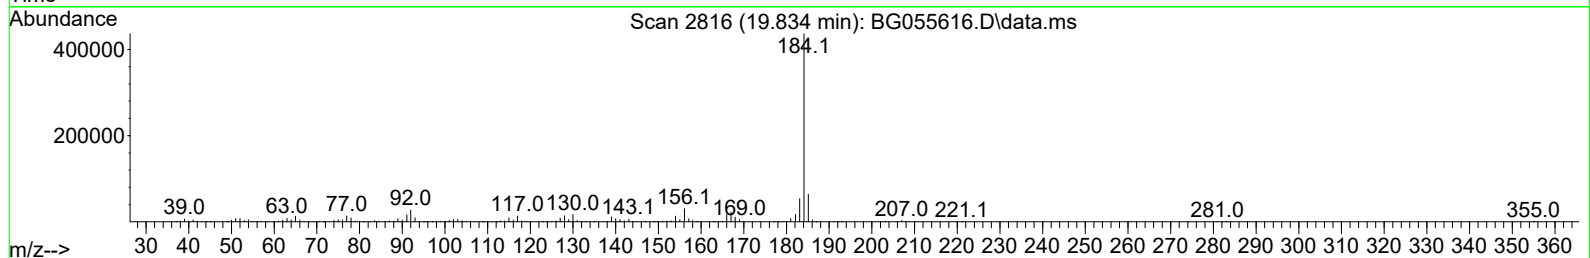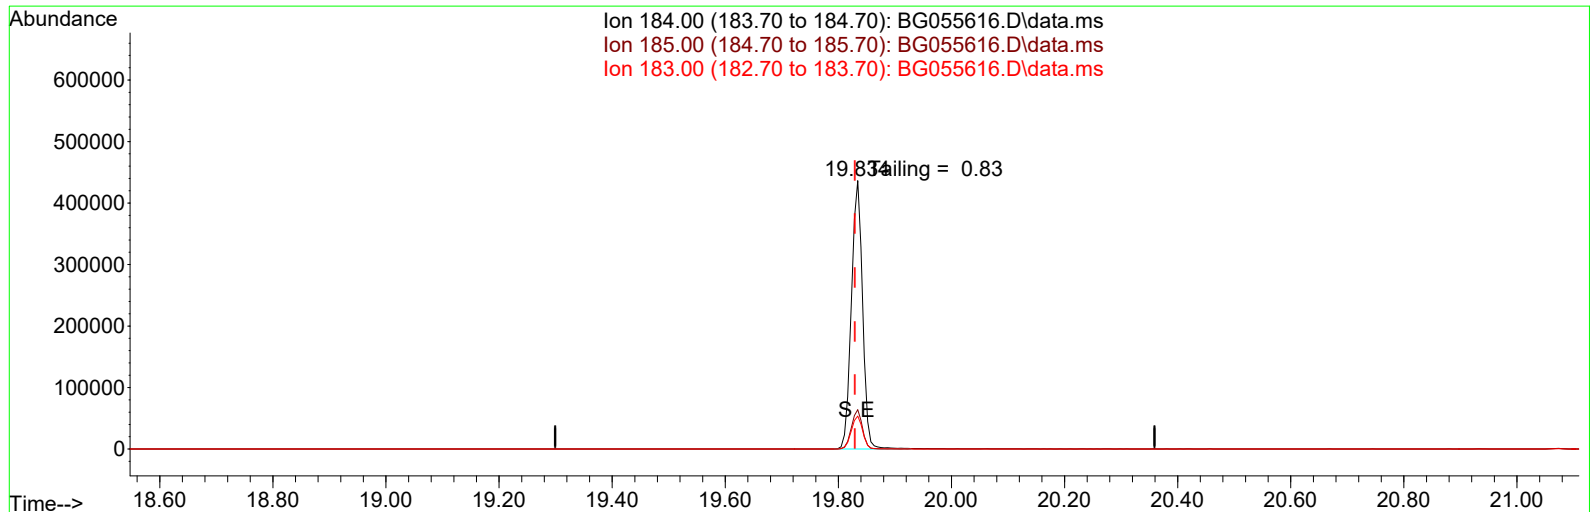

TIC: BG055616.D\data.ms

(77) Benzidine**19.834min (+ 0.005) 114381.45 ng****response 603424**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.66
183.00	12.70	12.32
0.00	0.00	0.00