
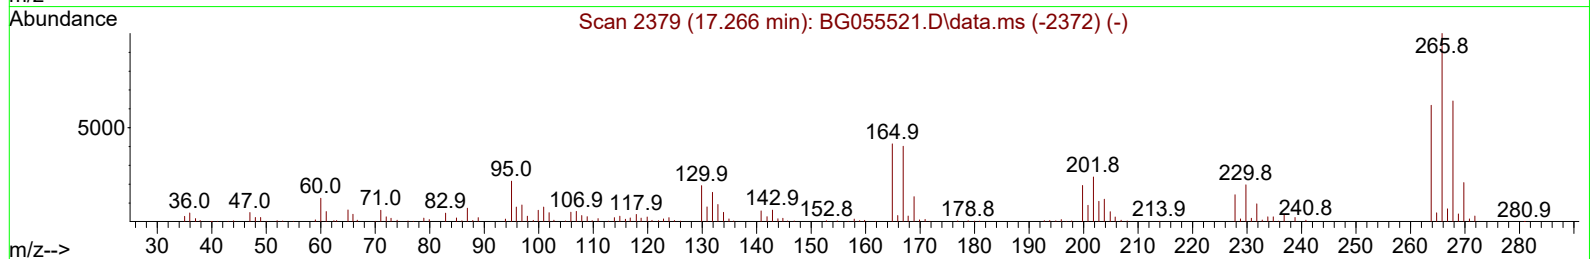
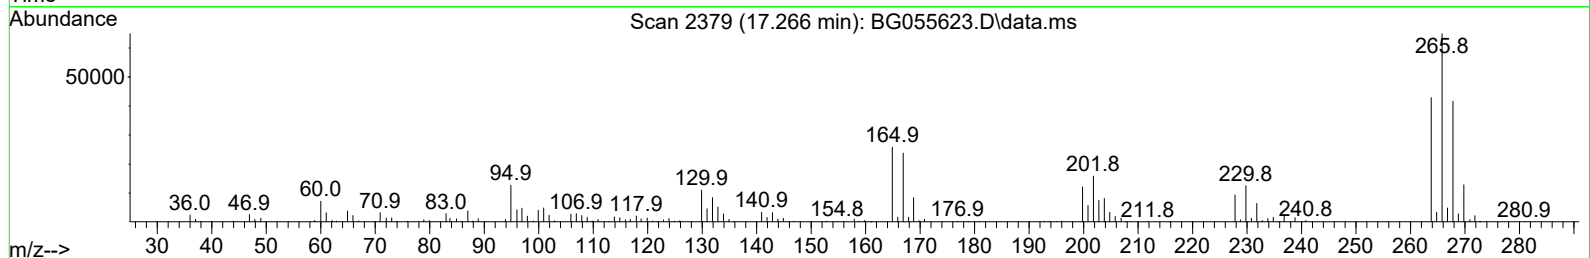


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111522\  
Data File : BG055623.D  
Acq On : 15 Nov 2022 15:34  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 16:09:06 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG110922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 10 03:39:46 2022  
Response via : Initial Calibration

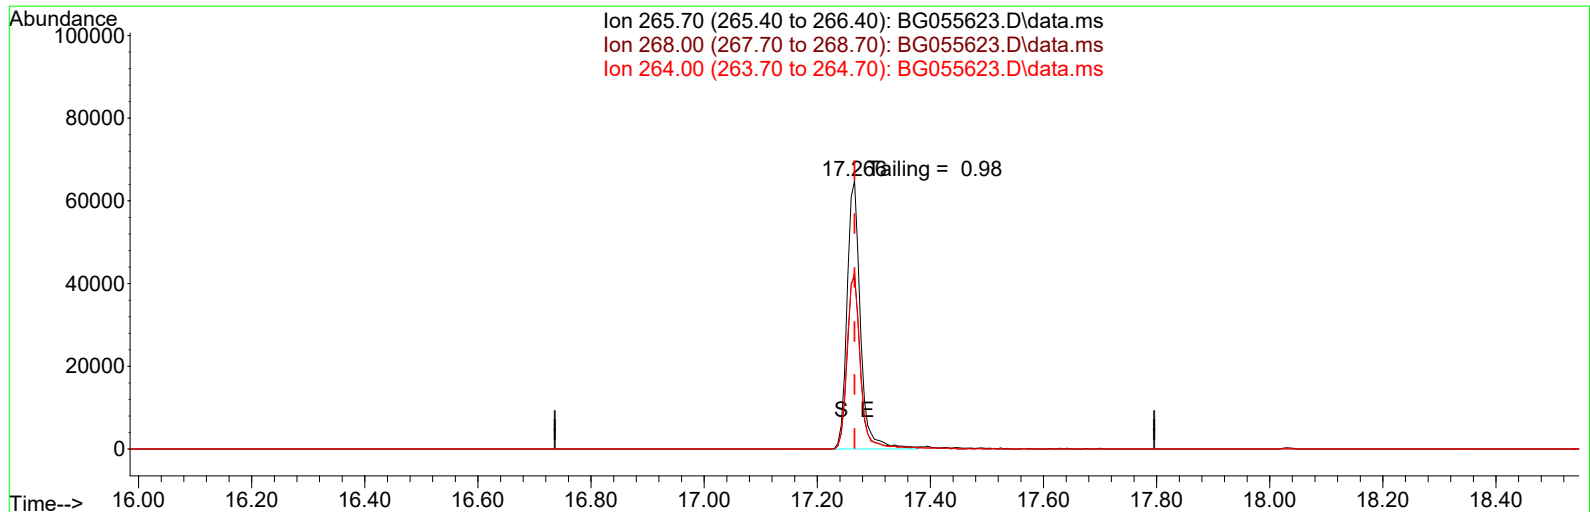

TIC: BG055623.D\data.ms

**(70) Pentachlorophenol (C)**




17.266min (-0.000) 35102.62 ng

response 106825

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.20  | 64.14  |
| 264.00 | 61.90  | 66.10  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111522\  
Data File : BG055623.D  
Acq On : 15 Nov 2022 15:34  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 16:09:06 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG110922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 10 03:39:46 2022  
Response via : Initial Calibration

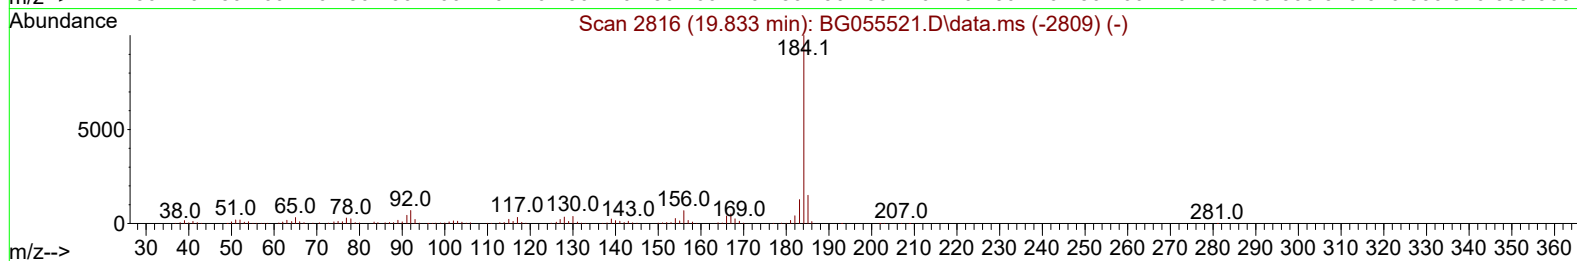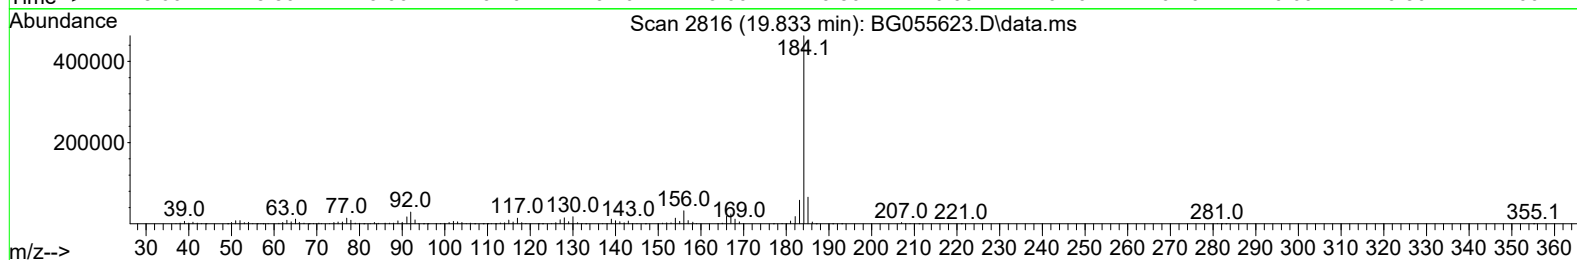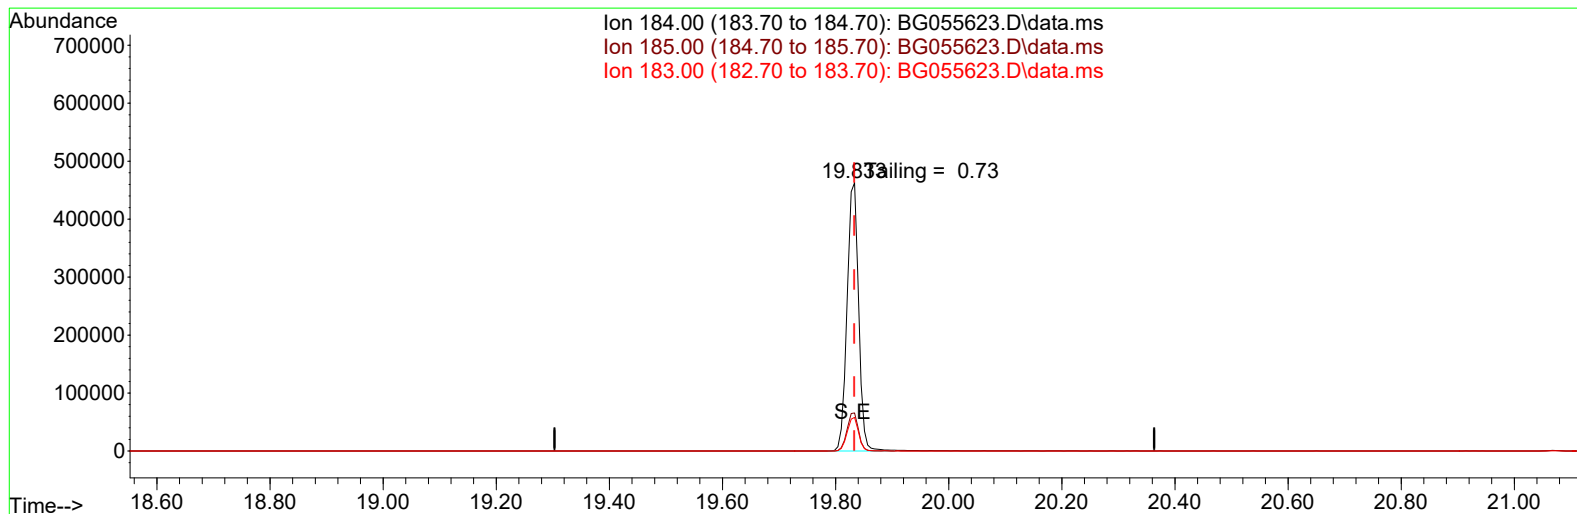

TIC: BG055623.D\data.ms

**(77) Benzidine****19.833min (+ 0.000) 399521.94 ng****response 659330**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.19  |
| 183.00 | 12.70  | 12.55  |
| 0.00   | 0.00   | 0.00   |