


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111522\  
 Data File : BG055616.D  
 Acq On : 15 Nov 2022 9:48  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG110922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Nov 16 01:36:26 2022

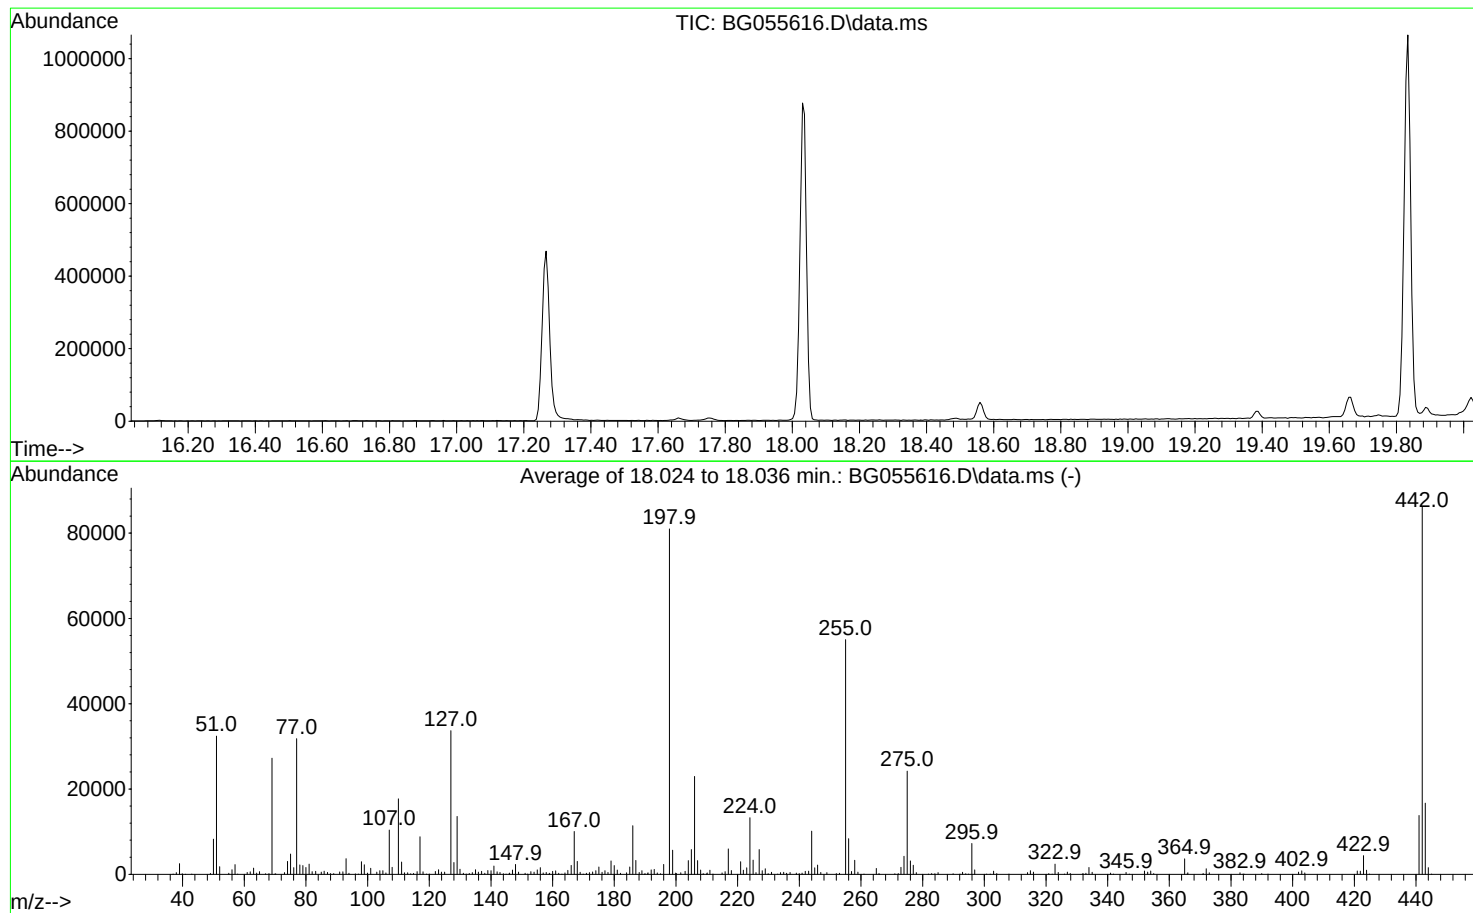




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.0         | 32387      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.6          | 162        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.6         | 27221      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 131        | PASS                |
| 127            | 198             | 10              | 80              | 41.6         | 33667      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 80992      | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 5664       | PASS                |
| 275            | 198             | 10              | 60              | 29.9         | 24178      | PASS                |
| 365            | 198             | 1               | 100             | 4.5          | 3630       | PASS                |
| 441            | 198             | 0.01            | 100             | 17.0         | 13790      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 86267      | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 16686      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111522\  
Data File : BG055616.D  
Acq On : 15 Nov 2022 9:48  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Nov 16 04:11:36 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG110922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 16 01:36:26 2022  
Response via : Initial Calibration

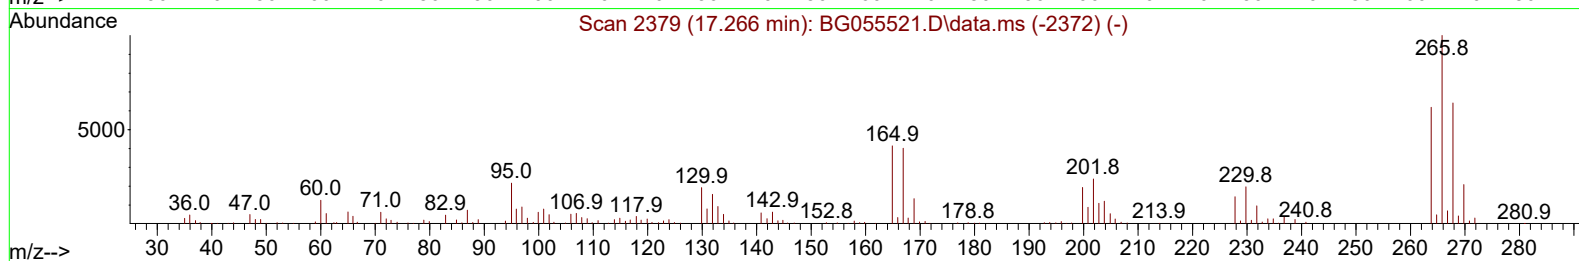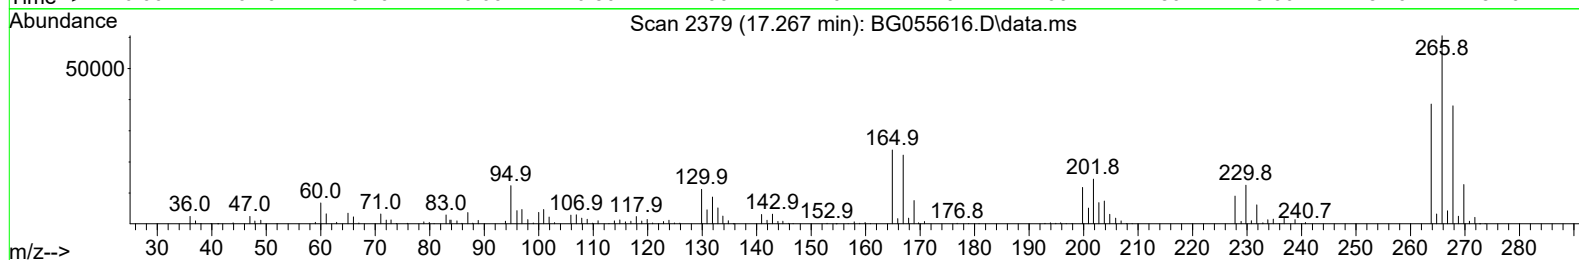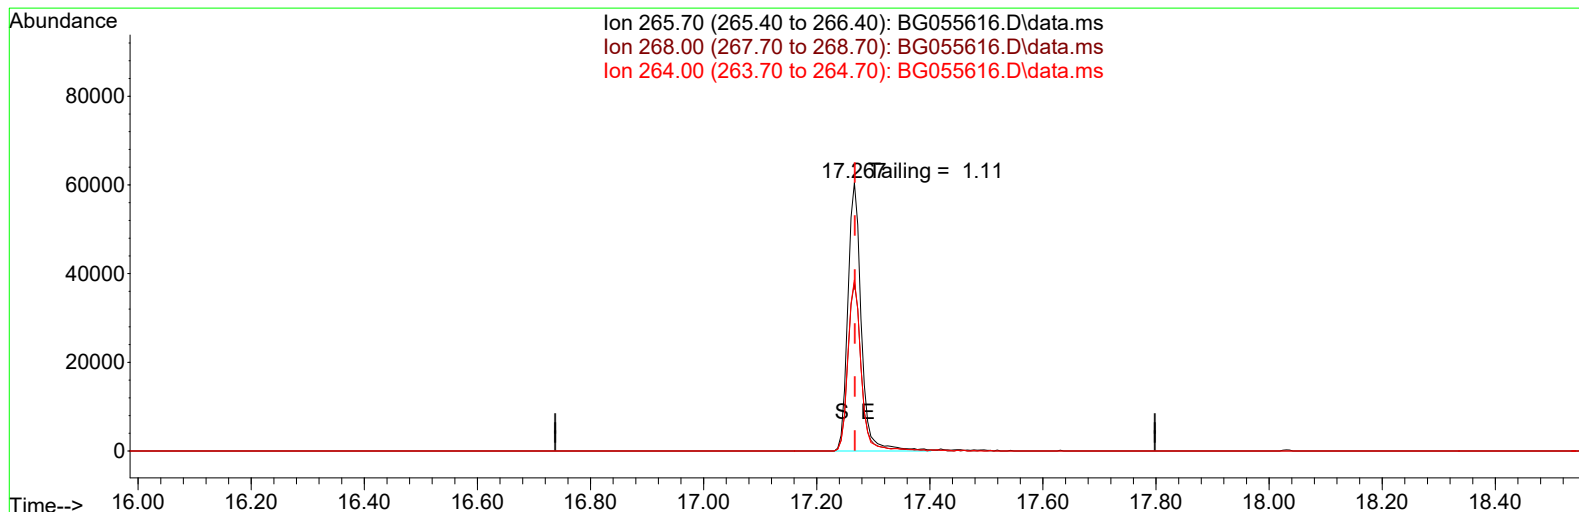

TIC: BG055616.D\data.ms

**(70) Pentachlorophenol (C)**

17.267min (-0.001) 24986.24 ng




response 100112

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.20  | 62.80  |
| 264.00 | 61.90  | 63.74  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG111522\  
Data File : BG055616.D  
Acq On : 15 Nov 2022 9:48  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Nov 16 04:11:36 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG110922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Nov 16 01:36:26 2022  
Response via : Initial Calibration

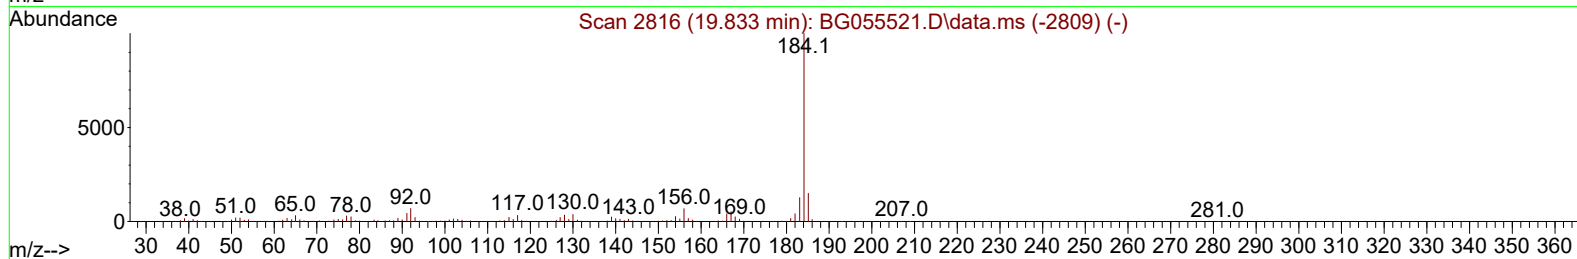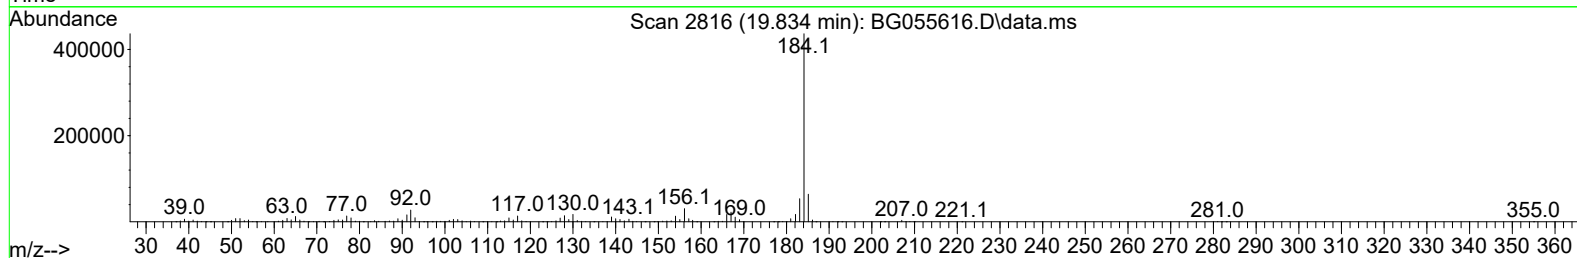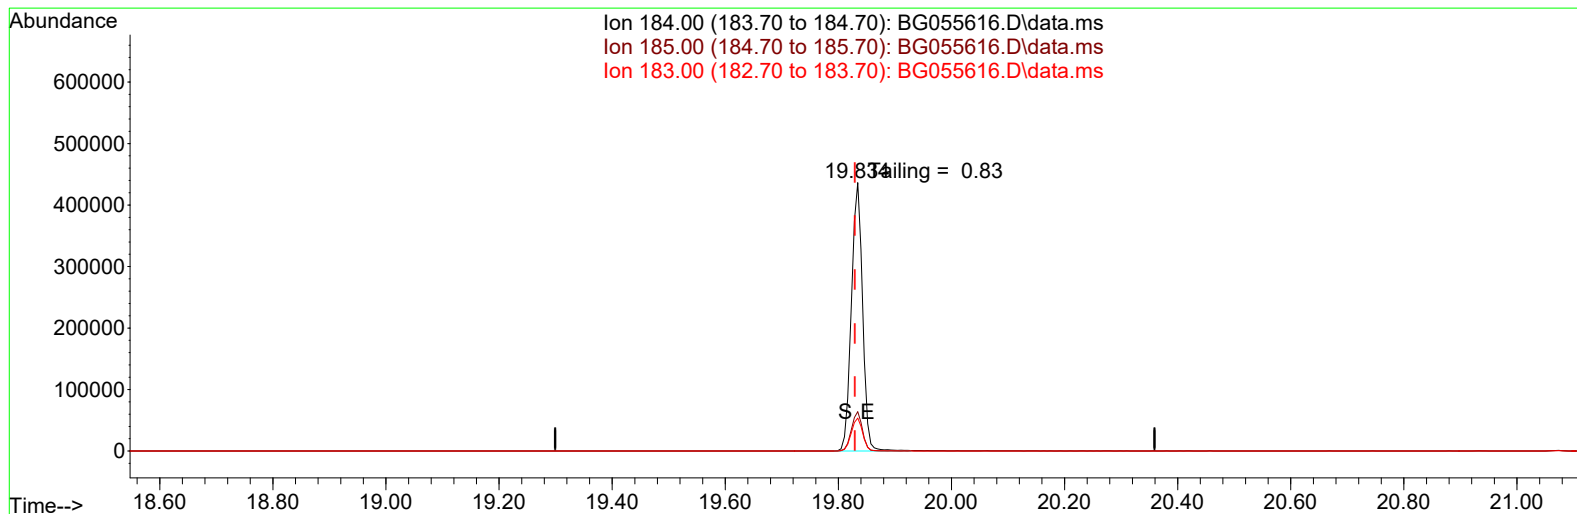

TIC: BG055616.D\data.ms

**(77) Benzidine**

**19.834min (+ 0.005) 114381.45 ng**

**response 603424**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.66  |
| 183.00 | 12.70  | 12.32  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/15/2022    | BNA_G            | <u>BG055616.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 273634           | 21.074             |
| DDD           | 6888             | 20.616             |
| DDE           | 370              | 20.116             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7258          | 280892           | 2.58               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP