


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111522\
Data File : BG055623.D
Acq On : 15 Nov 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 16 01:36:26 2022

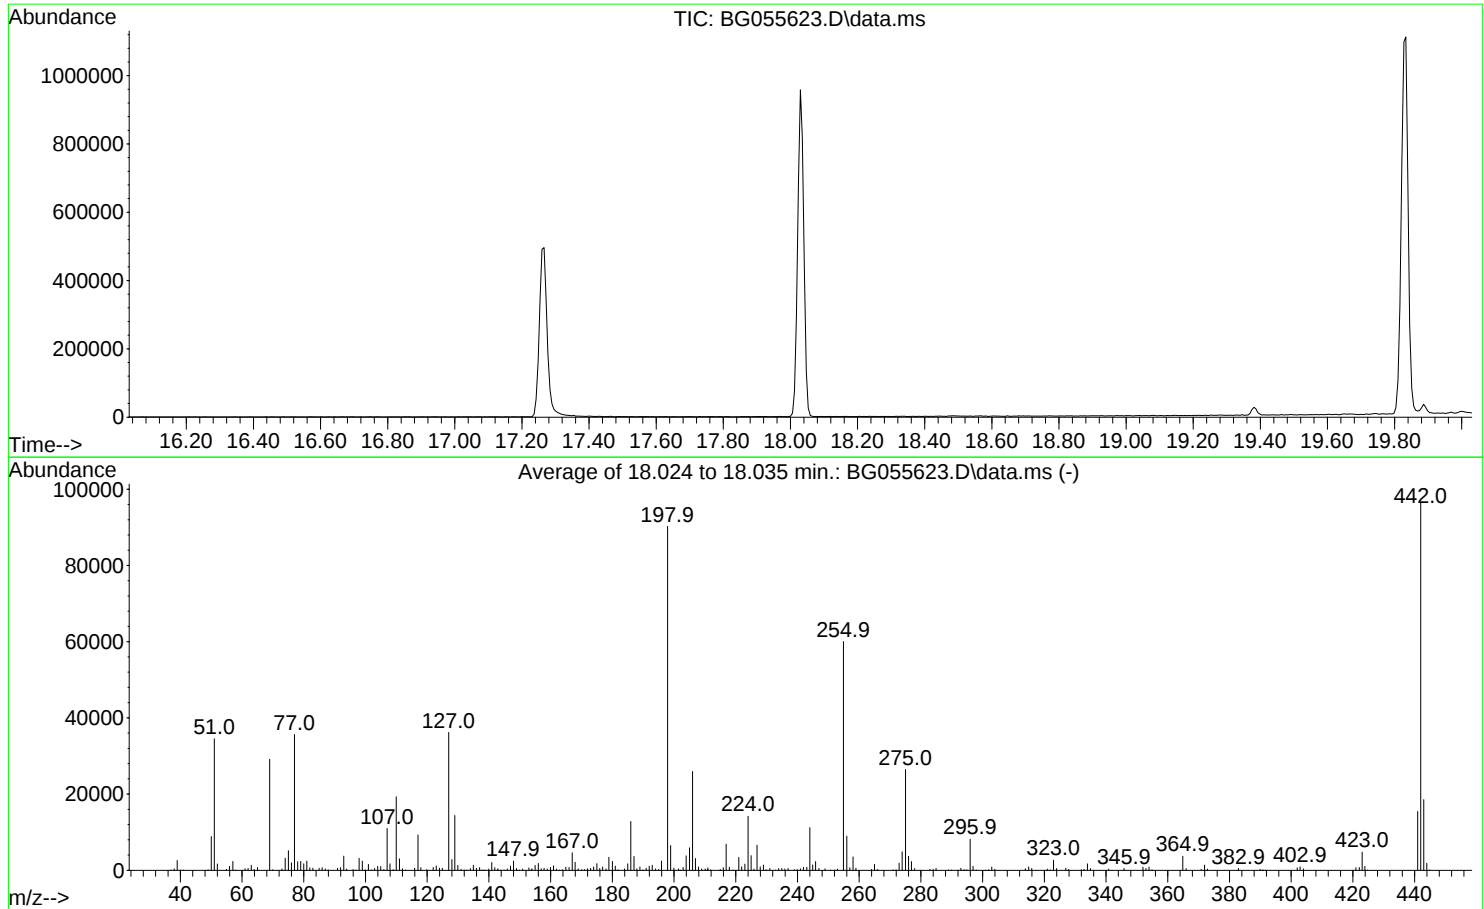




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	34509	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.3	29131	PASS
70	69	0.00	2	0.5	135	PASS
127	198	10	80	40.1	36160	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90248	PASS
199	198	5	9	7.2	6510	PASS
275	198	10	60	29.3	26469	PASS
365	198	1	100	4.1	3680	PASS
441	198	0.01	100	17.1	15419	PASS
442	442	50	100	100.0	96547	PASS
443	442	15	24	19.2	18560	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111522\
Data File : BG055623.D
Acq On : 15 Nov 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 16:09:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

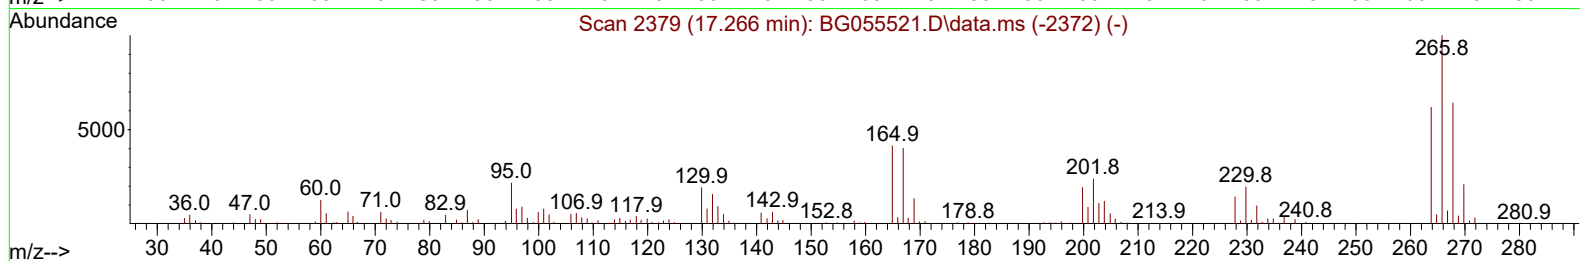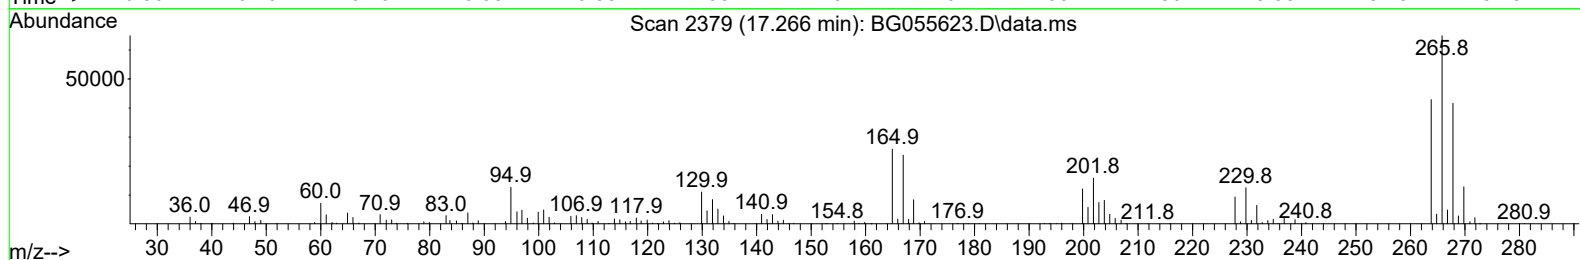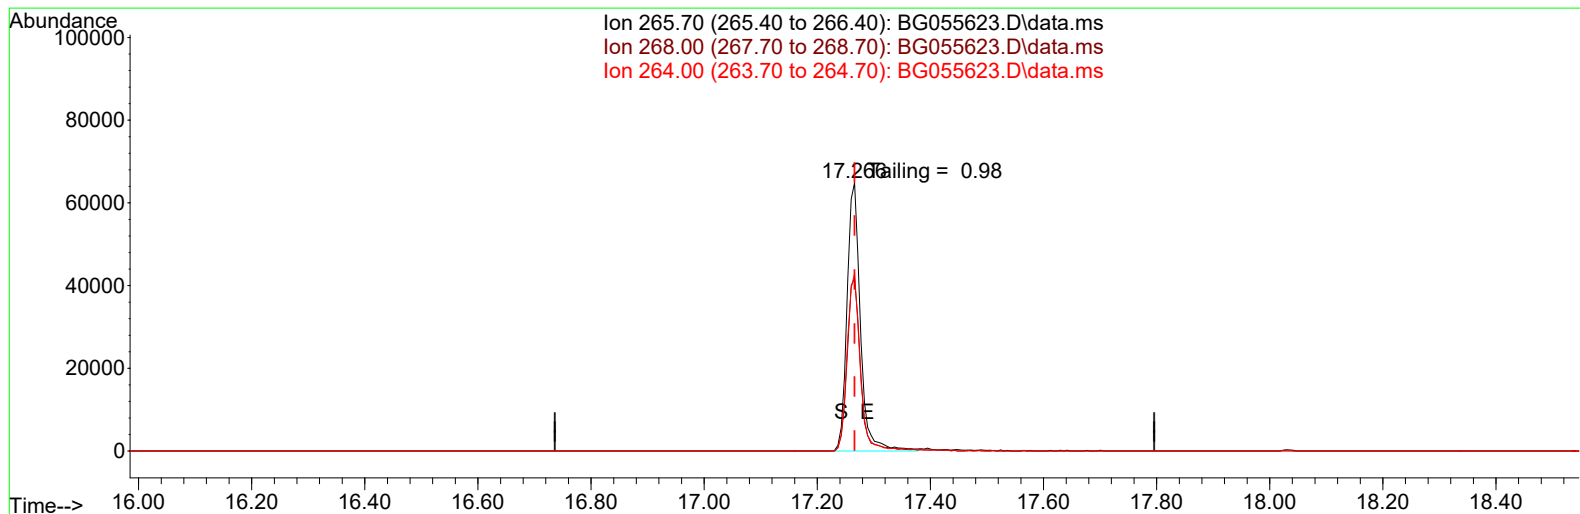

TIC: BG055623.D\data.ms

(70) Pentachlorophenol (C)

17.266min (-0.000) 35102.62 ng




response 106825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.14
264.00	61.90	66.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111522\
Data File : BG055623.D
Acq On : 15 Nov 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 15 16:09:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG110922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 10 03:39:46 2022
Response via : Initial Calibration

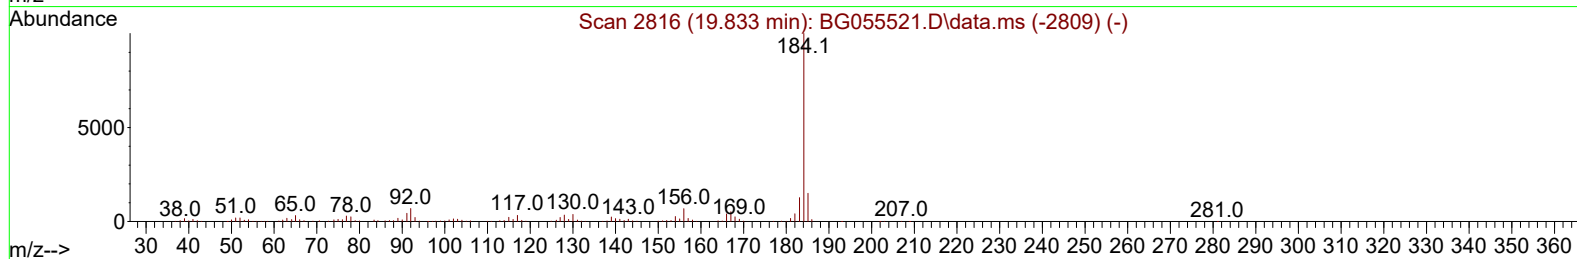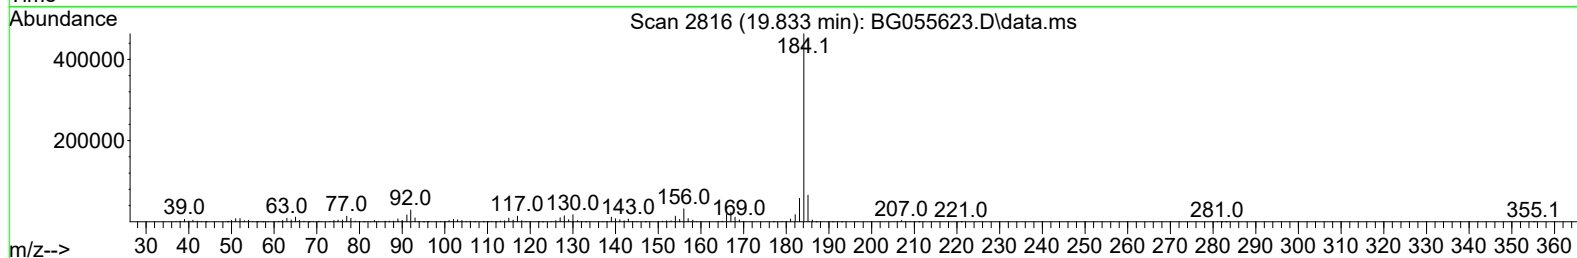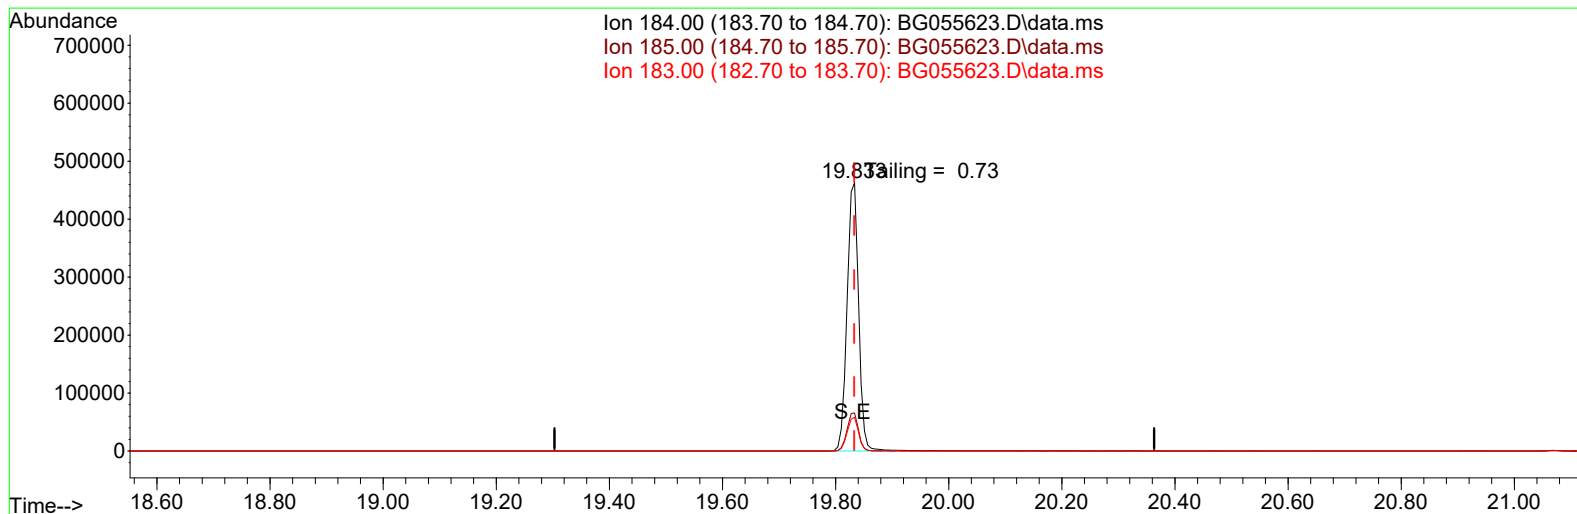

TIC: BG055623.D\data.ms

(77) Benzidine

19.833min (+ 0.000) 399521.94 ng

response 659330

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.19
183.00	12.70	12.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/15/2022	BNA_G	<u>BG055623.D</u>
Compound Name	Response	Retention Time
DDT	307406	21.067
DDD	7199	20.615
DDE	296	20.109
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7495	314901	2.38

Instrument :
BNA_G
ClientSampleId :
DFTPP