

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG111615\  
 Data File : BG019647.D  
 Acq On : 16 Nov 2015 23:08  
 Operator : UM/NP  
 Sample : G4323-03  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 A4HT4

Quant Time: Nov 17 02:02:15 2015  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG111615.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Nov 17 01:14:52 2015  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 8.15  | 152  | 27361    | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.98 | 136  | 115699   | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.78 | 164  | 97351    | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.53 | 188  | 292796   | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.79 | 240  | 414627   | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 25.11 | 264  | 399266   | 20.00 | ng/ul | 0.00     |

## System Monitoring Compounds

|                                |       |     |        |       |       |      |
|--------------------------------|-------|-----|--------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.44  | 96  | 3174   | 4.95  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 7.30  | 99  | 72092  | 25.72 | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.46  | 67  | 53230  | 28.98 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.67  | 132 | 48684  | 27.08 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.85  | 113 | 56755  | 24.46 | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 9.32  | 128 | 26193  | 27.57 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 10.05 | 143 | 32209  | 30.13 | ng/ul | 0.00 |
| 26) 2,4-Dichlorophenol-d3      | 10.59 | 165 | 59761  | 25.85 | ng/ul | 0.00 |
| 29) 4-Chloroaniline-d4         | 11.11 | 131 | 71473  | 32.57 | ng/ul | 0.00 |
| 44) Dimethylphthalate-d6       | 14.18 | 166 | 259725 | 29.50 | ng/ul | 0.00 |
| 47) Acenaphthylene-d8          | 14.48 | 160 | 263674 | 27.63 | ng/ul | 0.00 |
| 52) 4-Nitrophenol-d4           | 14.97 | 143 | 40509  | 29.20 | ng/ul | 0.00 |
| 58) Fluorene-d10               | 15.77 | 176 | 215708 | 27.38 | ng/ul | 0.00 |
| 63) 4,6-Dinitro-2-methylphenol | 15.88 | 200 | 49364  | 26.10 | ng/ul | 0.00 |
| 71) Anthracene-d10             | 17.62 | 188 | 389195 | 27.38 | ng/ul | 0.00 |
| 79) Pyrene-d10                 | 19.89 | 212 | 471990 | 24.98 | ng/ul | 0.00 |
| 90) Benzo(a)pyrene-d12         | 24.88 | 264 | 512425 | 24.58 | ng/ul | 0.00 |


| Target Compounds      |       |     |        |       |       | Qvalue |
|-----------------------|-------|-----|--------|-------|-------|--------|
| 6) Phenol             | 7.33  | 94  | 5122   | 1.69  | ng/ul | 94     |
| 45) Dimethylphthalate | 14.22 | 163 | 161096 | 18.45 | ng/ul | 99     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG111615\  
Data File : BG019647.D  
Acq On : 16 Nov 2015 23:08  
Operator : UM/NP  
Sample : G4323-03  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
A4HT4

Quant Time: Nov 17 02:02:15 2015  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\SOM02.2-EPA-BG111615.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Nov 17 01:14:52 2015  
Response via : Initial Calibration

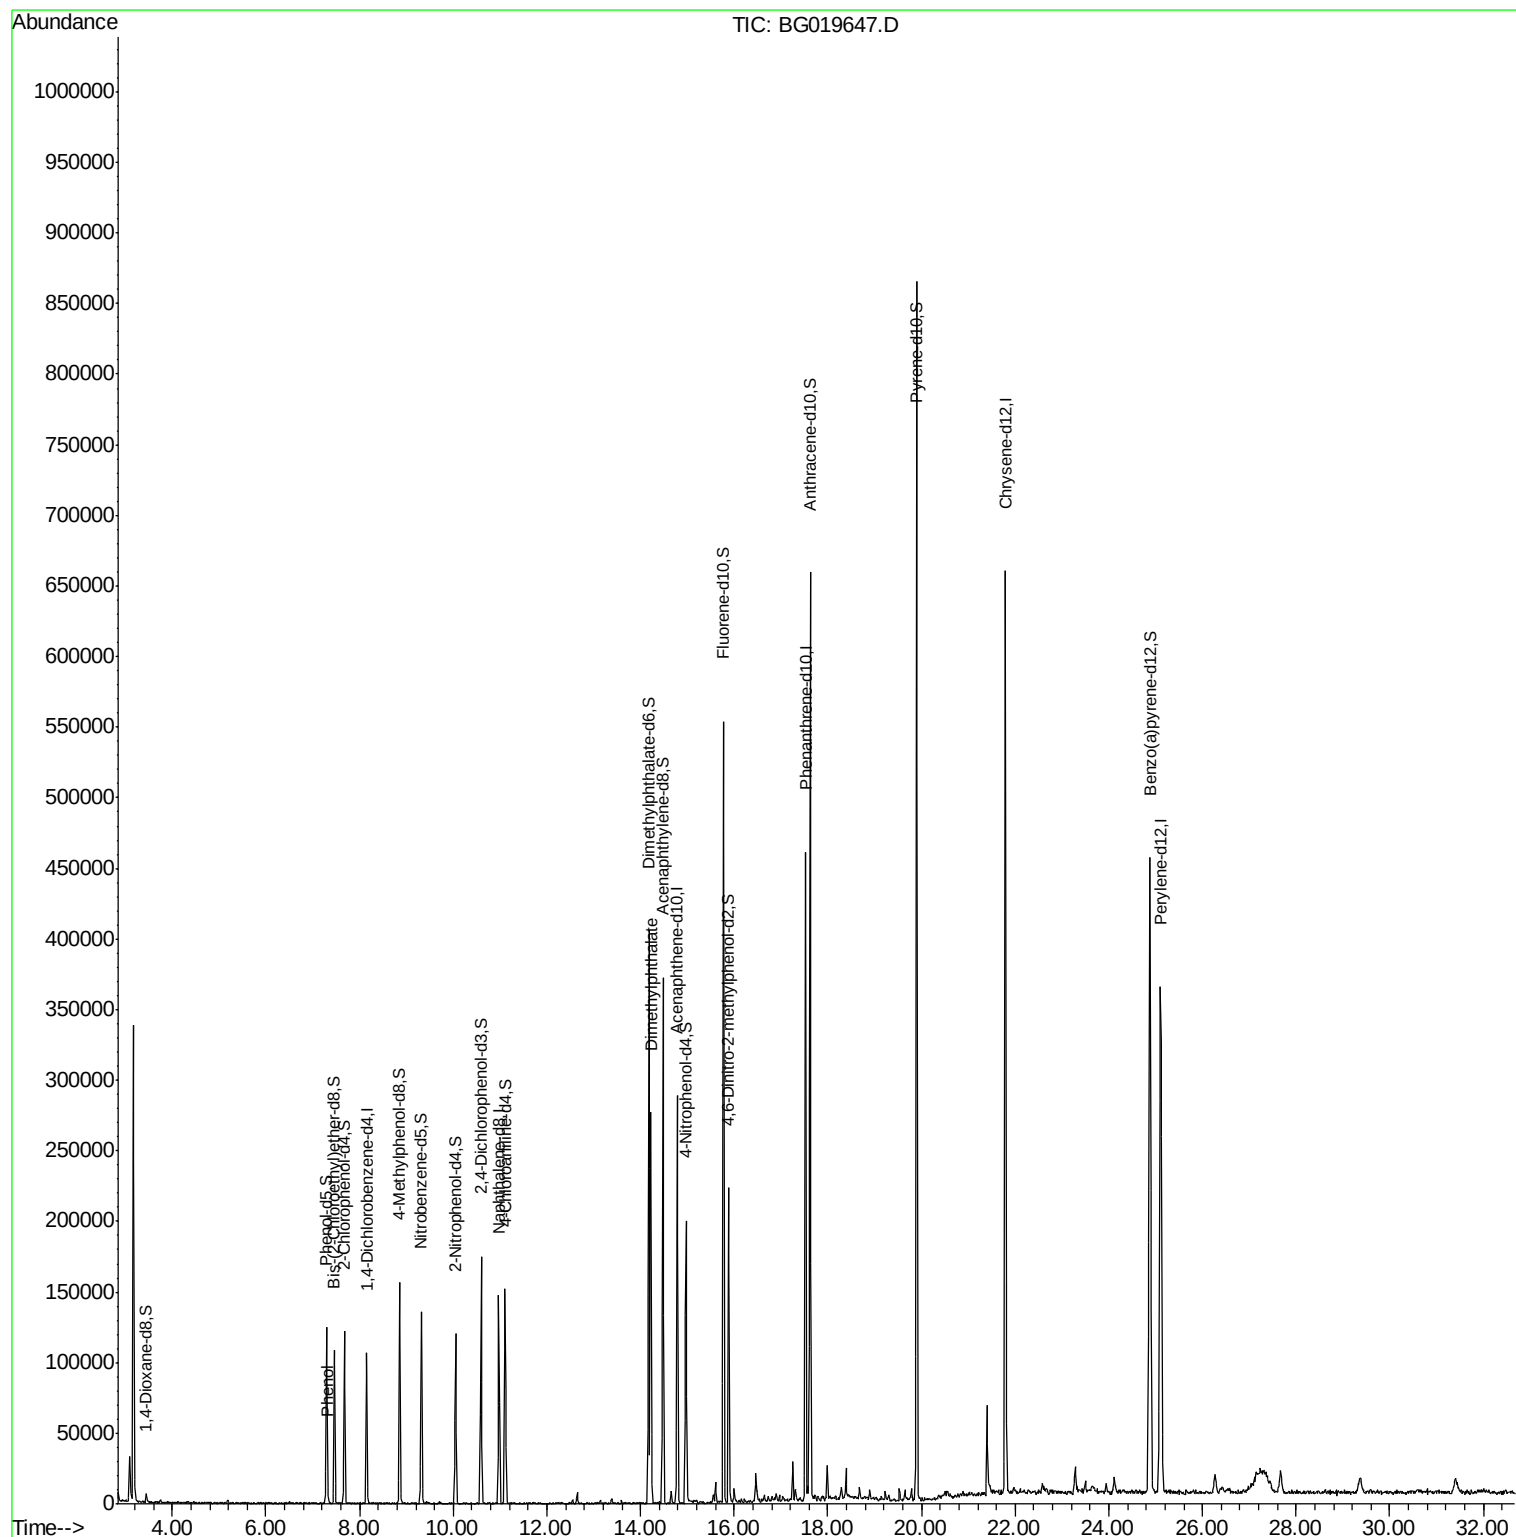

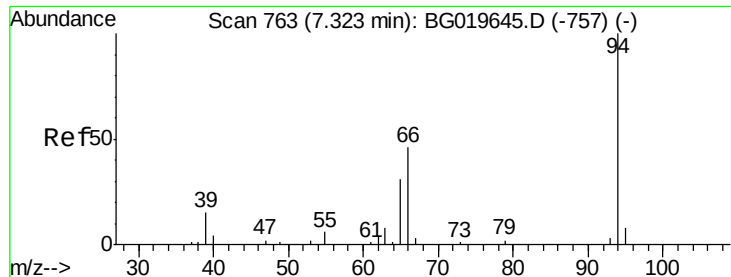

#6

Phenol

Concen: 1.69 ng/ul

RT: 7.33 min Scan# 764

Delta R.T. 0.00 min

Lab File: BG019647.D

Acq: 16 Nov 2015 23:08

Instrument :

BNA\_G

ClientSampleId :

A4HT4


Tgt Ion: 94 Resp: 5122

Ion Ratio Lower Upper




94 100

65 35.7 27.4 41.0

66 54.9 39.0 58.6

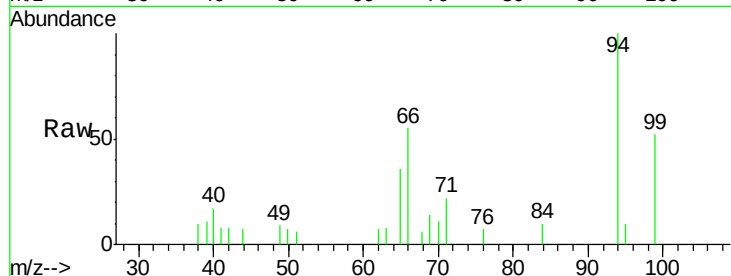

Abundance Ion 94.00 (93.70 to 94.70): BGC  
Ion 65.00 (64.70 to 65.70): BGC  
Ion 66.00 (65.70 to 66.70): BGC

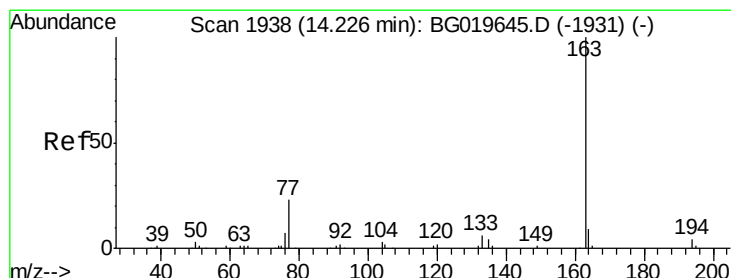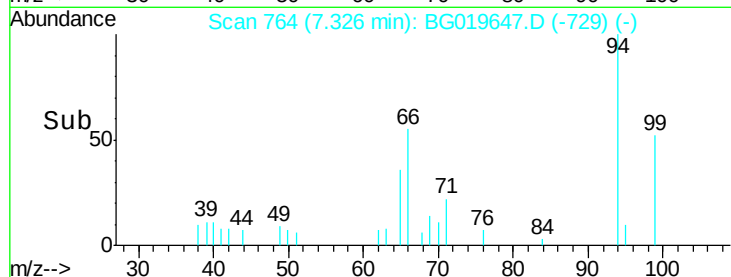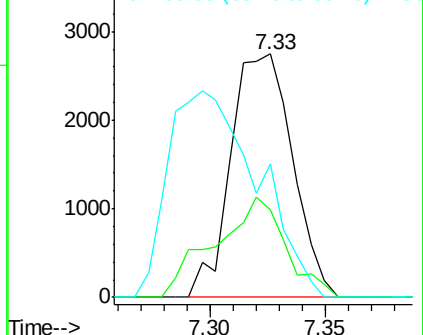

#45

Dimethylphthalate

Concen: 18.45 ng/ul

RT: 14.22 min Scan# 1938

Delta R.T. -0.00 min

Lab File: BG019647.D

Acq: 16 Nov 2015 23:08


Tgt Ion: 163 Resp: 161096

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.6 8.3 12.5

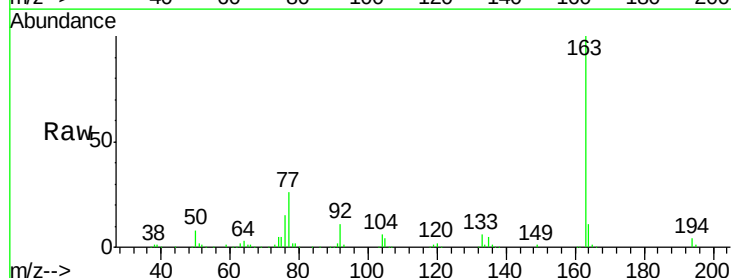

Abundance Ion 163.00 (162.70 to 163.70): E  
Ion 194.00 (193.70 to 194.70): E  
Ion 164.00 (163.70 to 164.70): E

