

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111615\
 Data File : BG019653.D
 Acq On : 17 Nov 2015 2:57
 Operator : UM/NP
 Sample : G4323-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4HW1

Quant Time: Nov 17 03:56:14 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 17 01:14:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	24473	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	103772	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.78	164	84780	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.52	188	246728	20.00	ng/ul	0.00
78) Chrysene-d12	21.79	240	337350	20.00	ng/ul	0.00
86) Perylene-d12	25.10	264	316911	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	2754	4.81	ng/uL	0.00
5) Phenol-d5	7.29	99	62061	24.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	46239	28.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.67	132	40888	25.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	45666	22.00	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	22747	26.70	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	26341	27.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	50552	24.38	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	63038	32.03	ng/ul	0.00
44) Dimethylphthalate-d6	14.18	166	213916	27.90	ng/ul	0.00
47) Acenaphthylene-d8	14.48	160	220553	26.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.97	143	33425	27.67	ng/ul	0.00
58) Fluorene-d10	15.77	176	181768	26.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.88	200	38641	24.24	ng/ul	0.00
71) Anthracene-d10	17.62	188	320751	26.78	ng/ul	0.00
79) Pyrene-d10	19.90	212	377893	24.58	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.88	264	405942	24.54	ng/ul	0.00


Target Compounds						Qvalue
6) Phenol	7.32	94	3732	1.38	ng/ul	97
45) Dimethylphthalate	14.22	163	97563	12.83	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111615\
Data File : BG019653.D
Acq On : 17 Nov 2015 2:57
Operator : UM/NP
Sample : G4323-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4HW1

Quant Time: Nov 17 03:56:14 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 17 01:14:52 2015
Response via : Initial Calibration

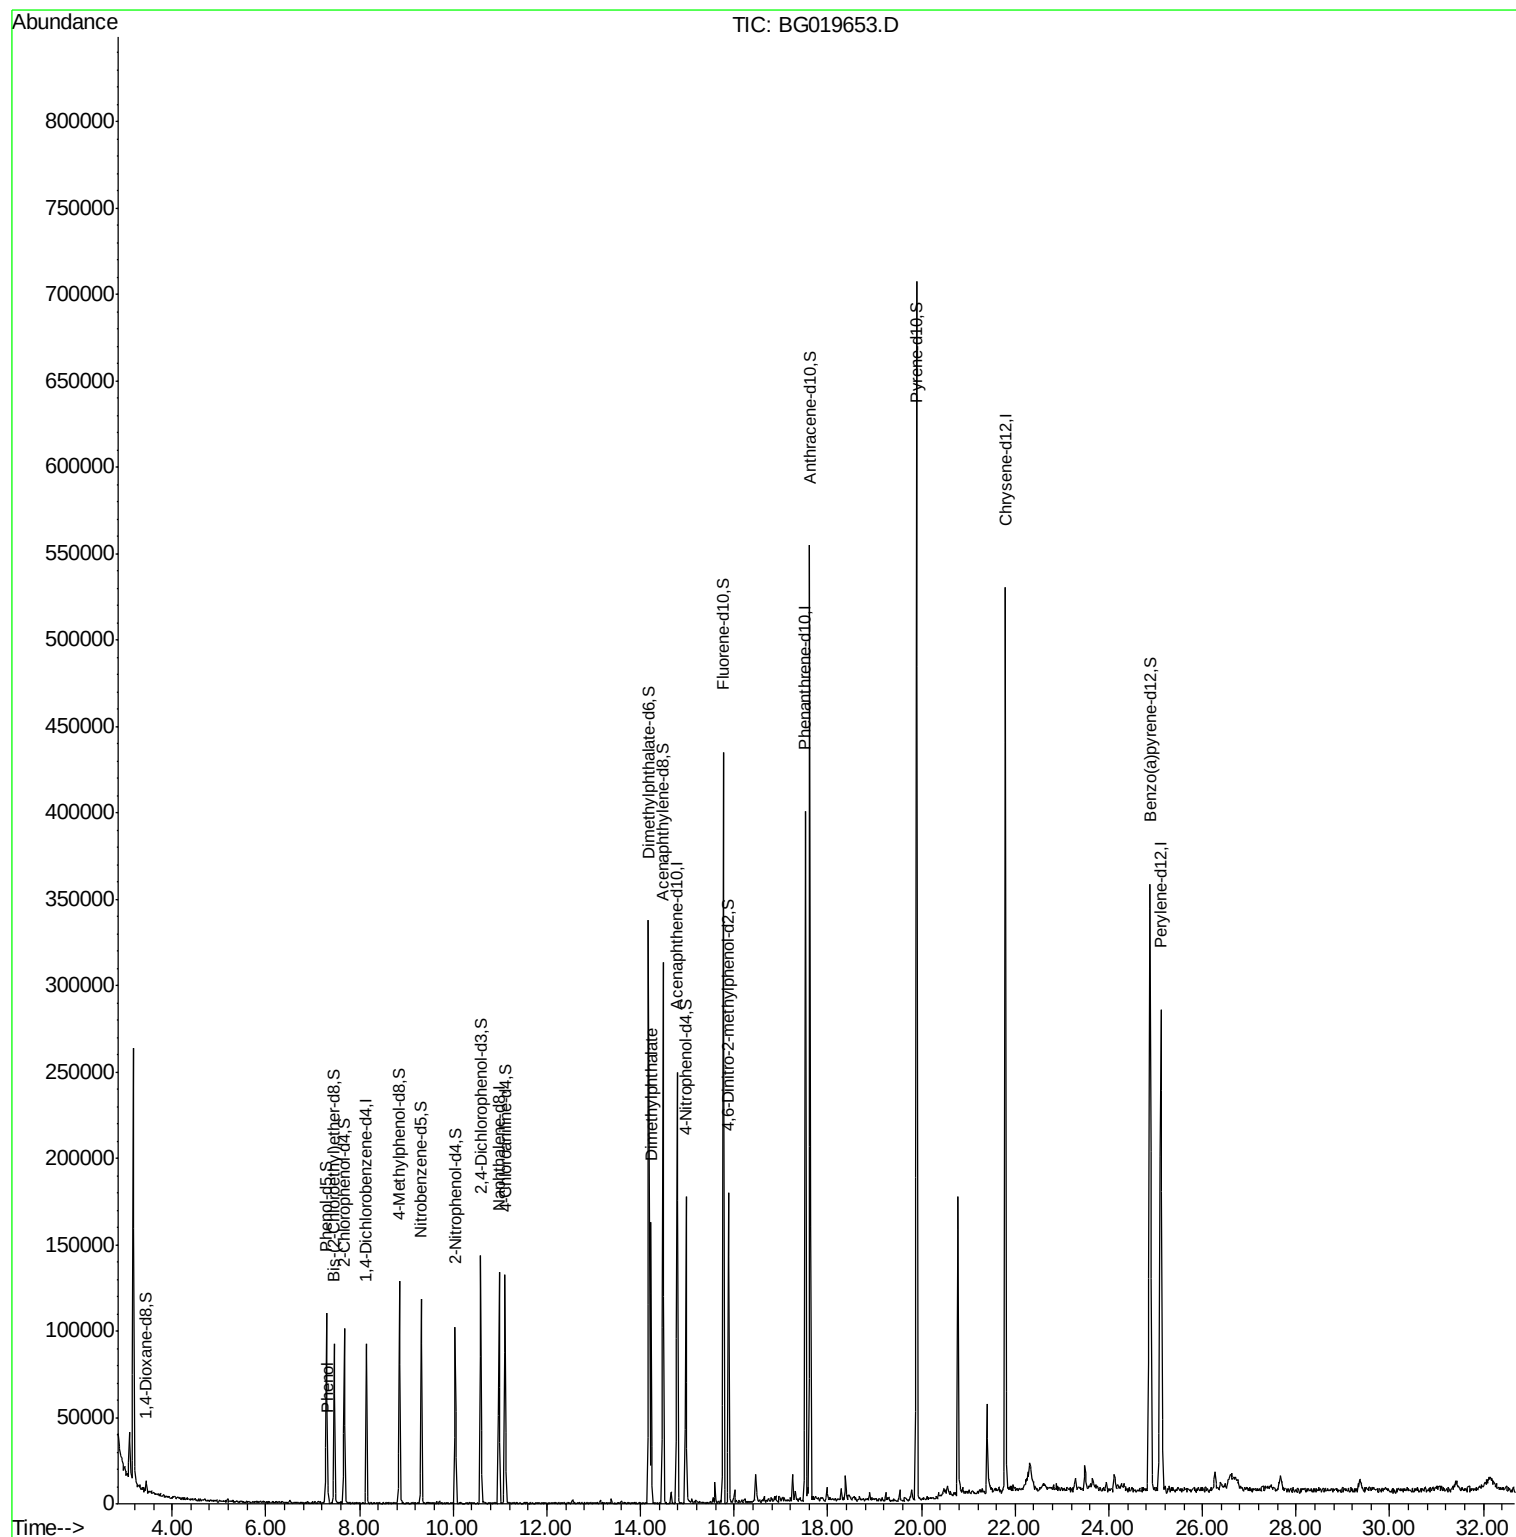

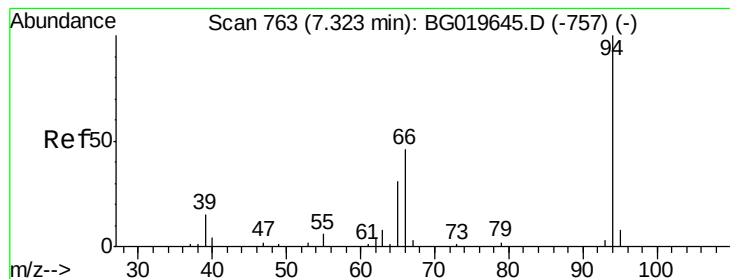

#6

Phenol

Concen: 1.38 ng/ul

RT: 7.32 min Scan# 763

Delta R.T. 0.00 min

Lab File: BG019653.D

Acq: 17 Nov 2015 2:57

Instrument :

BNA_G

ClientSampleId :

A4HW1


Tgt Ion: 94 Resp: 3732

Ion Ratio Lower Upper




94 100

65 33.8 27.4 41.0

66 45.9 39.0 58.6

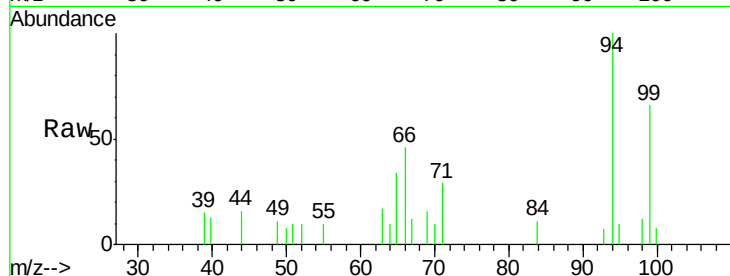

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

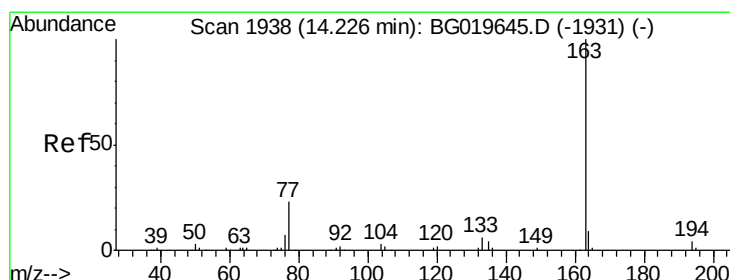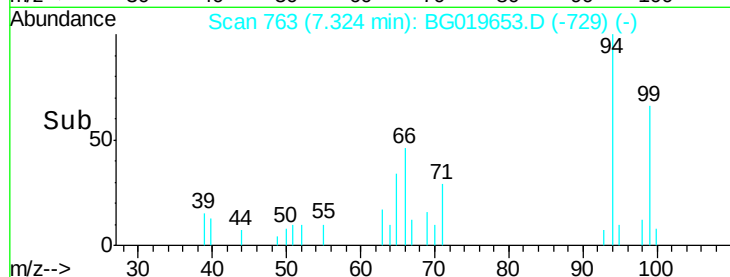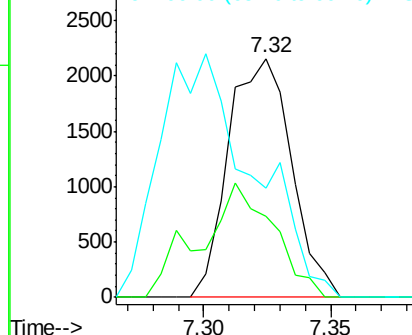

#45

Dimethylphthalate

Concen: 12.83 ng/ul

RT: 14.22 min Scan# 1937

Delta R.T. -0.00 min

Lab File: BG019653.D

Acq: 17 Nov 2015 2:57


Tgt Ion: 163 Resp: 97563

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 10.6 8.3 12.5

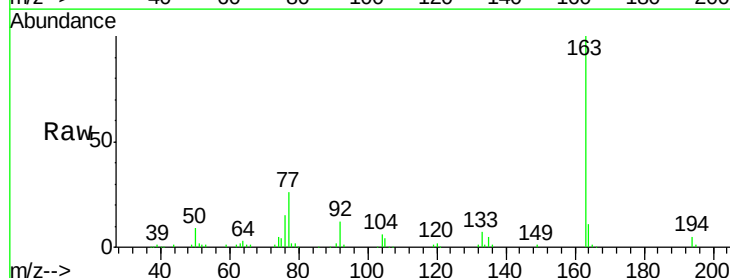

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

