
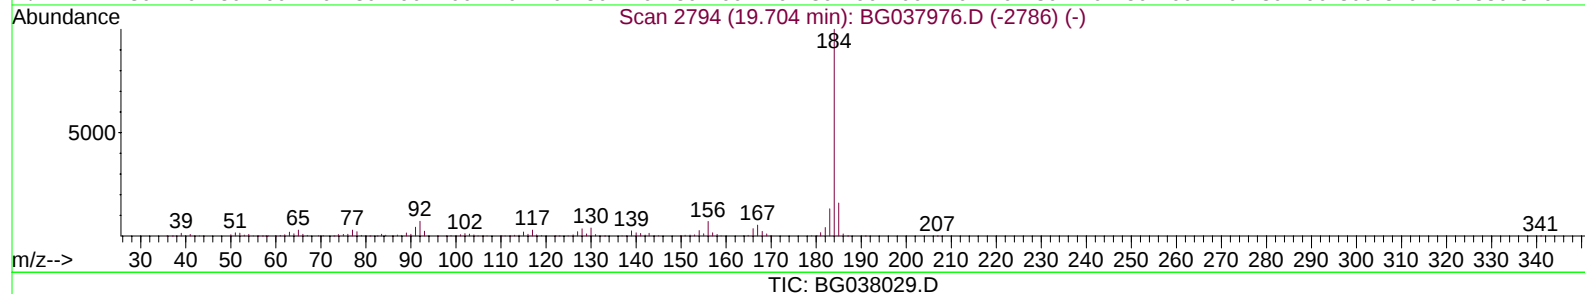
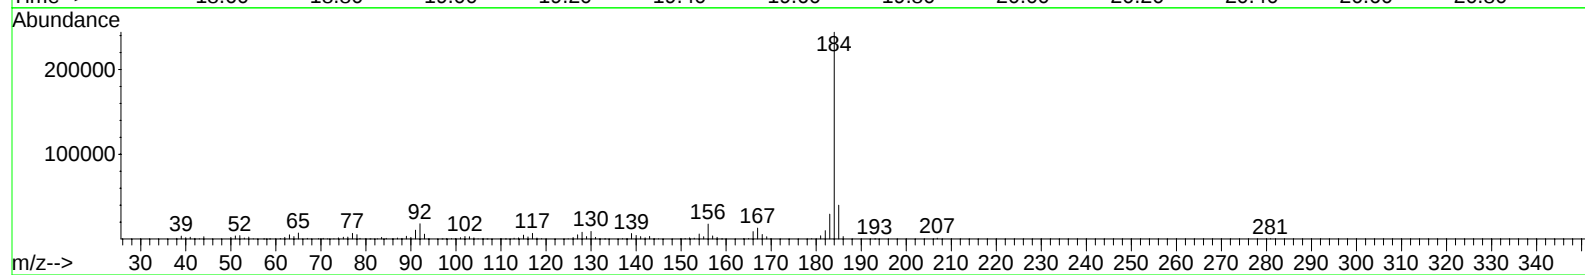


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111618\  
Data File : BG038029.D  
Acq On : 16 Nov 2018 11:30  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 17:04:10 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 13 16:39:28 2018  
Response via : Initial Calibration

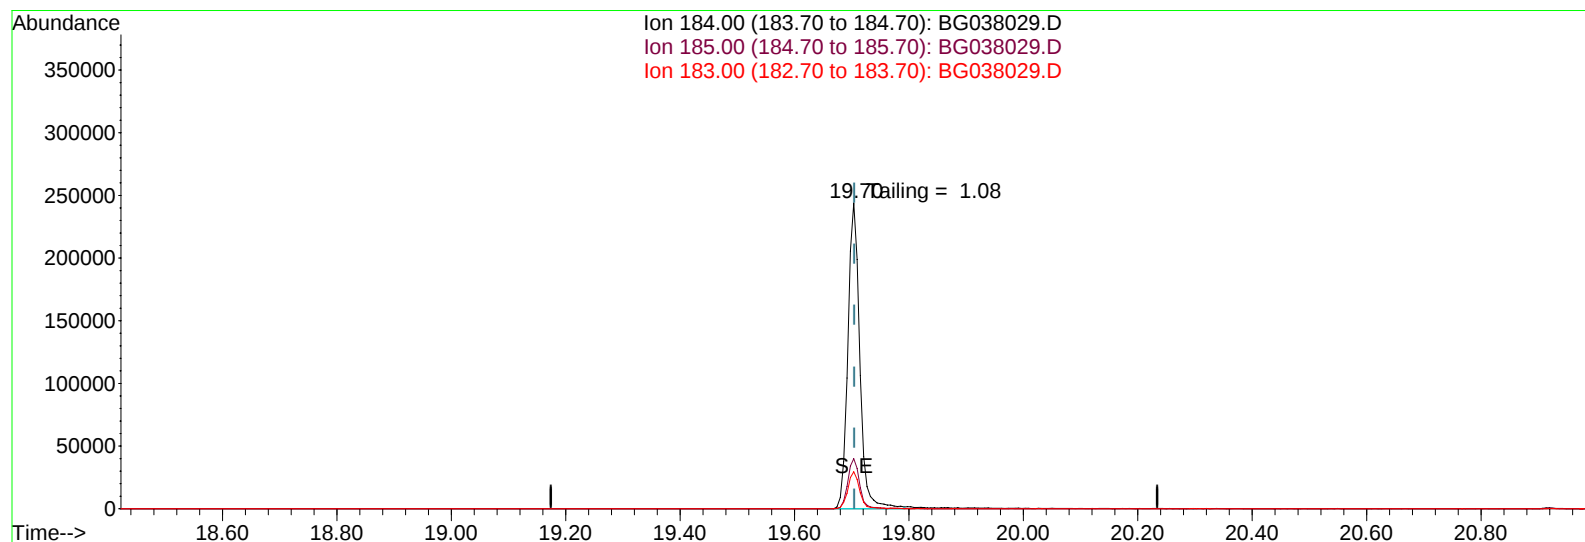

(77) Benzidine




19.703min (-0.001) 92952.94ng

response 358781

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 16.40 |
| 183.00 | 12.70 | 12.09 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111618\  
Data File : BG038029.D  
Acq On : 16 Nov 2018 11:30  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 17:04:10 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 13 16:39:28 2018  
Response via : Initial Calibration

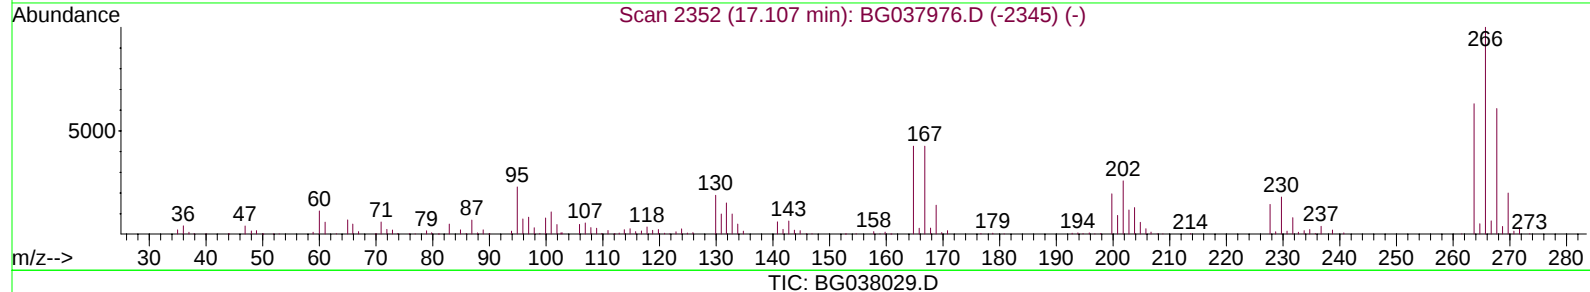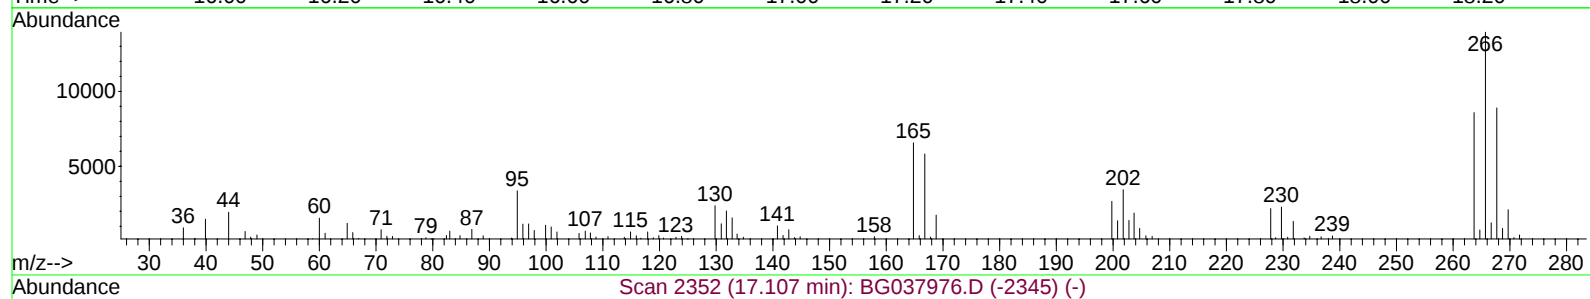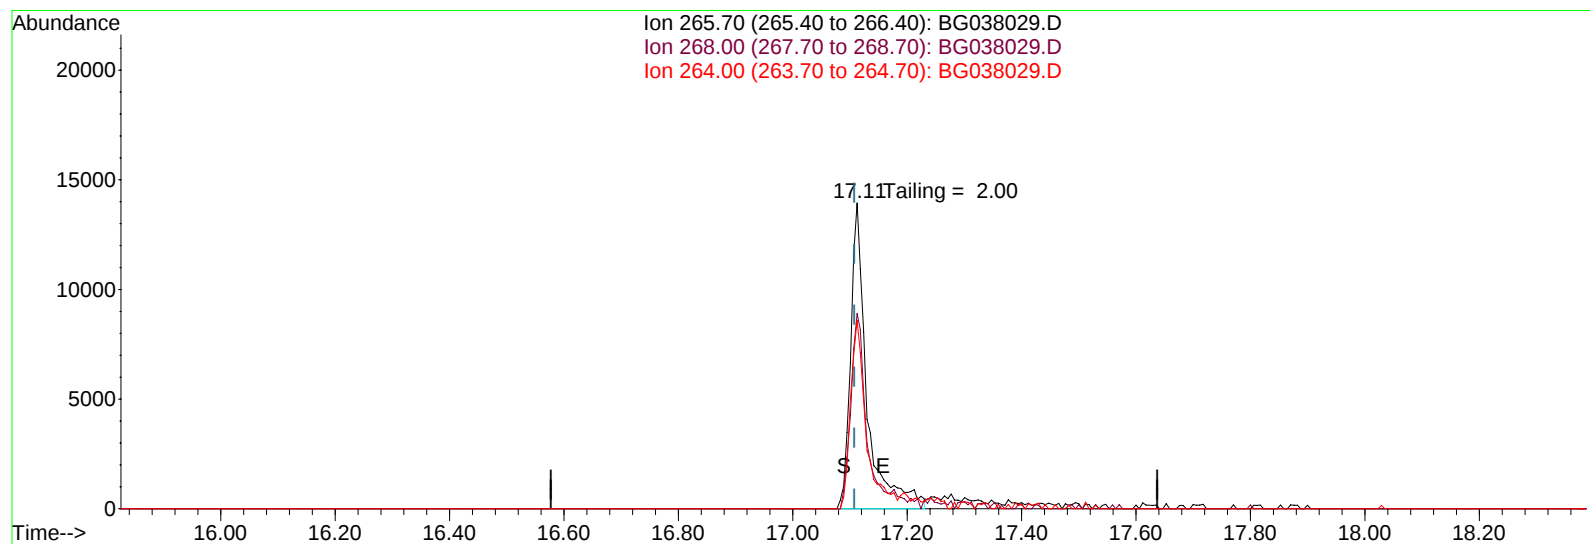

(70) Pentachlorophenol (C)

17.112min (+0.005) 17529.03ng

response 28324

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 70.01 |
| 264.00 | 73.60 | 67.06 |
| 0.00   | 0.00  | 0.00  |