


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111618\  
 Data File : BG038047.D  
 Acq On : 16 Nov 2018 23:52  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG111318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Nov 13 16:39:28 2018

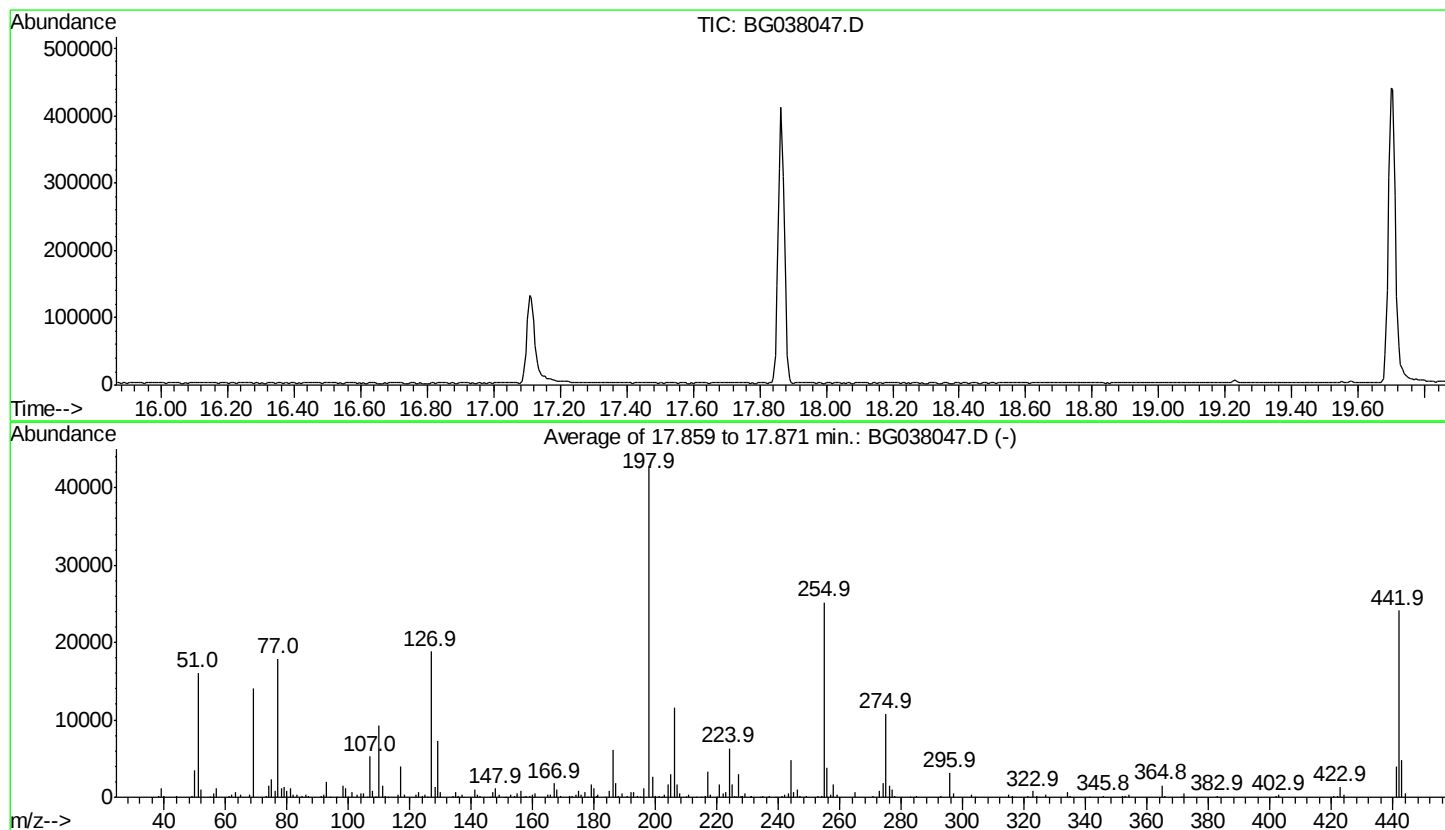

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 37.5      | 16079   | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 279     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.9      | 14100   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 43.9      | 18817   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 42853   | PASS             |
| 199         | 198          | 5            | 9            | 6.3       | 2721    | PASS             |
| 275         | 198          | 10           | 60           | 25.3      | 10832   | PASS             |
| 365         | 198          | 1            | 100          | 3.6       | 1530    | PASS             |
| 441         | 198          | 0.01         | 100          | 9.3       | 3987    | PASS             |
| 442         | 198          | 50           | 100          | 56.3      | 24122   | PASS             |
| 443         | 442          | 15           | 24           | 20.0      | 4821    | PASS             |