
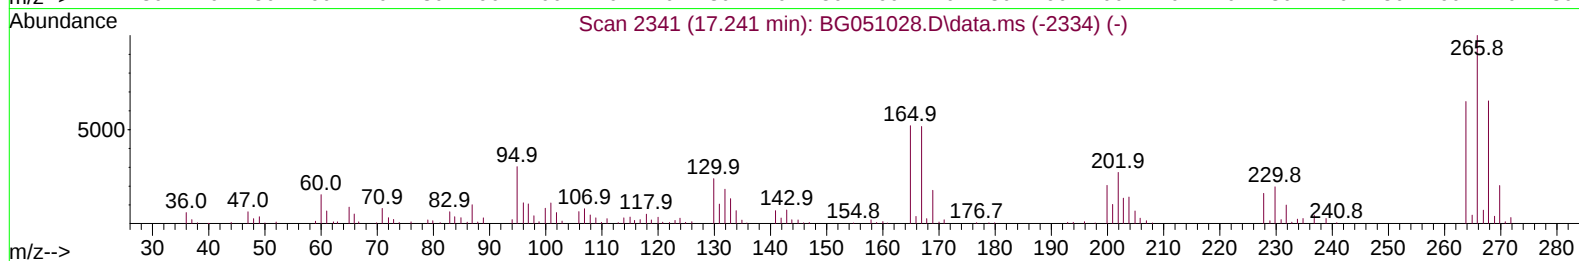
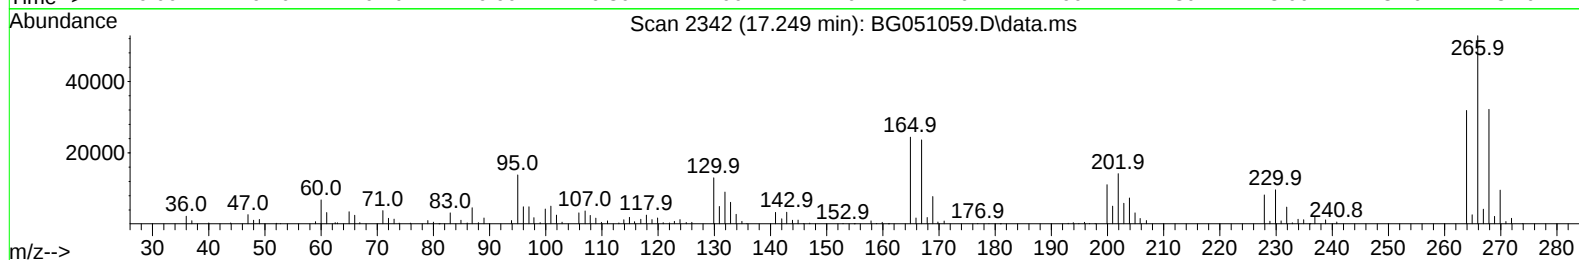


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\  
Data File : BG051059.D  
Acq On    : 16 Nov 2021    9:10  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 16 10:09:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

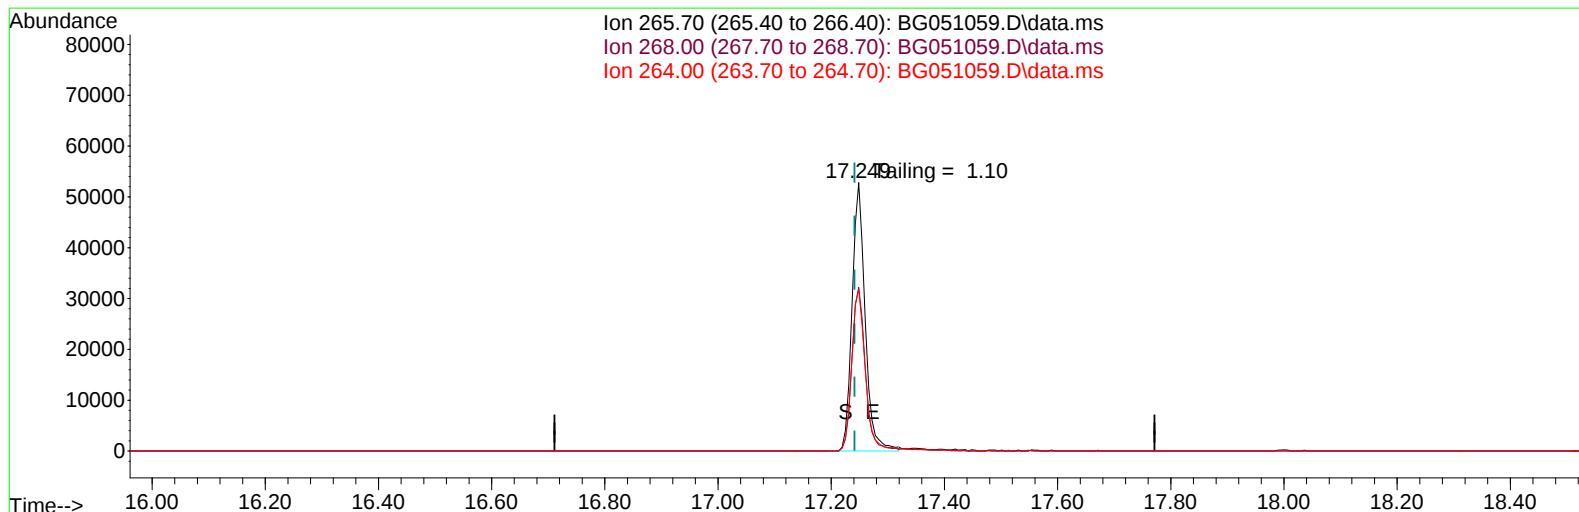

TIC: BG051059.D\data.ms

(70) Pentachlorophenol (C)




17.249min (+ 0.008) 33744.81 ng

response 84901

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.01
264.00	61.30	60.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
 Data File : BG051059.D
 Acq On : 16 Nov 2021 9:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 10:09:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 03:55:35 2021
 Response via : Initial Calibration

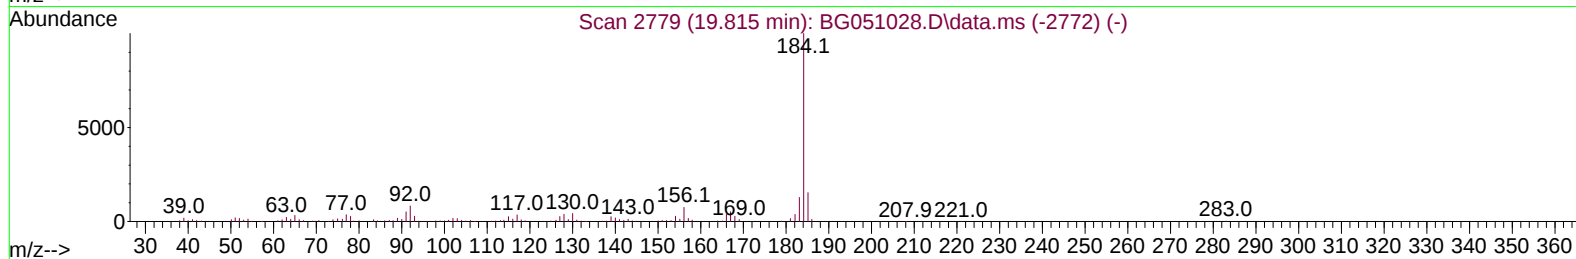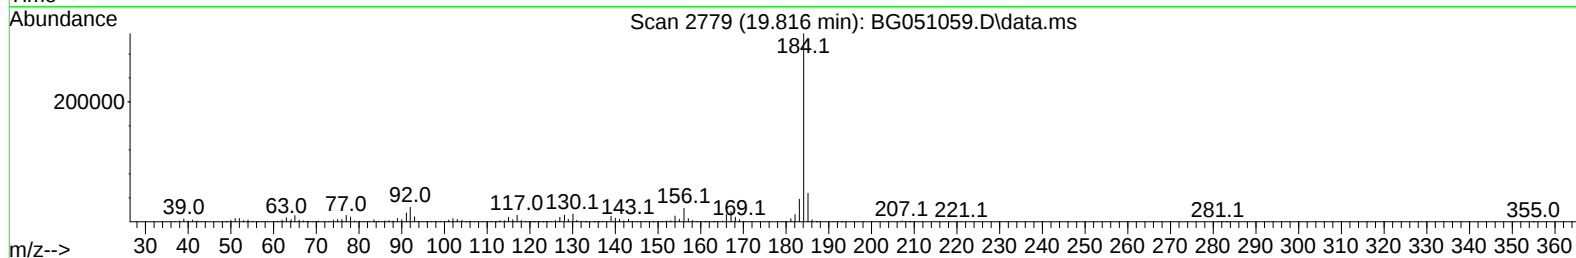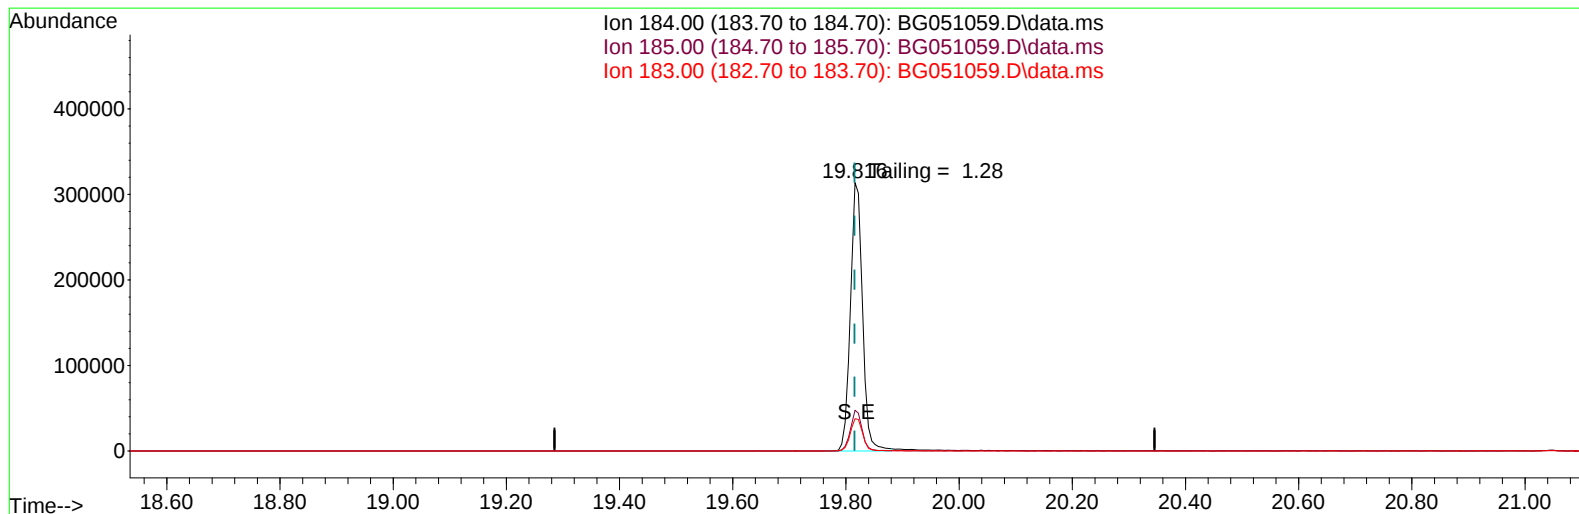

TIC: BG051059.D\data.ms

(77) Benzidine

19.816min (+ 0.001) 0.00 ng

response 473060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.20
183.00	11.70	12.04
0.00	0.00	0.00