
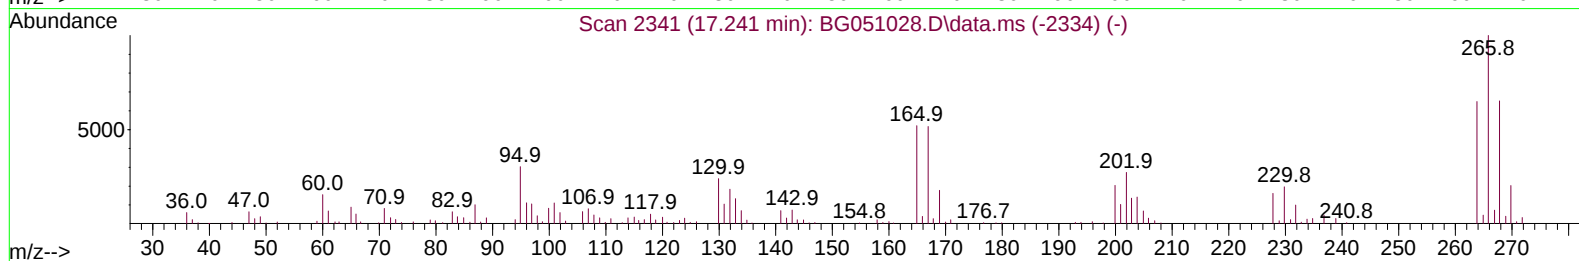
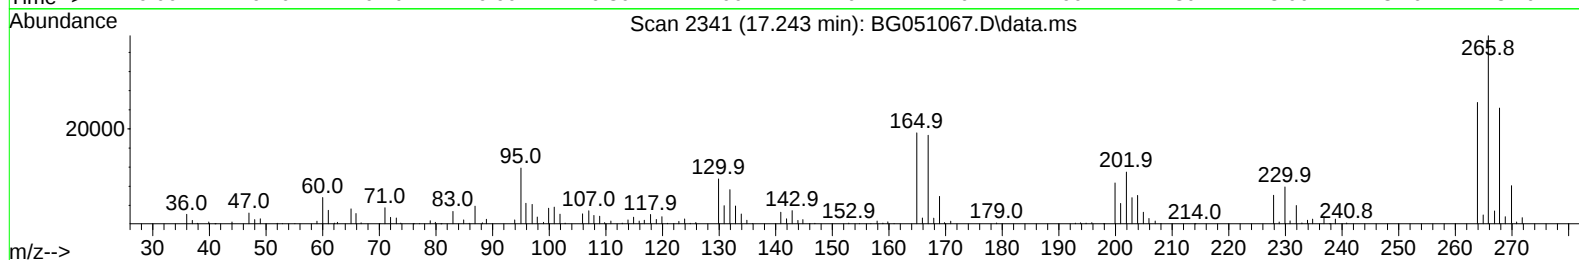


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
Data File : BG051067.D
Acq On    : 16 Nov 2021  15:04
Operator  : CG/JU
Sample    : DFTPP
Misc      :
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Nov 16 15:59:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

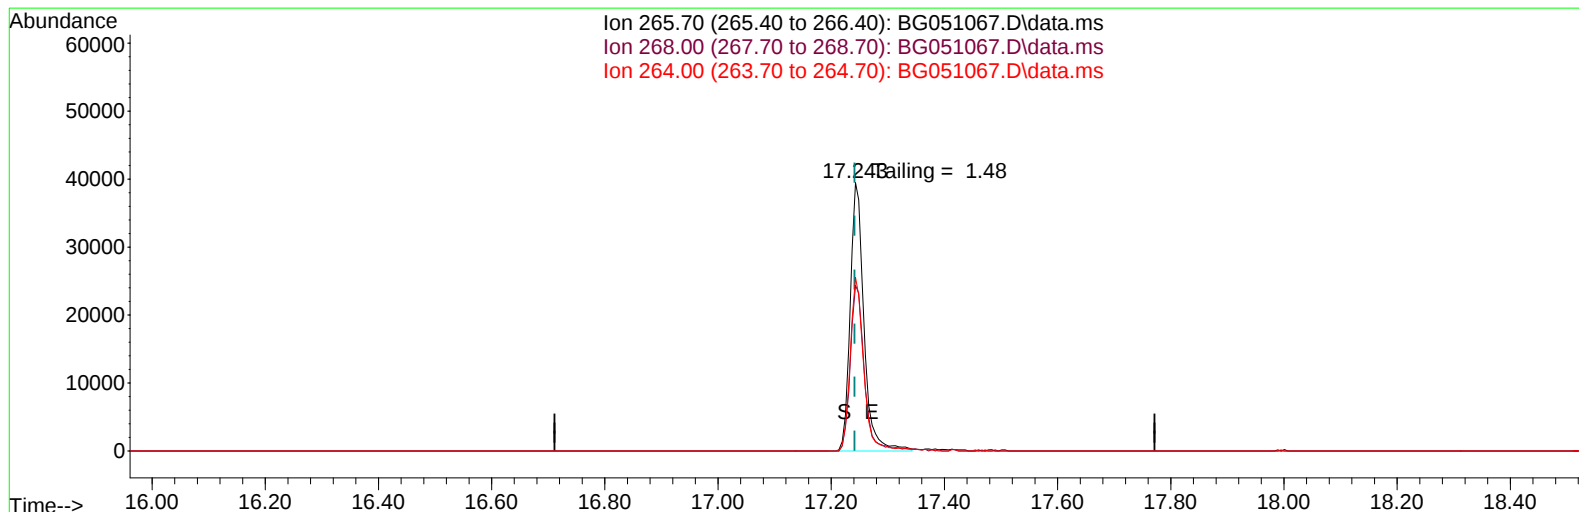

TIC: BG051067.D\data.ms

(70) Pentachlorophenol (C)




17.243min (+ 0.002) 44989.87 ng

response **66863**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.72
264.00	61.30	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
Data File : BG051067.D
Acq On : 16 Nov 2021 15:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 15:59:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

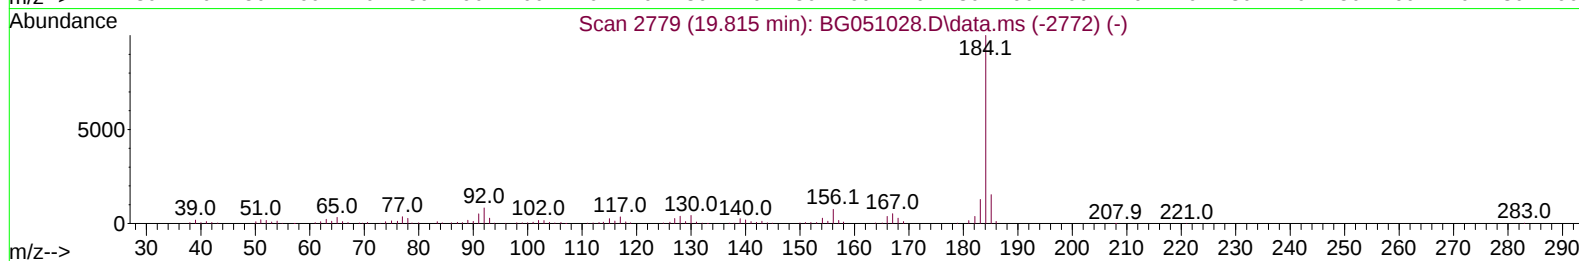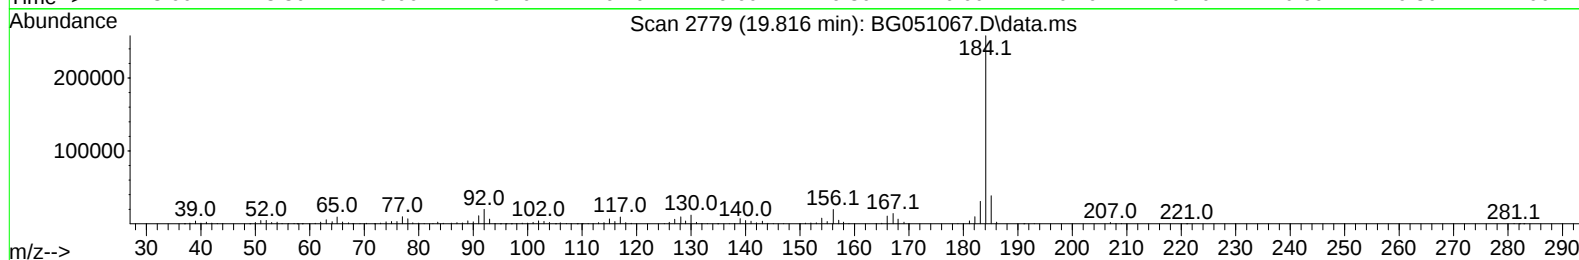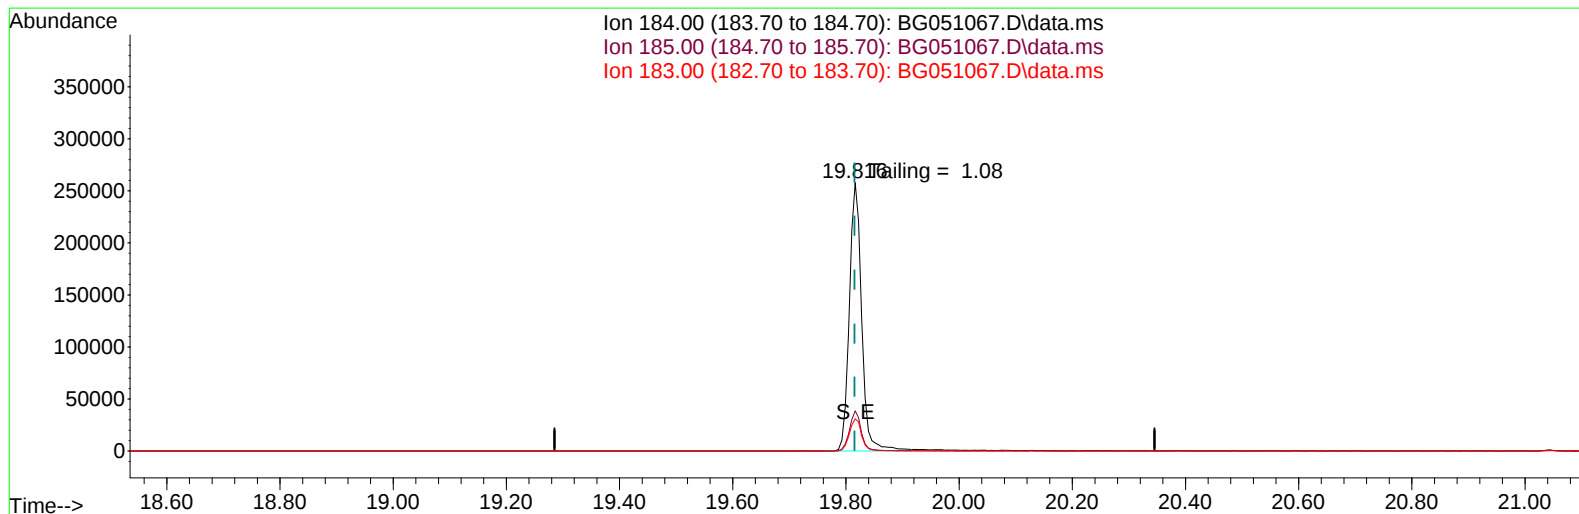

TIC: BG051067.D\data.ms

(77) Benzidine**19.816min (+ 0.001) 0.00 ng****response 391771**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.95
183.00	11.70	11.99
0.00	0.00	0.00