


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
 Data File : BG051059.D
 Acq On : 16 Nov 2021 9:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 03:55:35 2021

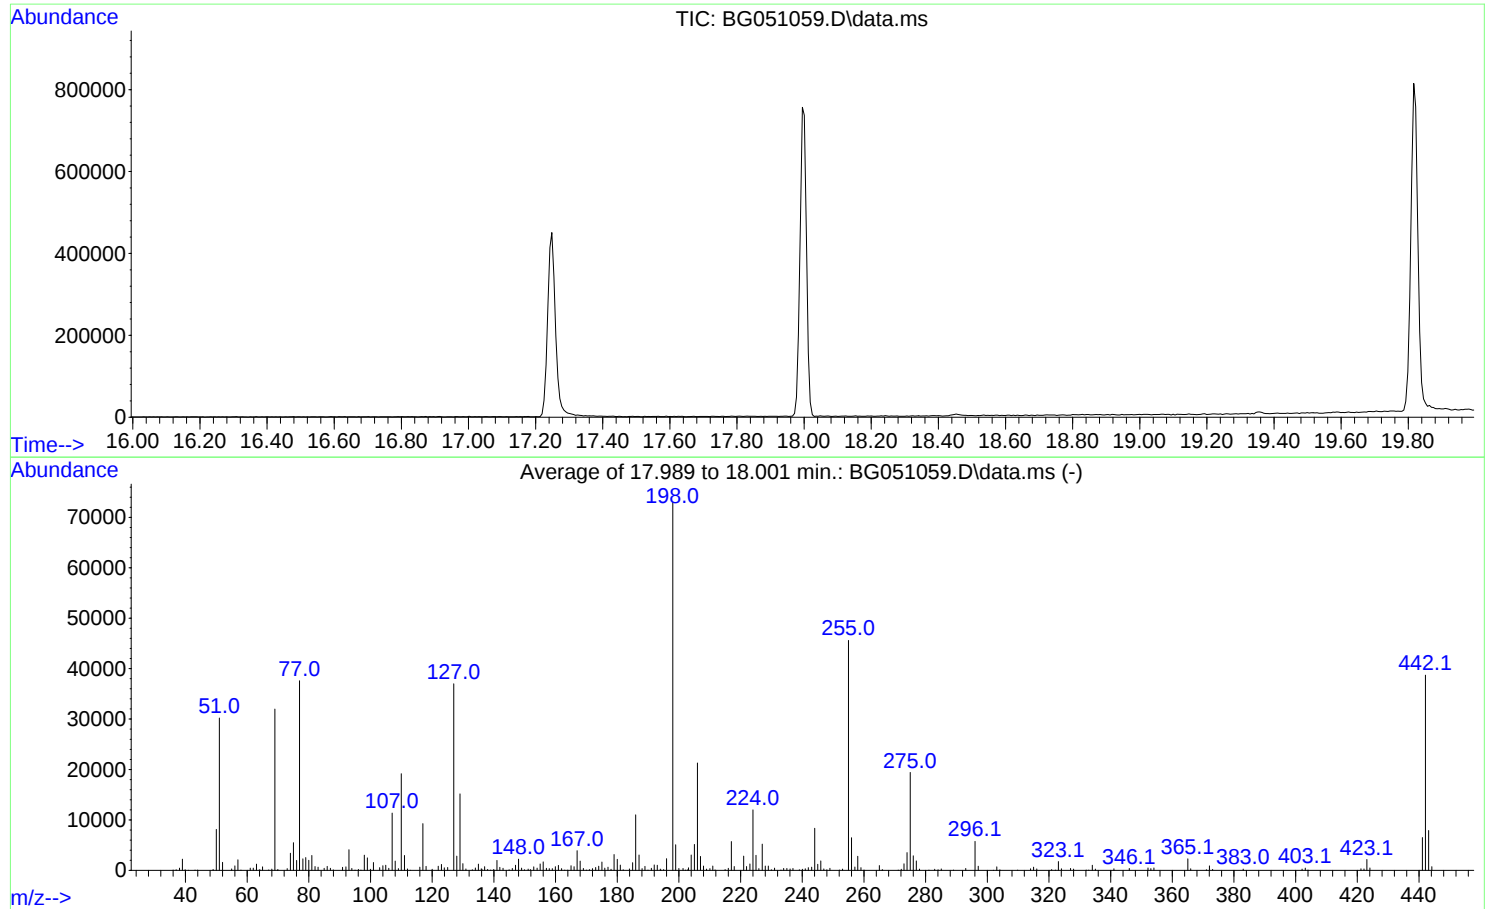




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	30211	PASS
68	69	0.00	2	0.8	259	PASS
69	198	0.00	100	43.8	31984	PASS
70	69	0.00	2	0.5	173	PASS
127	198	10	80	50.7	37008	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72944	PASS
199	198	5	9	7.0	5083	PASS
275	198	10	60	26.6	19408	PASS
365	198	1	100	3.1	2273	PASS
441	198	0.01	100	8.9	6509	PASS
442	442	50	100	100.0	38709	PASS
443	442	15	24	20.5	7917	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
Data File : BG051059.D
Acq On : 16 Nov 2021 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 16 10:09:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

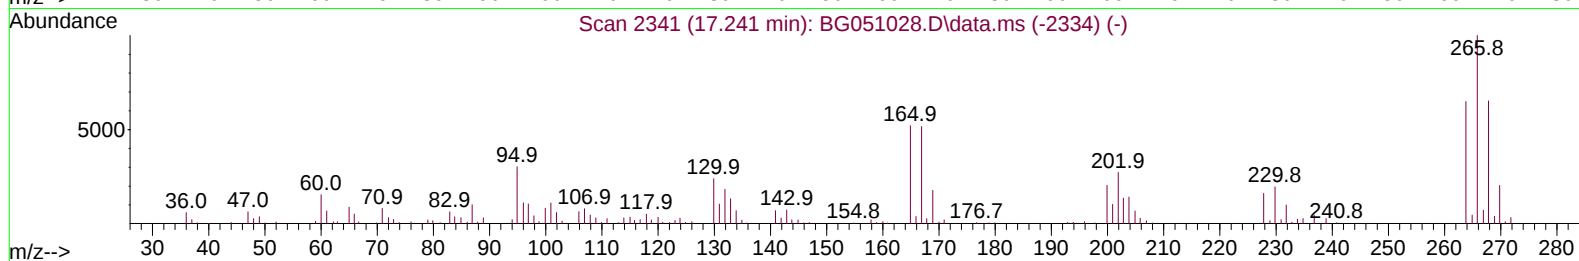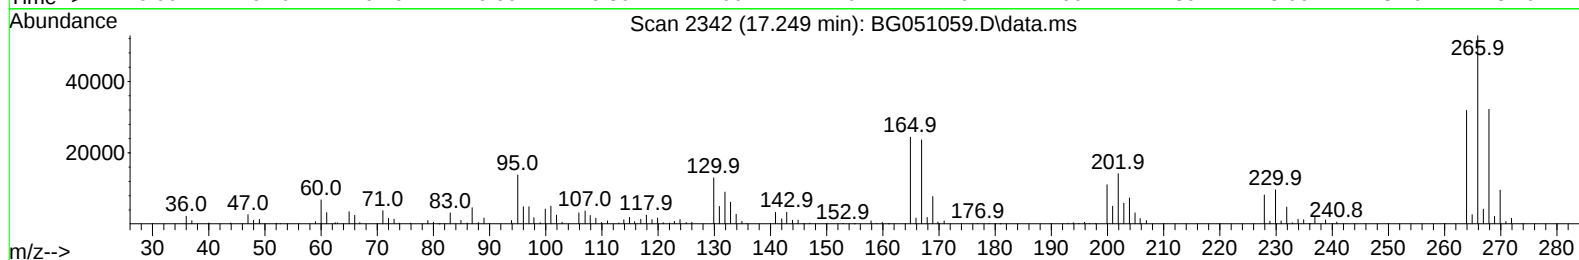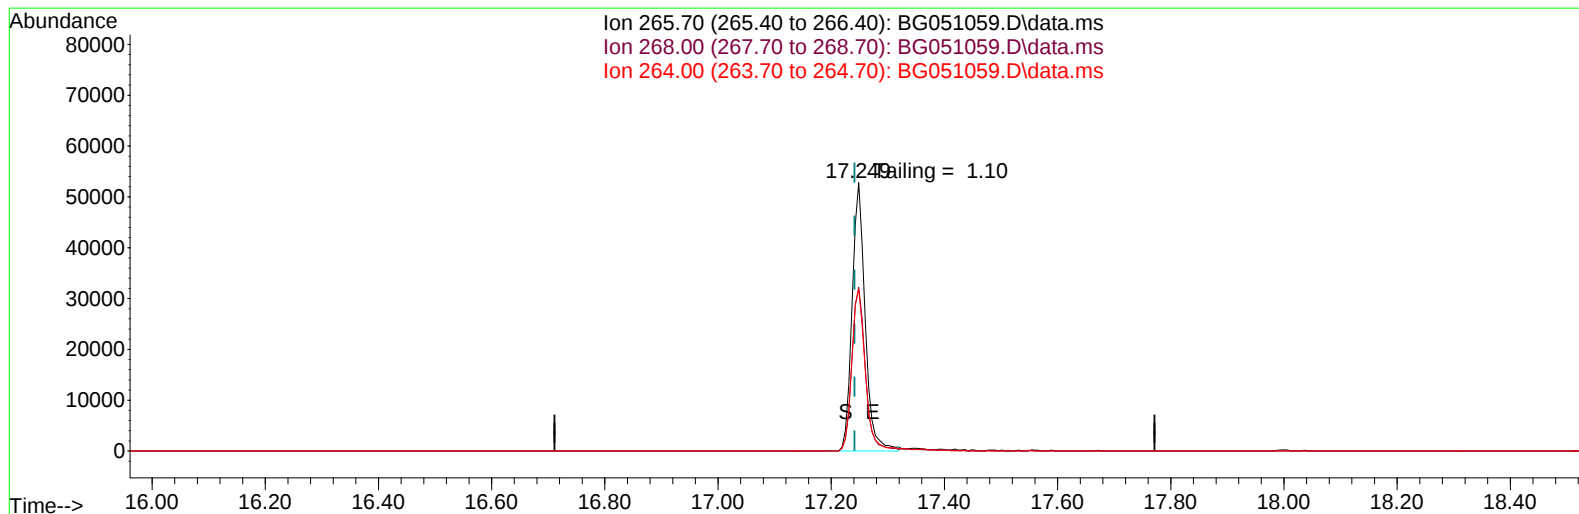

TIC: BG051059.D\data.ms

(70) Pentachlorophenol (C)

17.249min (+ 0.008) 33744.81 ng




response 84901

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.01
264.00	61.30	60.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
 Data File : BG051059.D
 Acq On : 16 Nov 2021 9:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 16 10:09:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 03:55:35 2021
 Response via : Initial Calibration

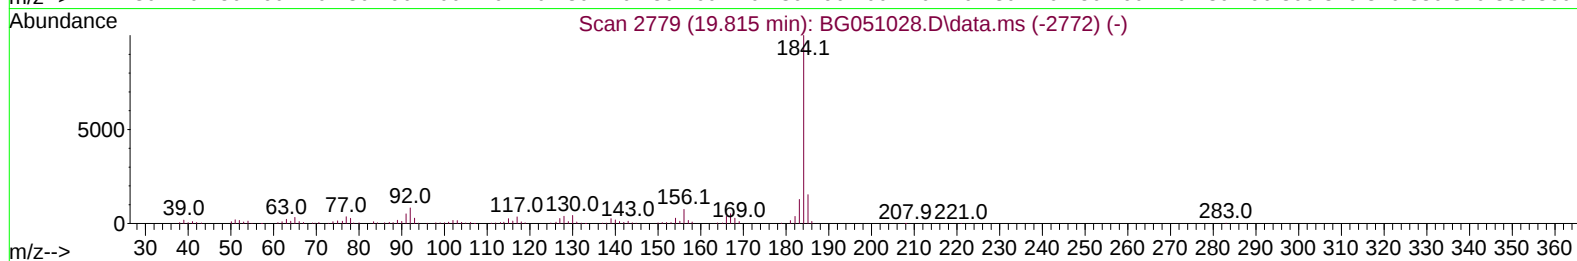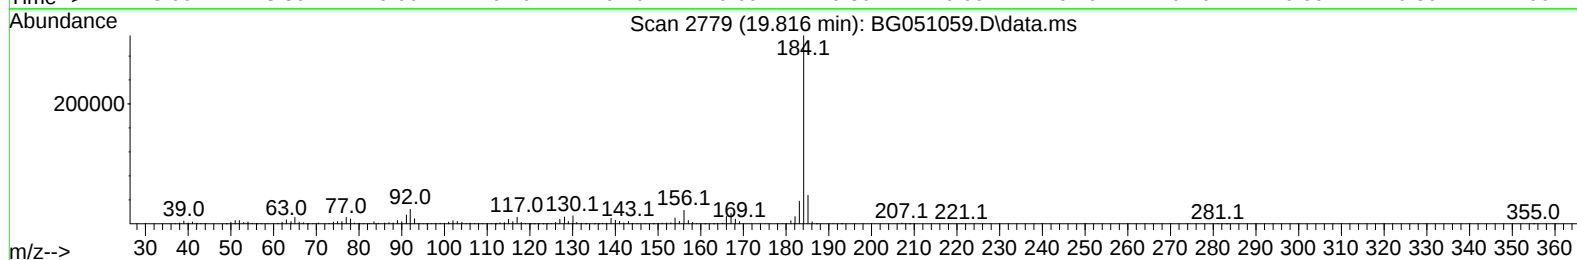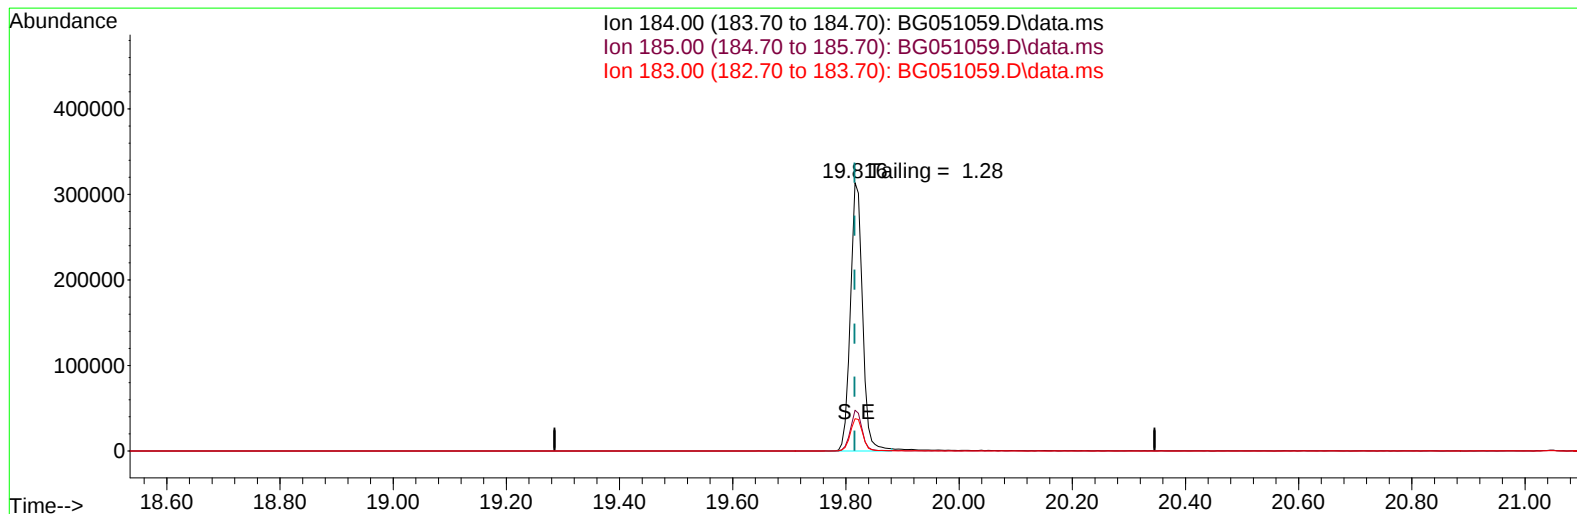

TIC: BG051059.D\data.ms

(77) Benzidine

19.816min (+ 0.001) 0.00 ng

response 473060

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.20
183.00	11.70	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/16/2021	BNA_G	BG051059.D
Compound Name	Response	Retention Time
DDT	222698	21.04
DDD	15654	20.59
DDE	0	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15654	238352	6.57