
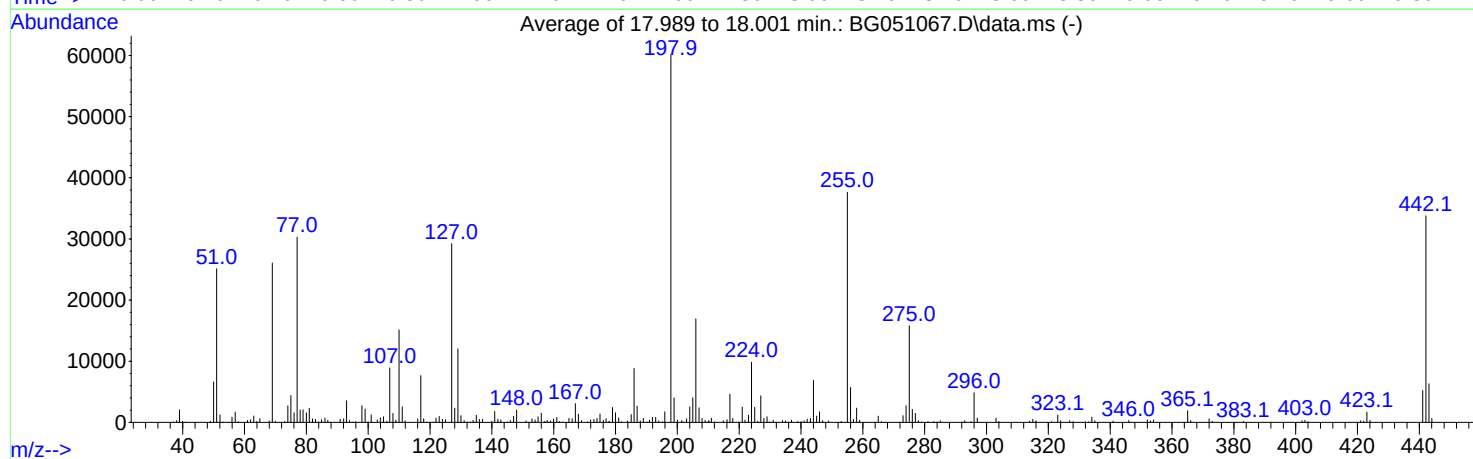


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
 Data File : BG051067.D
 Acq On : 16 Nov 2021 15:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 03:55:35 2021

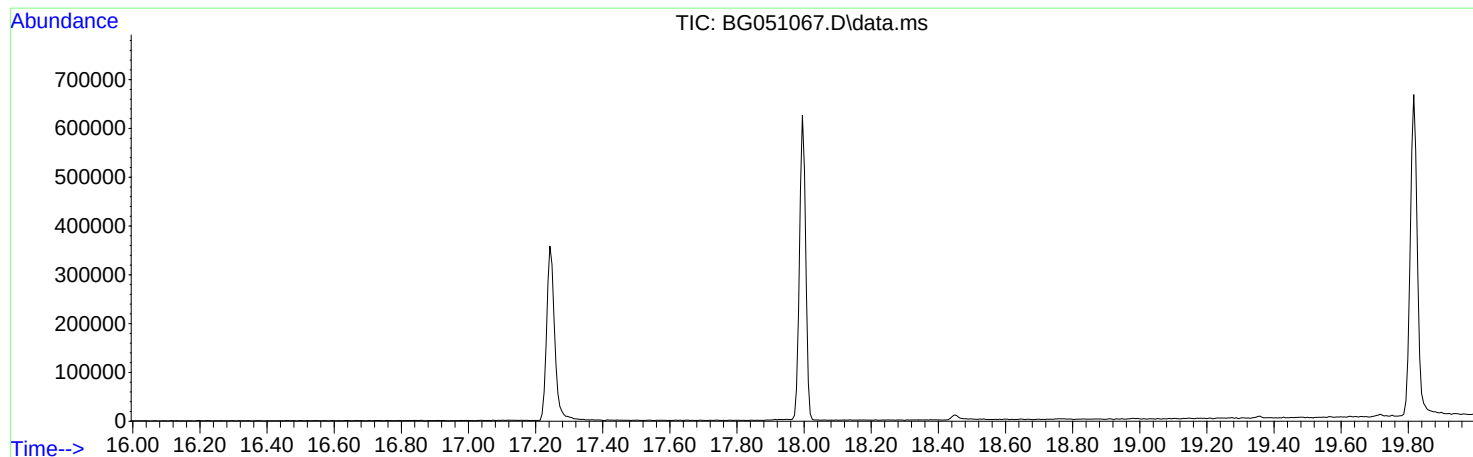




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	25123	PASS
68	69	0.00	2	0.9	233	PASS
69	198	0.00	100	43.3	26053	PASS
70	69	0.00	2	0.7	189	PASS
127	198	10	80	48.6	29235	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60160	PASS
199	198	5	9	6.7	4011	PASS
275	198	10	60	26.3	15811	PASS
365	198	1	100	3.2	1900	PASS
441	198	0.01	100	8.7	5206	PASS
442	442	50	100	100.0	33789	PASS
443	442	15	24	18.7	6308	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\  
Data File : BG051067.D  
Acq On    : 16 Nov 2021  15:04  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 16 15:59:10 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

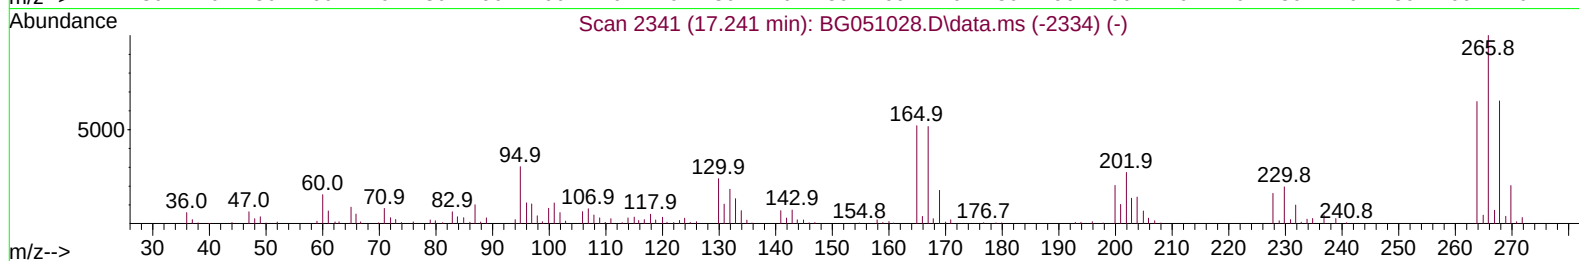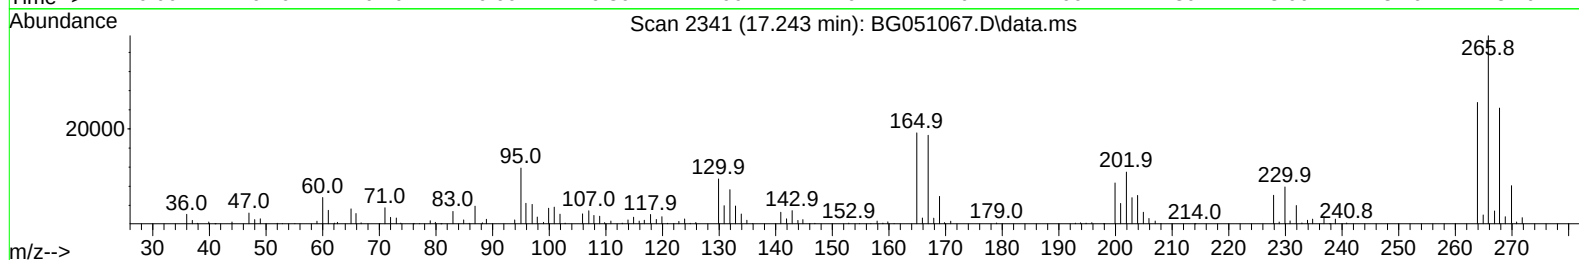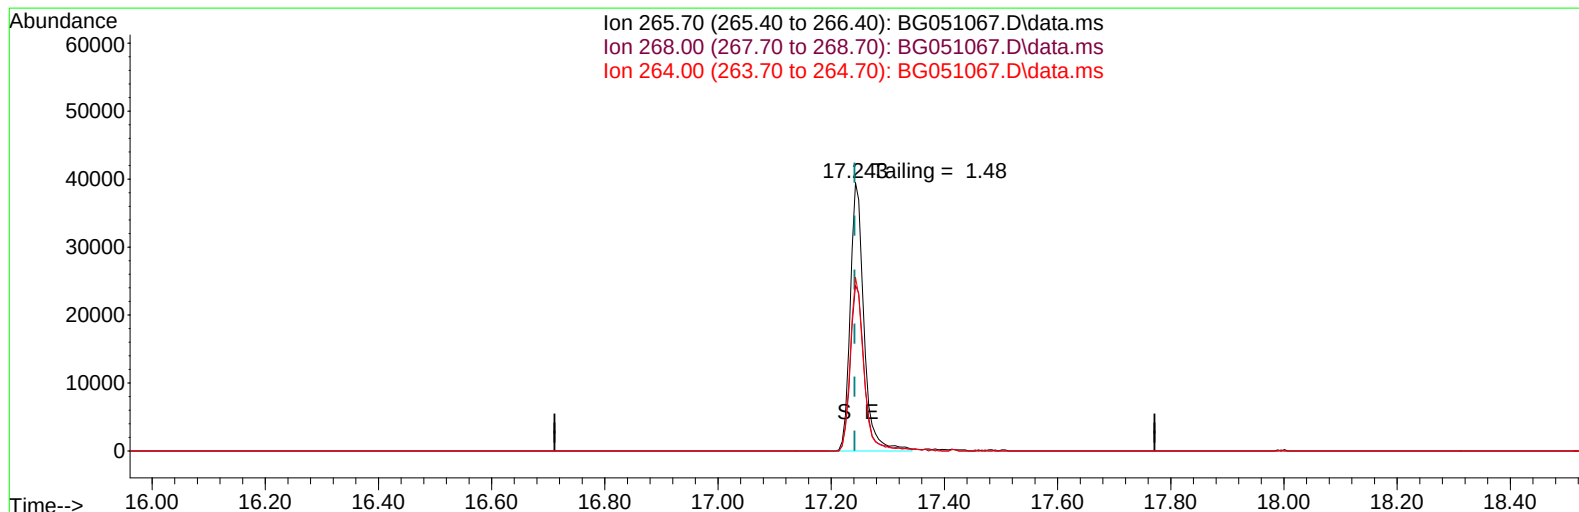

TIC: BG051067.D\data.ms

(70) Pentachlorophenol (C)

17.243min (+ 0.002) 44989.87 ng




response **66863**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.72
264.00	61.30	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111621\
 Data File : BG051067.D
 Acq On : 16 Nov 2021 15:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 16 15:59:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 03:55:35 2021
 Response via : Initial Calibration

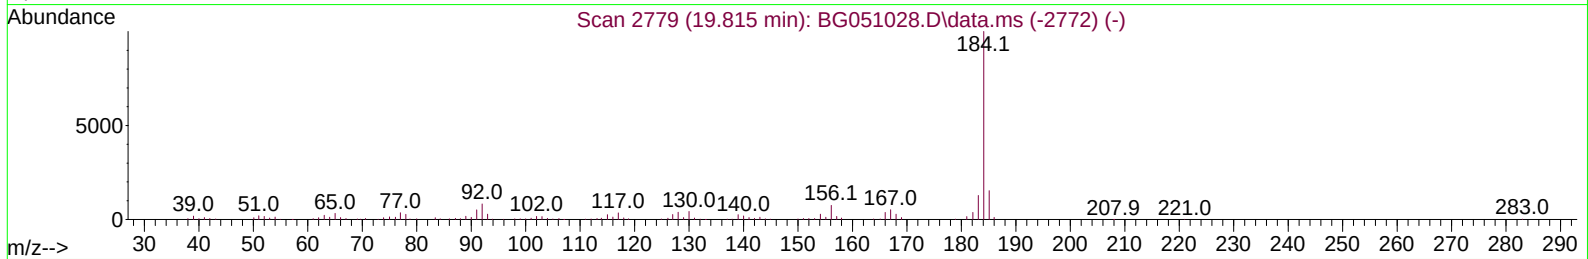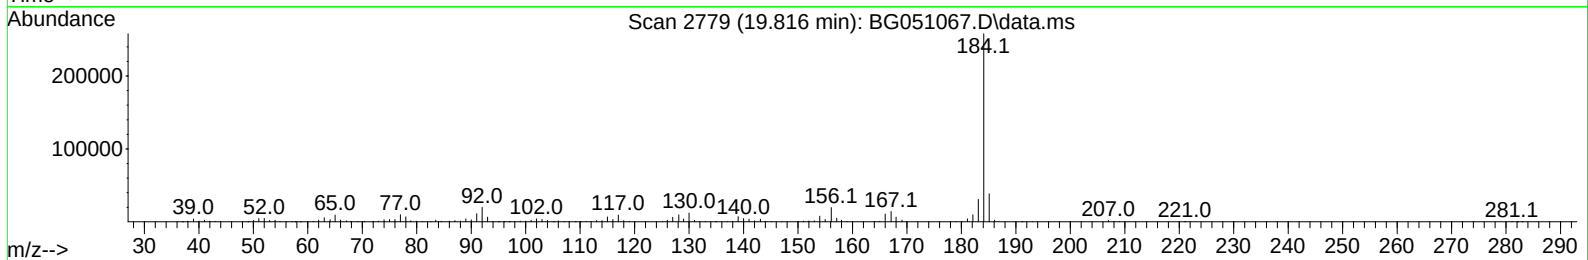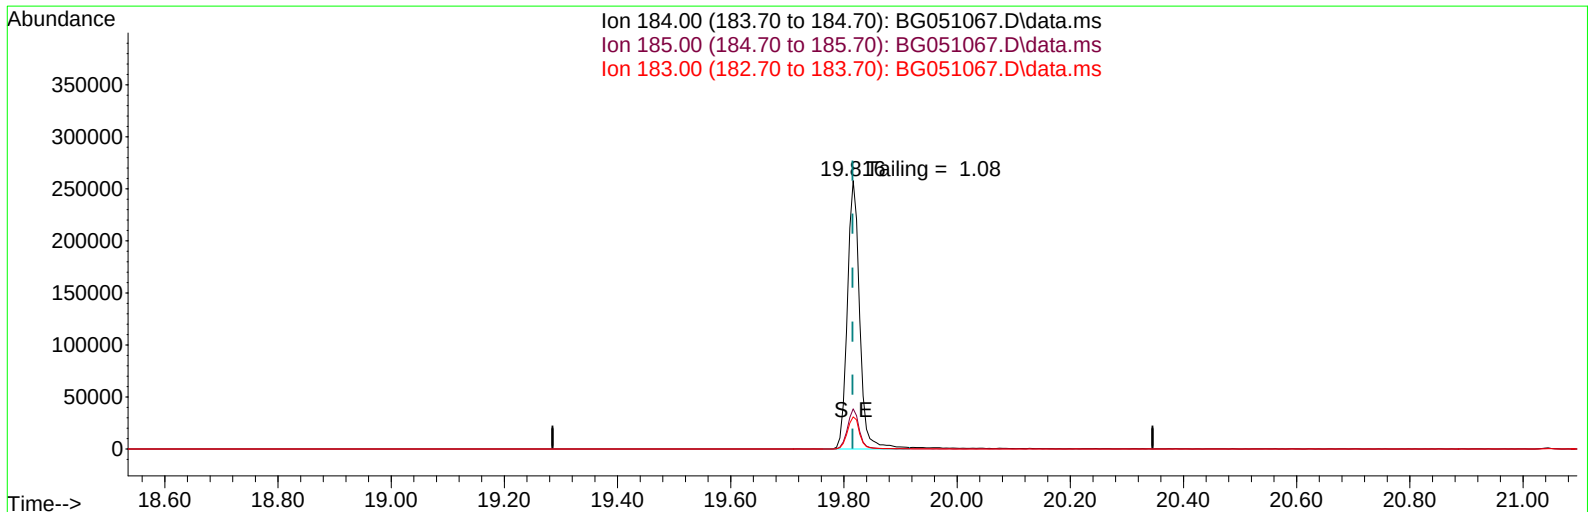

TIC: BG051067.D\data.ms

(77) Benzidine

19.816min (+ 0.001) 0.00 ng

response 391771

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.95
183.00	11.70	11.99
0.00	0.00	0.00

Instrument :
BNA_G
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/16/2021	BNA_G	BG051067.D
Compound Name	Response	Retention Time
DDT	192917	21.04
DDD	11025	20.59
DDE	0	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11025	203942	5.41