
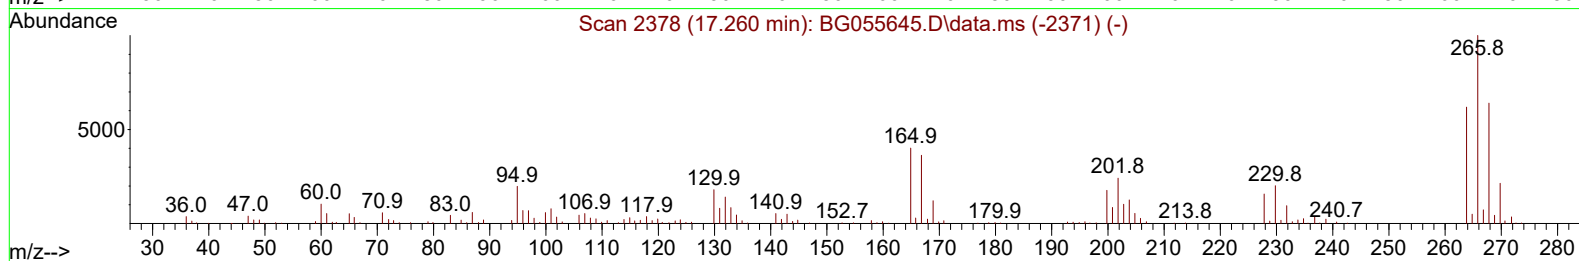
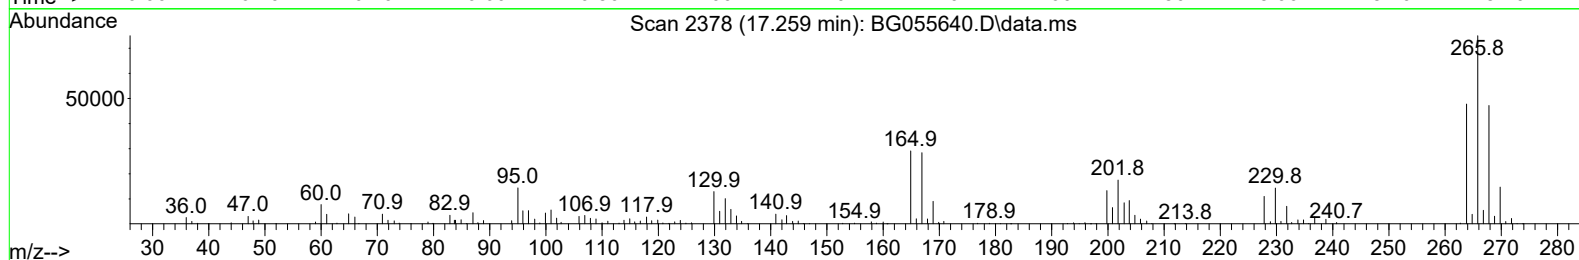


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111622\
 Data File : BG055640.D
 Acq On : 16 Nov 2022 9:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 16:19:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:17:44 2022
 Response via : Initial Calibration

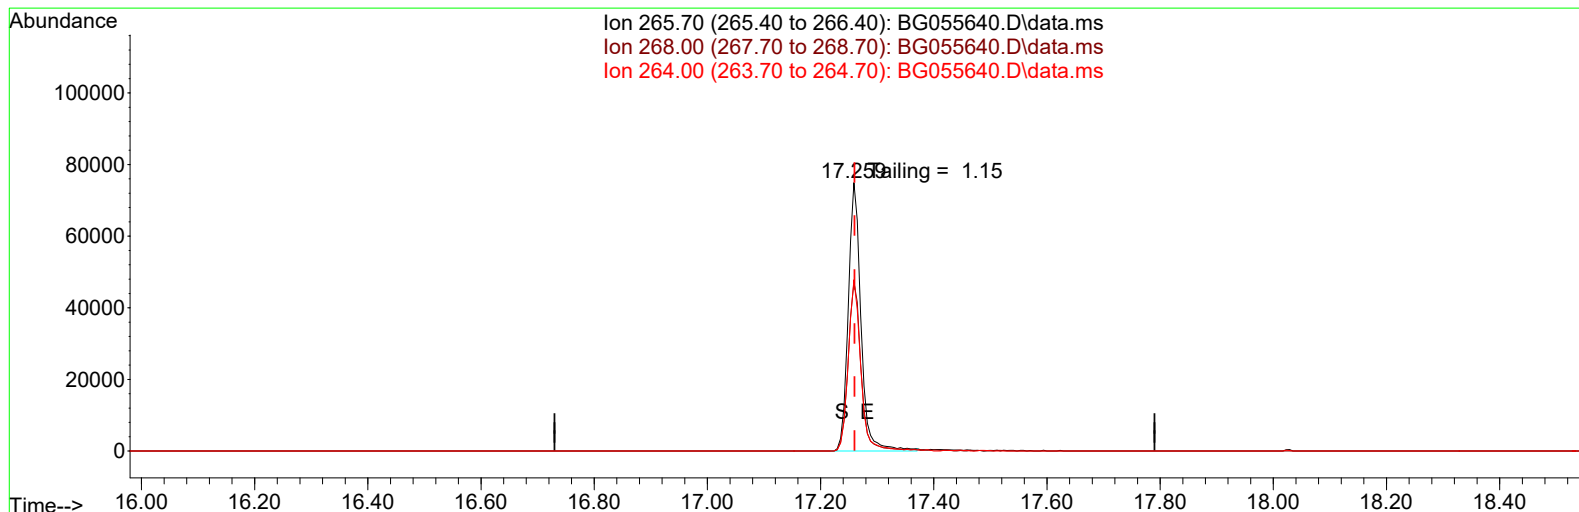

TIC: BG055640.D\data.ms

(70) Pentachlorophenol (C)




17.259min (-0.001) 139456.77 ng

response 117480

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.94
264.00	61.90	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111622\
 Data File : BG055640.D
 Acq On : 16 Nov 2022 9:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 16:19:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:17:44 2022
 Response via : Initial Calibration

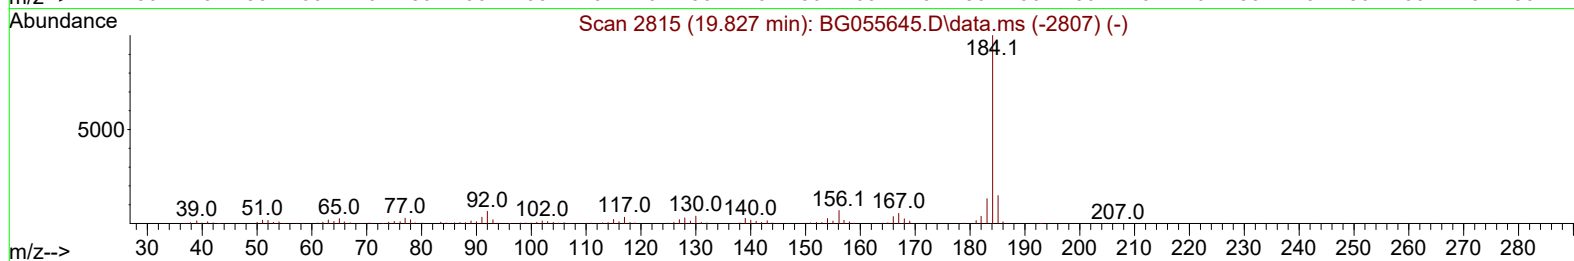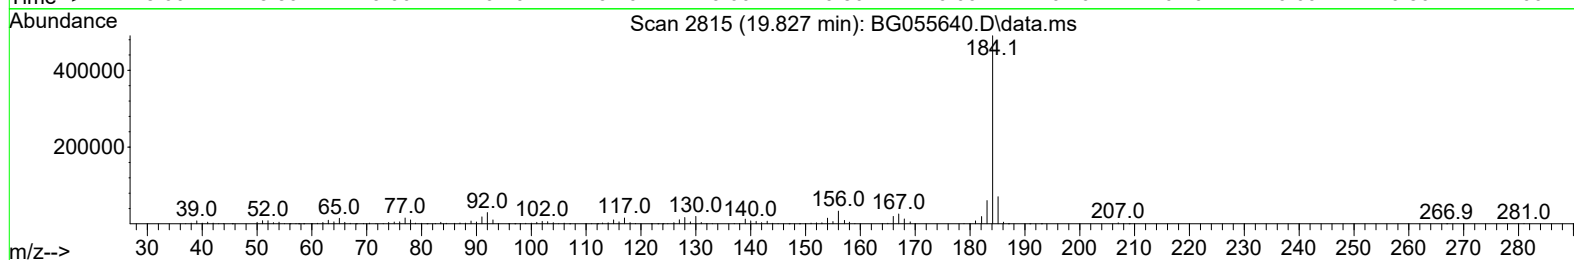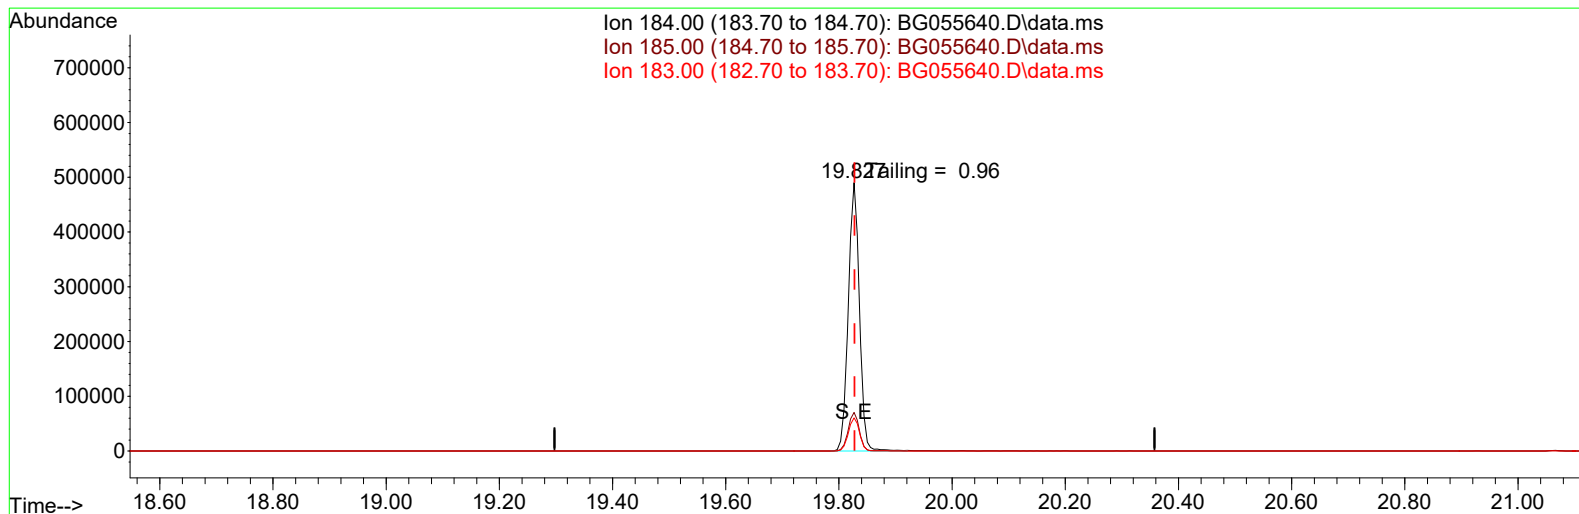

TIC: BG055640.D\data.ms

(77) Benzidine

19.827min (-0.001) 0.00 ng

response 668416

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.39
183.00	13.20	12.34
0.00	0.00	0.00