

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111622\
 Data File : BG055654.D
 Acq On : 16 Nov 2022 19:42
 Operator : CG/JU
 Sample : N5607-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-40A

Quant Time: Nov 17 02:13:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 02:02:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.253	152	43424	20.000	ng	0.00
21) Naphthalene-d8	11.079	136	190907	20.000	ng	0.00
39) Acenaphthene-d10	14.875	164	135200	20.000	ng	0.00
64) Phenanthrene-d10	17.613	188	298832	20.000	ng	0.00
76) Chrysene-d12	21.908	240	291870	20.000	ng	-0.01
86) Perylene-d12	25.321	264	306965	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.779	112	215489	89.697	ng	0.00
7) Phenol-d6	7.389	99	314533	98.353	ng	0.00
23) Nitrobenzene-d5	9.422	82	200661	55.555	ng	0.00
42) 2,4,6-Tribromophenol	16.355	330	156561	82.236	ng	0.00
45) 2-Fluorobiphenyl	13.500	172	497112	55.084	ng	0.00
79) Terphenyl-d14	20.198	244	771133	52.844	ng	0.00
Target Compounds						
84) Bis(2-ethylhexyl)phtha...	21.772	149	39728	3.574	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111622\
Data File : BG055654.D
Acq On : 16 Nov 2022 19:42
Operator : CG/JU
Sample : N5607-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-40A

Quant Time: Nov 17 02:13:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration




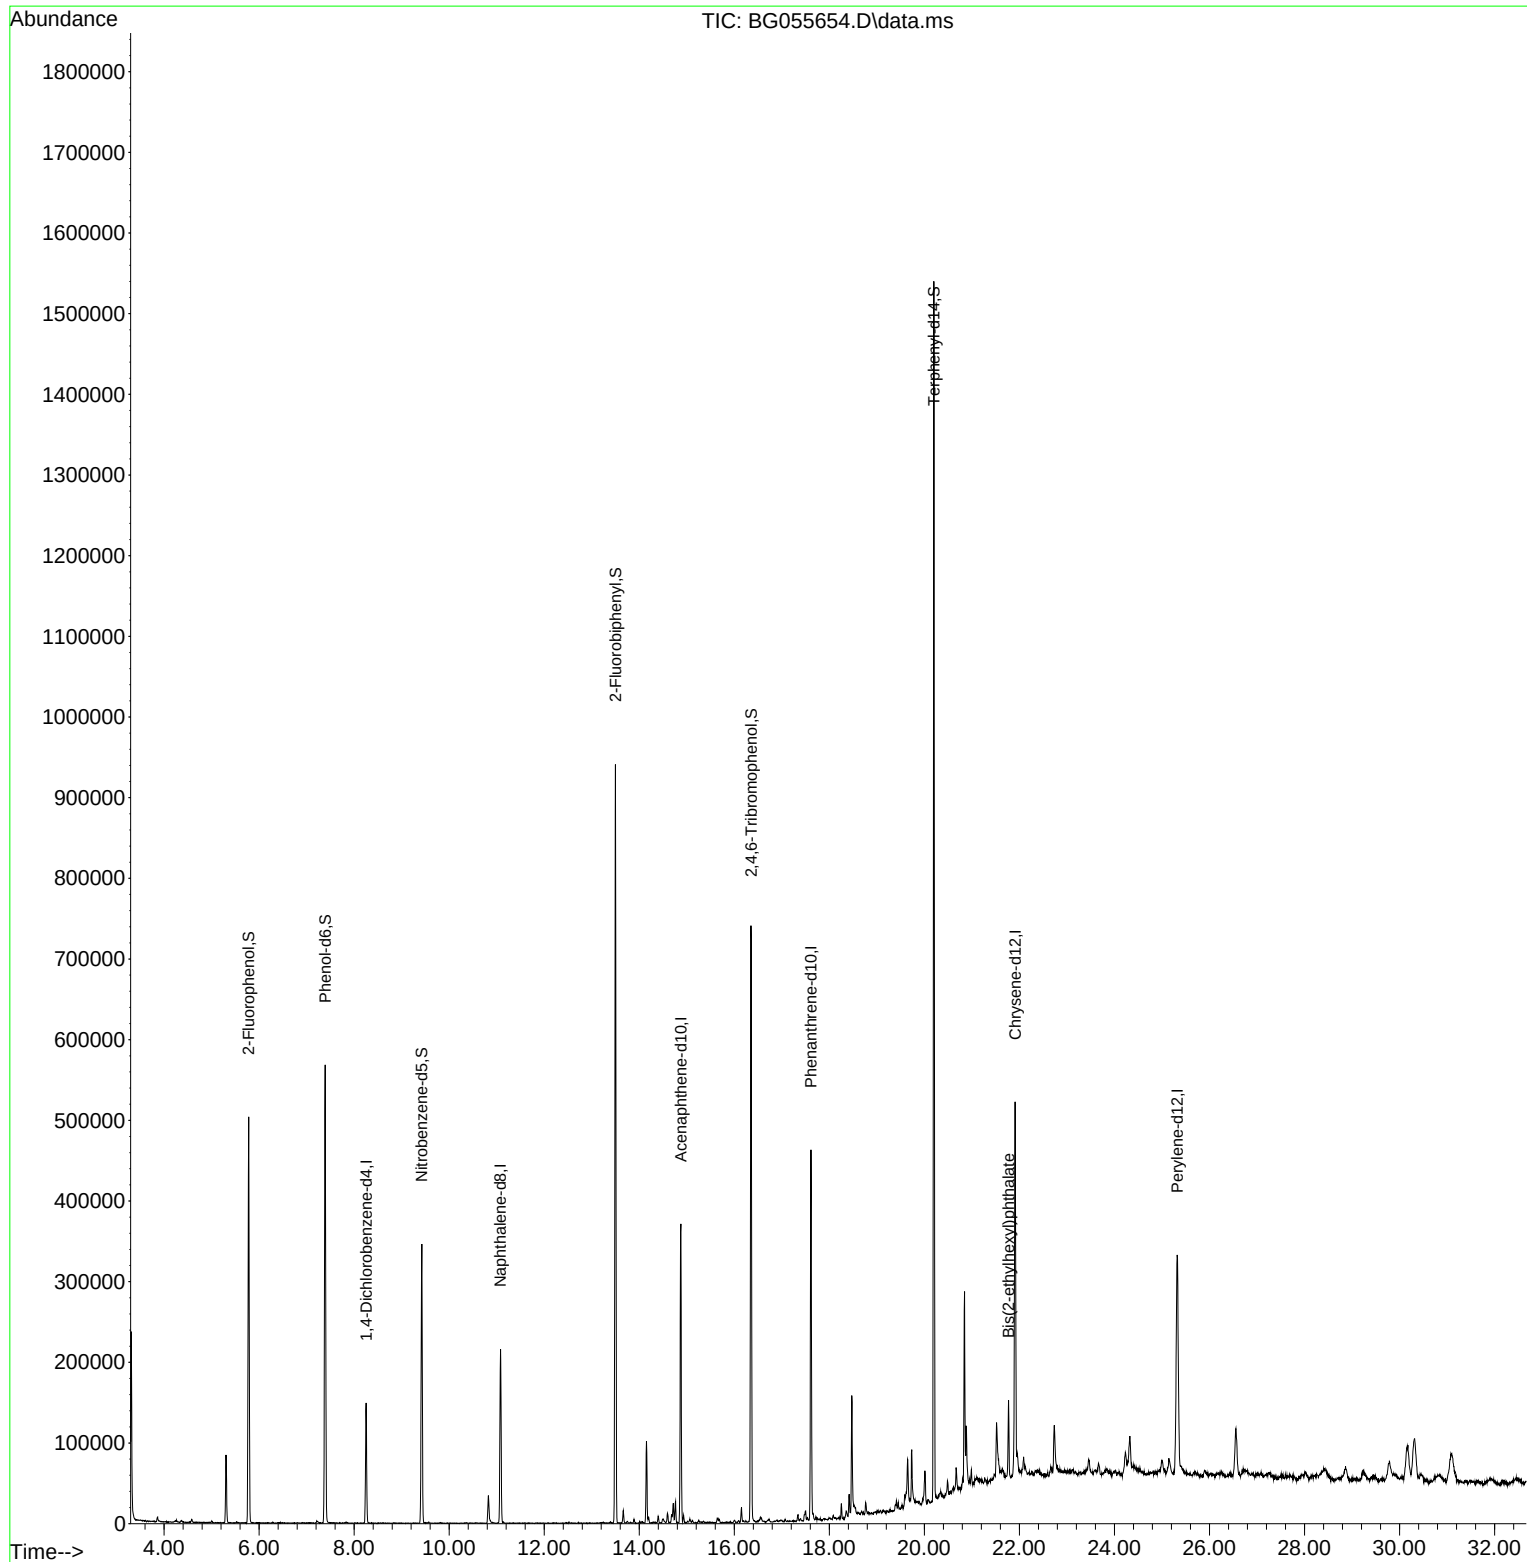


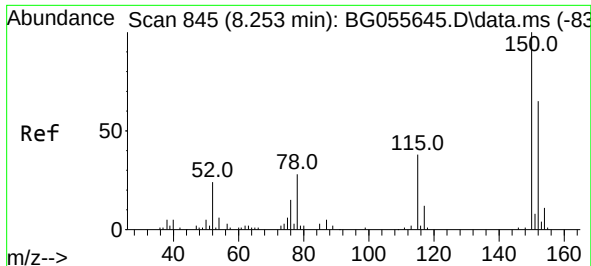

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.253 min Scan# 845
Delta R.T. -0.000 min
Lab File: BG055654.D
Acq: 16 Nov 2022 19:42




Instrument :
BNA_G
ClientSampleId :
SB-40A


Tgt Ion:152 Resp: 43424
Ion Ratio Lower Upper
152 100
150 152.0 123.0 184.6
115 58.1 47.0 70.4

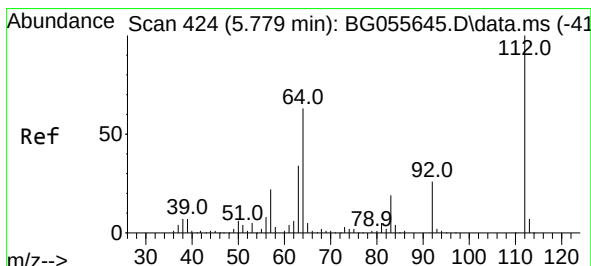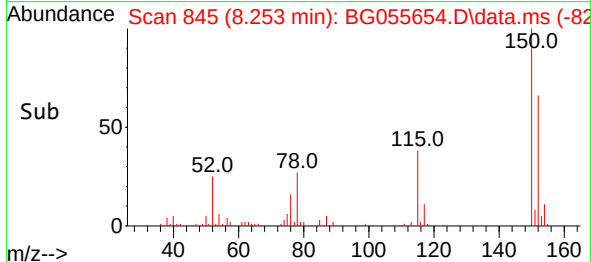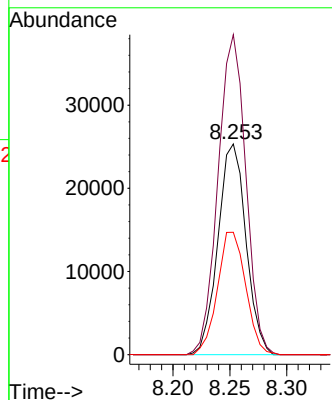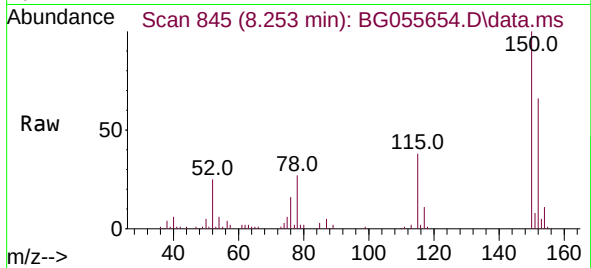

#5
2-Fluorophenol
Concen: 89.697 ng
RT: 5.779 min Scan# 424
Delta R.T. 0.000 min
Lab File: BG055654.D
Acq: 16 Nov 2022 19:42

Tgt Ion:112 Resp: 215489
Ion Ratio Lower Upper
112 100
64 64.6 50.6 76.0
63 35.7 27.5 41.3


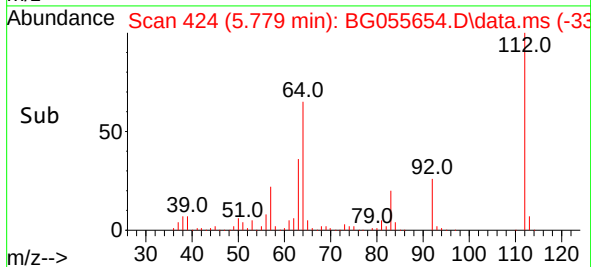
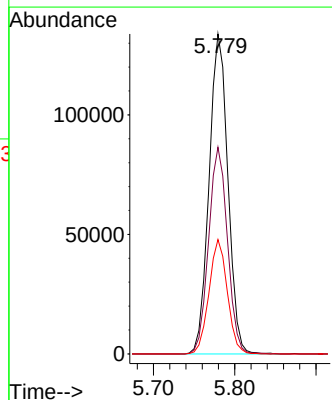
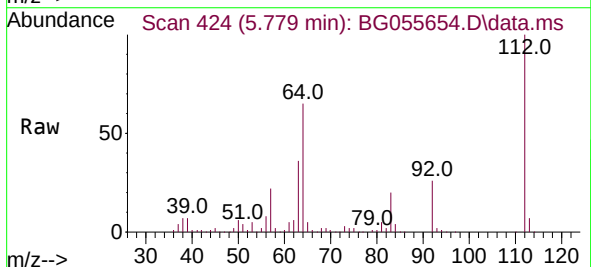


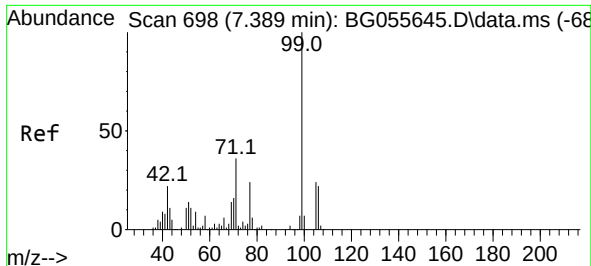

#7
Phenol-d6
Concen: 98.353 ng
RT: 7.389 min Scan# 698
Delta R.T. 0.000 min
Lab File: BG055654.D
Acq: 16 Nov 2022 19:42




Instrument :
BNA_G
ClientSampleId :
SB-40A


Tgt Ion: 99 Resp: 314533
Ion Ratio Lower Upper
99 100
42 22.0 18.0 27.0
71 35.4 29.0 43.6

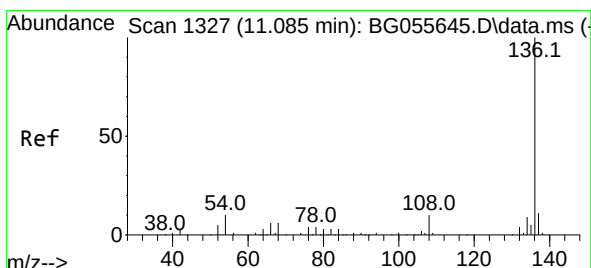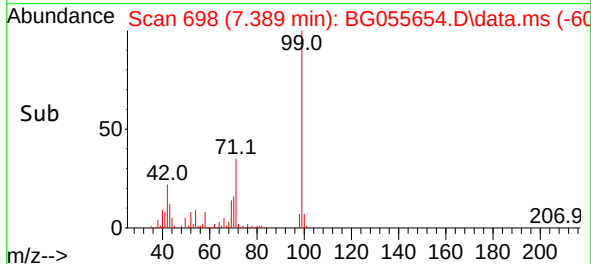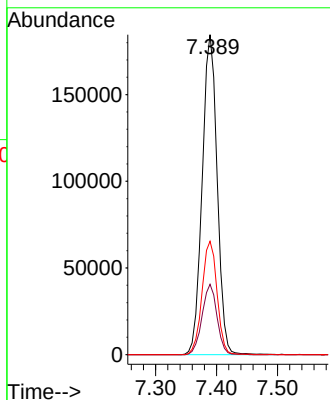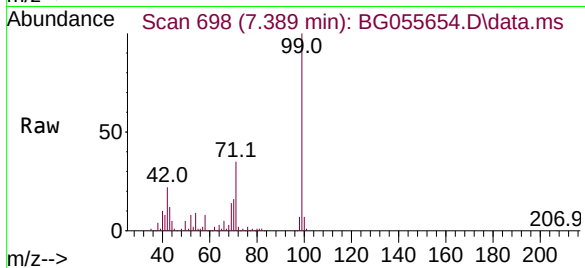

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.079 min Scan# 1326
Delta R.T. -0.006 min
Lab File: BG055654.D
Acq: 16 Nov 2022 19:42

Tgt Ion:136 Resp: 190907
Ion Ratio Lower Upper
136 100
137 11.0 9.0 13.6
54 9.8 7.8 11.6
68 6.0 5.0 7.4

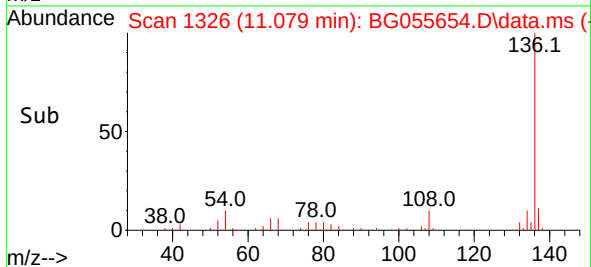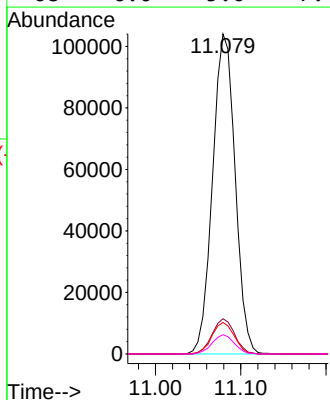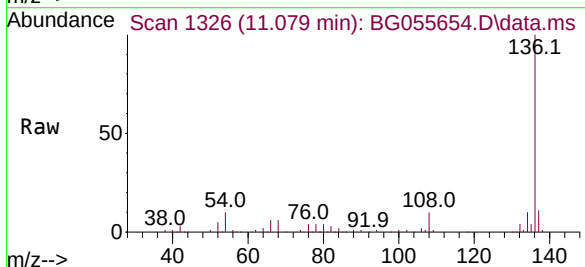

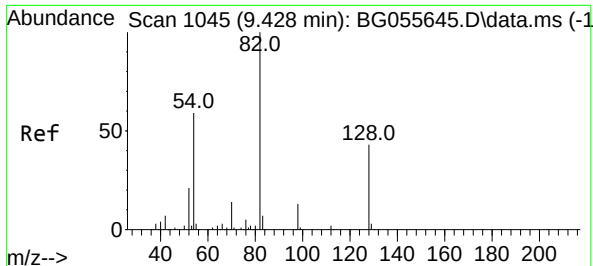

#23

Nitrobenzene-d5

Concen: 55.555 ng

RT: 9.422 min Scan# 1045

Delta R.T. -0.006 min

Lab File: BG055654.D

Acq: 16 Nov 2022 19:42

Instrument :

BNA_G

ClientSampleId :

SB-40A





Tgt Ion: 82 Resp: 200661

Ion Ratio Lower Upper

82 100

128 42.9 34.1 51.1

54 60.1 47.3 70.9

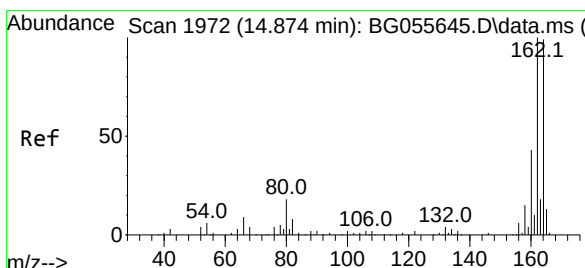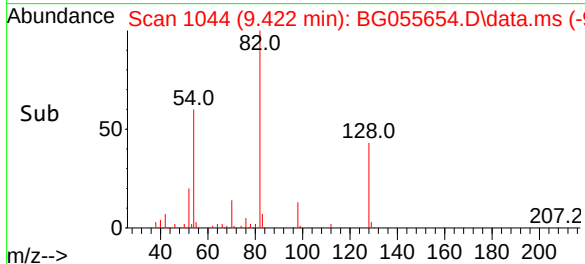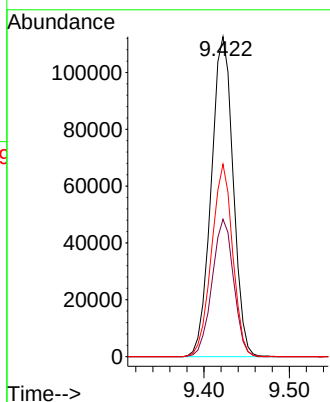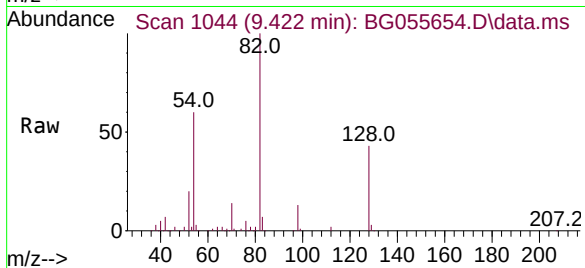

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.875 min Scan# 1972

Delta R.T. 0.000 min

Lab File: BG055654.D

Acq: 16 Nov 2022 19:42




Tgt Ion:164 Resp: 135200


Ion Ratio Lower Upper

164 100

162 102.1 81.1 121.7

160 44.4 34.8 52.2


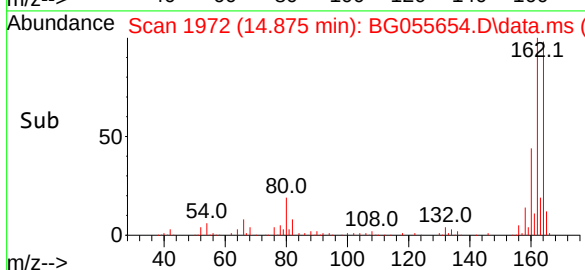
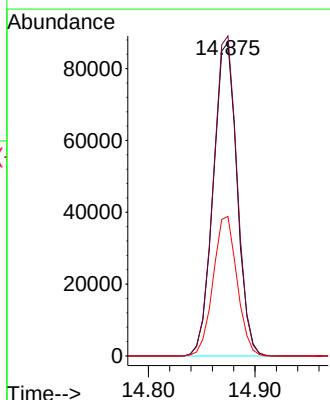
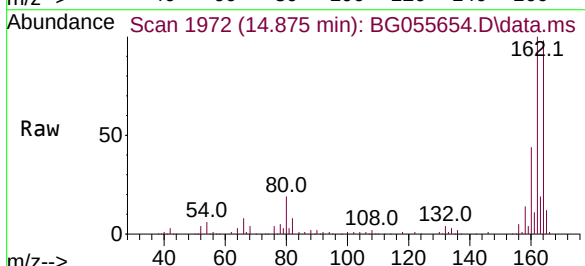


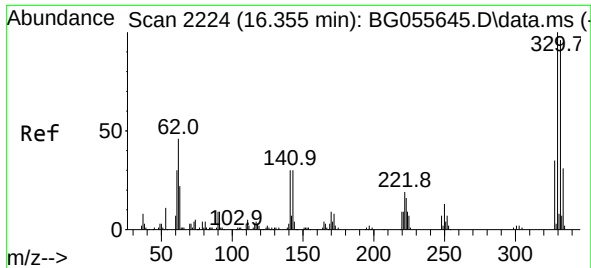

#42
 2,4,6-Tribromophenol
 Concen: 82.236 ng
 RT: 16.355 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BG055654.D
 Acq: 16 Nov 2022 19:42




Instrument :
 BNA_G
 ClientSampleId :
 SB-40A


Tgt Ion:330 Resp: 156561
 Ion Ratio Lower Upper
 330 100
 332 96.9 77.8 116.8
 141 29.9 23.9 35.9

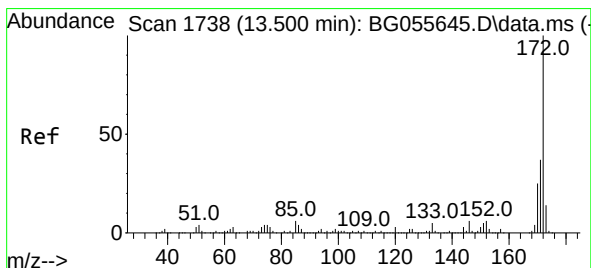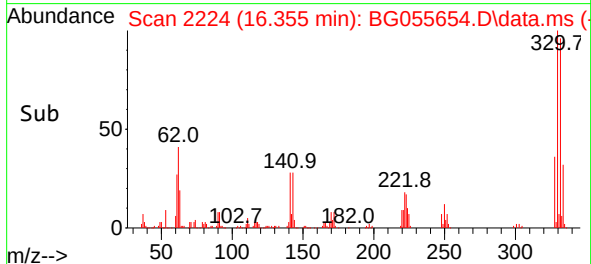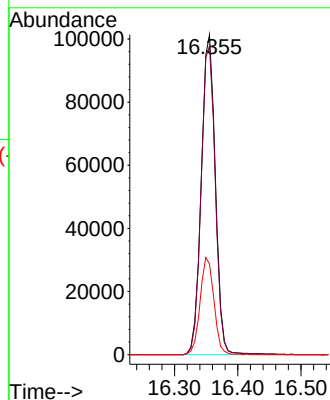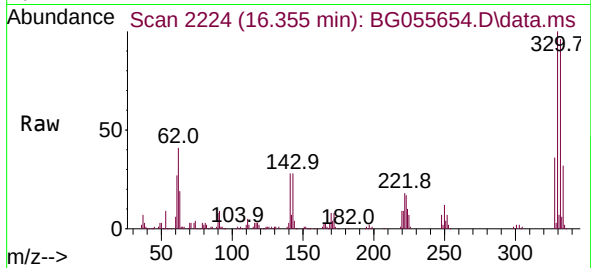

#45
 2-Fluorobiphenyl
 Concen: 55.084 ng
 RT: 13.500 min Scan# 1738
 Delta R.T. 0.000 min
 Lab File: BG055654.D
 Acq: 16 Nov 2022 19:42

Tgt Ion:172 Resp: 497112
 Ion Ratio Lower Upper
 172 100
 171 36.5 29.8 44.6
 170 25.3 20.2 30.4


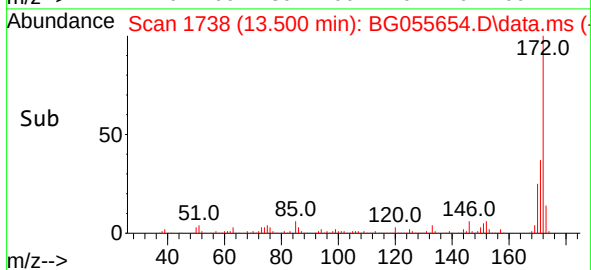
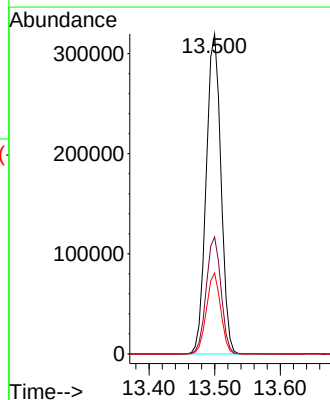
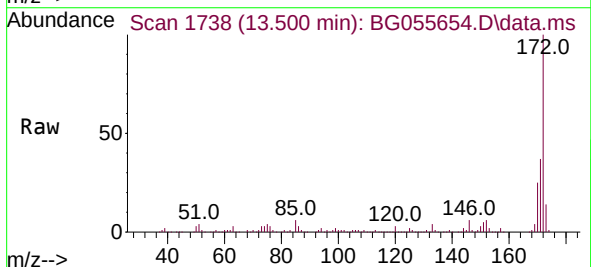


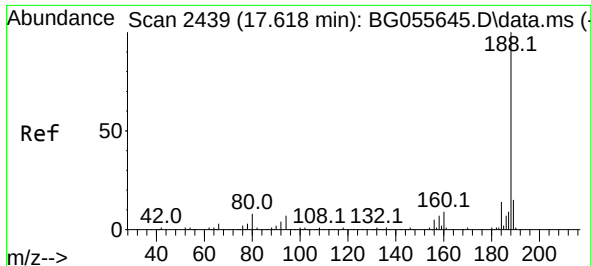

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.613 min Scan# 2438
Delta R.T. -0.006 min
Lab File: BG055654.D
Acq: 16 Nov 2022 19:42




Instrument :
BNA_G
ClientSampleId :
SB-40A


Tgt Ion:188 Resp: 298832
Ion Ratio Lower Upper
188 100
94 7.3 5.4 8.2
80 8.6 6.6 10.0

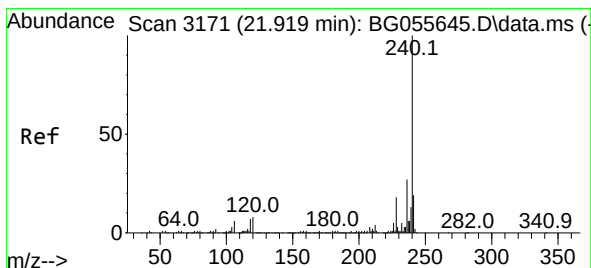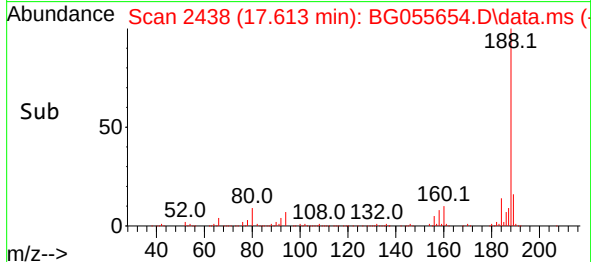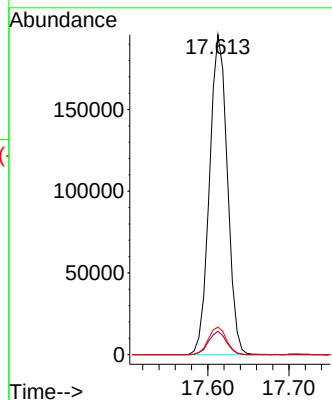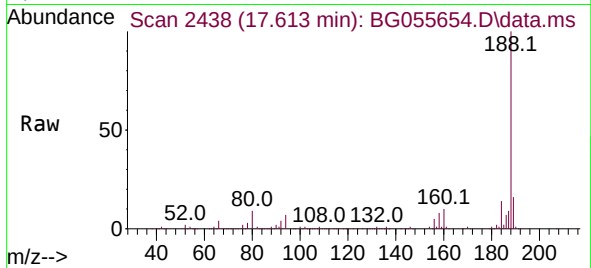

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.908 min Scan# 3169
Delta R.T. -0.011 min
Lab File: BG055654.D
Acq: 16 Nov 2022 19:42

Tgt Ion:240 Resp: 291870
Ion Ratio Lower Upper
240 100
120 8.0 6.3 9.5
236 26.9 21.9 32.9


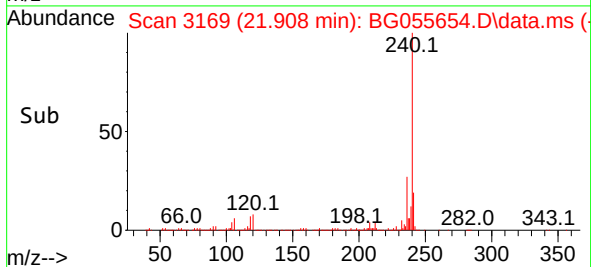
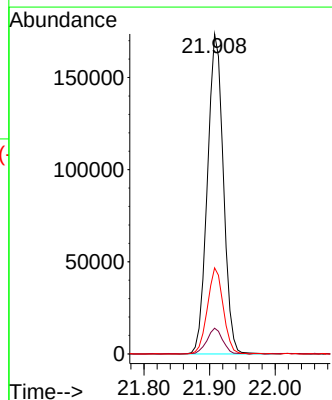
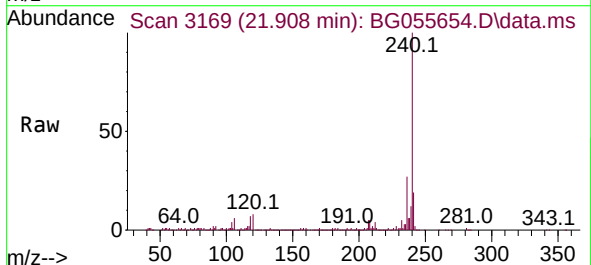


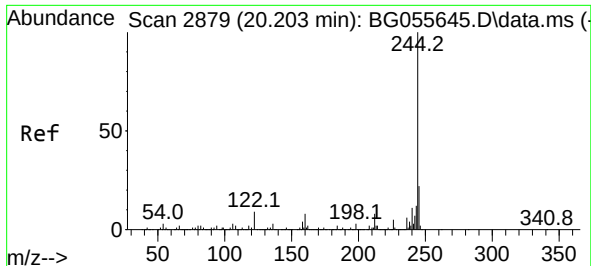

#79
 Terphenyl-d14
 Concen: 52.844 ng
 RT: 20.198 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BG055654.D
 Acq: 16 Nov 2022 19:42




Instrument :
 BNA_G
 ClientSampleId :
 SB-40A


Tgt Ion:244 Resp: 771133
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.3 9.5
 122 8.9 6.9 10.3

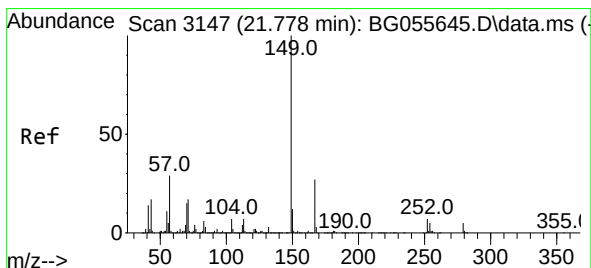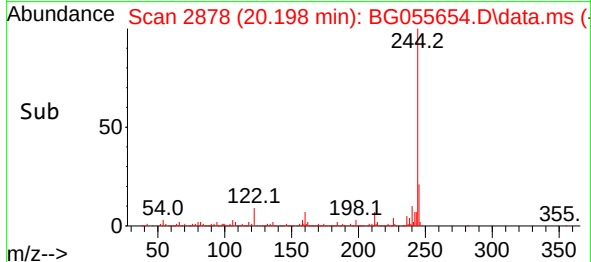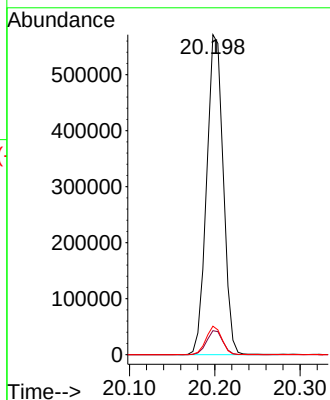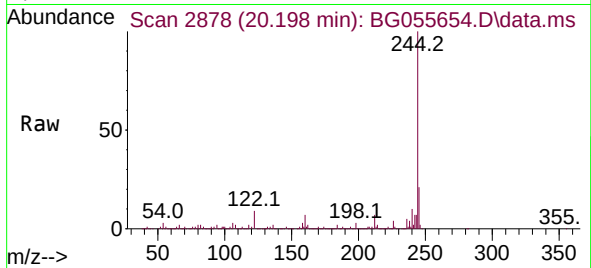

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 3.574 ng
 RT: 21.772 min Scan# 3146
 Delta R.T. -0.006 min
 Lab File: BG055654.D
 Acq: 16 Nov 2022 19:42

Tgt Ion:149 Resp: 39728
 Ion Ratio Lower Upper
 149 100
 167 26.6 22.0 33.0
 279 4.5 3.7 5.5

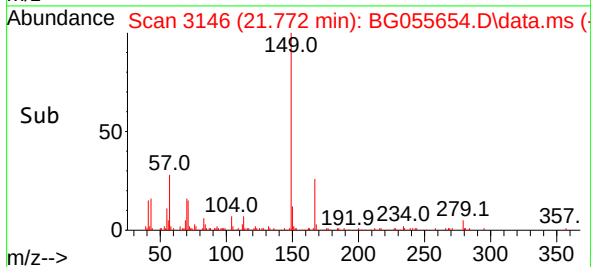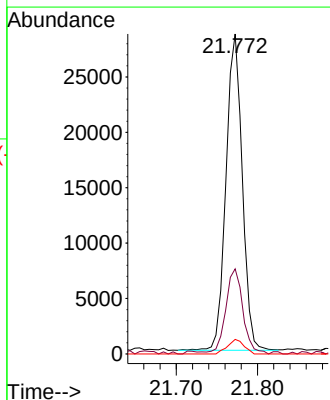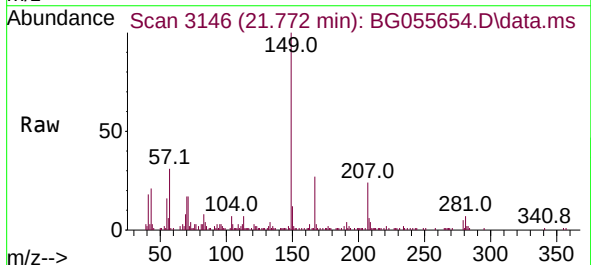

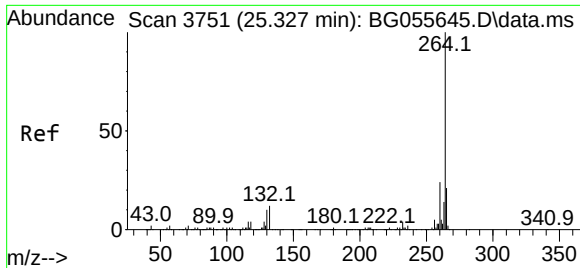

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.321 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BG055654.D
 Acq: 16 Nov 2022 19:42

Instrument :
 BNA_G
 ClientSampleId :
 SB-40A

Tgt Ion:264 Resp: 306965

Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.5	29.3
265	21.1	17.1	25.7

