
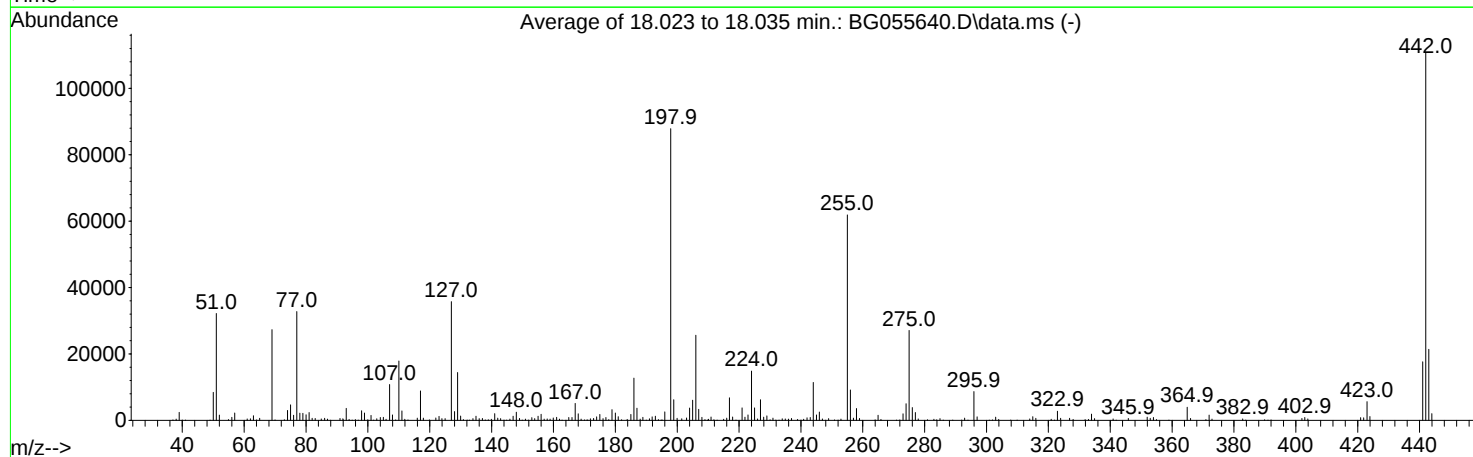


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111622\
 Data File : BG055640.D
 Acq On : 16 Nov 2022 9:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 17 02:02:46 2022

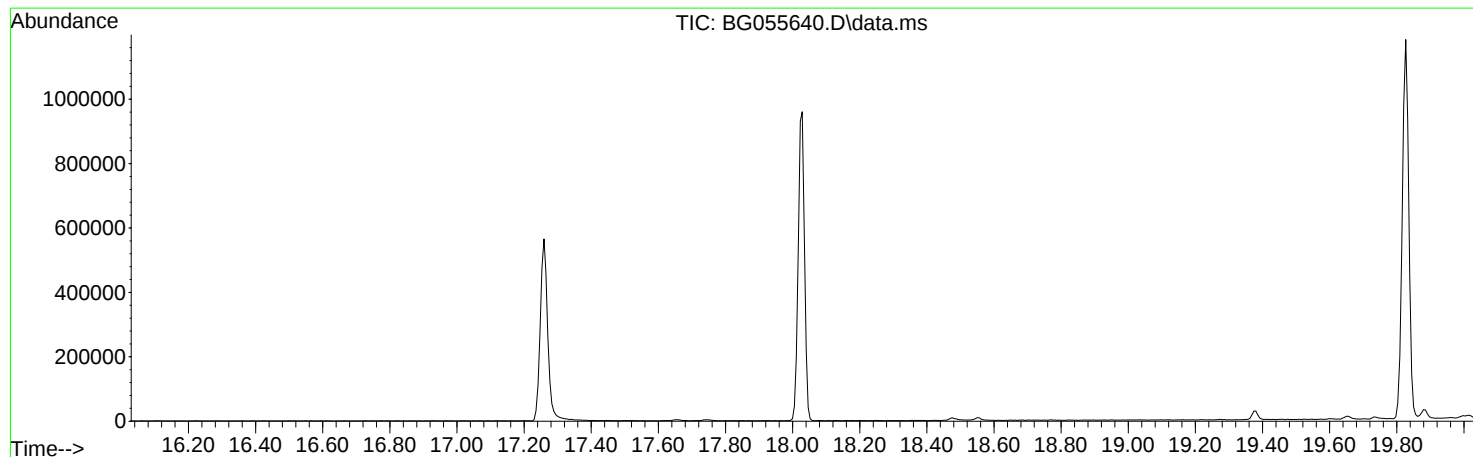




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	32181	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.1	27299	PASS
70	69	0.00	2	0.5	144	PASS
127	198	10	80	40.7	35736	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87840	PASS
199	198	5	9	7.1	6217	PASS
275	198	10	60	30.8	27072	PASS
365	198	1	100	4.5	3944	PASS
441	198	0.01	100	20.1	17617	PASS
442	442	50	100	100.0	110813	PASS
443	442	15	24	19.3	21365	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111622\
Data File : BG055640.D
Acq On : 16 Nov 2022 9:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 16 16:19:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 16:17:44 2022
Response via : Initial Calibration

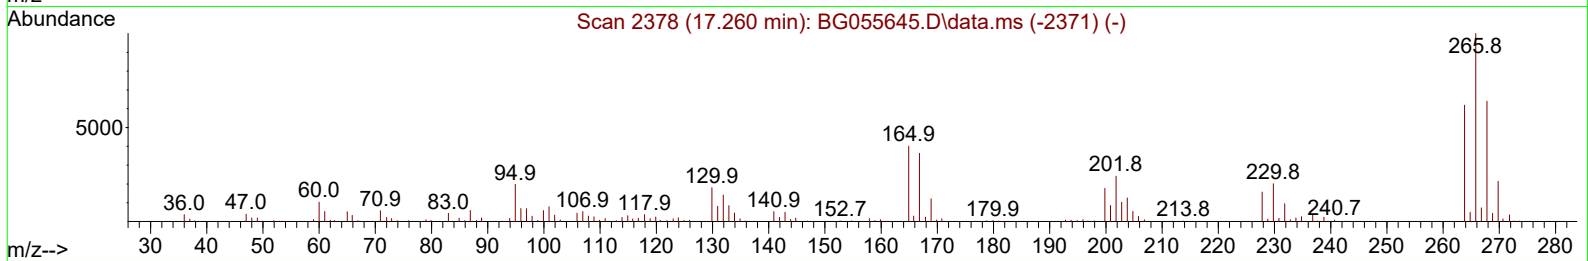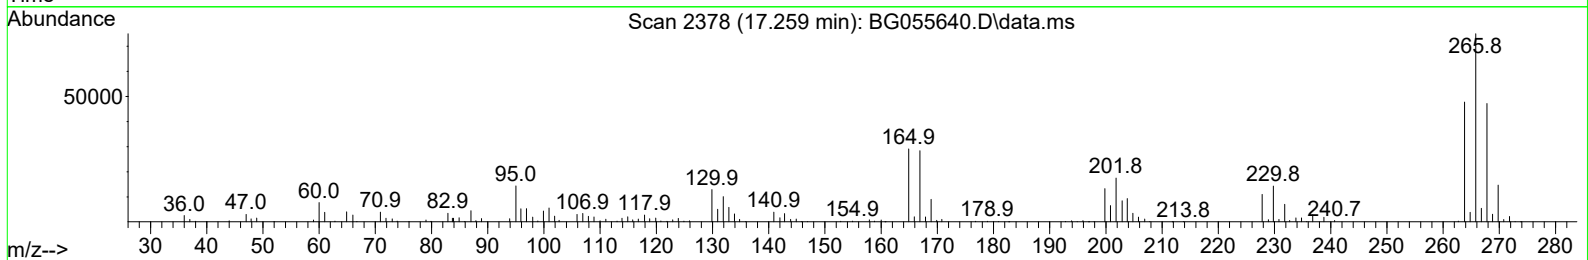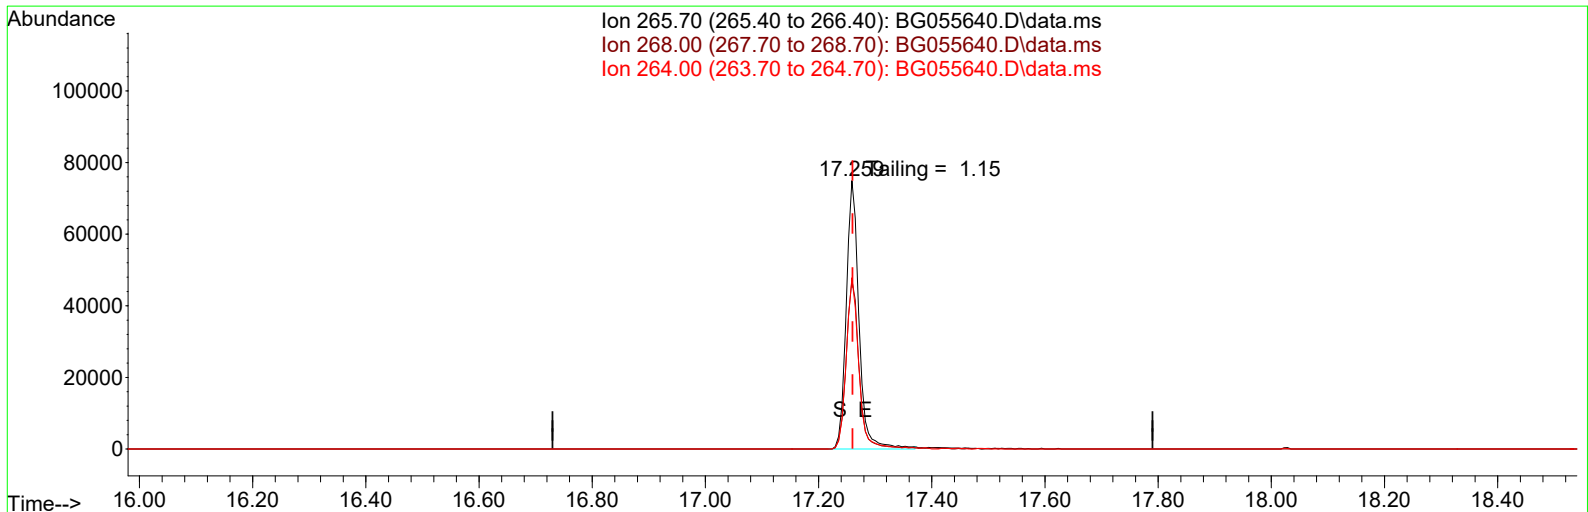

TIC: BG055640.D\data.ms

(70) Pentachlorophenol (C)

17.259min (-0.001) 139456.77 ng




response 117480

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.94
264.00	61.90	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111622\
 Data File : BG055640.D
 Acq On : 16 Nov 2022 9:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 16 16:19:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 16:17:44 2022
 Response via : Initial Calibration

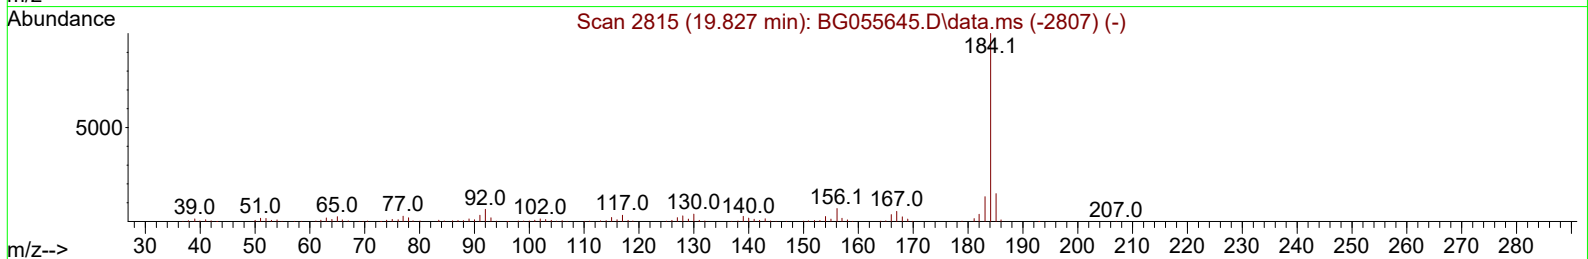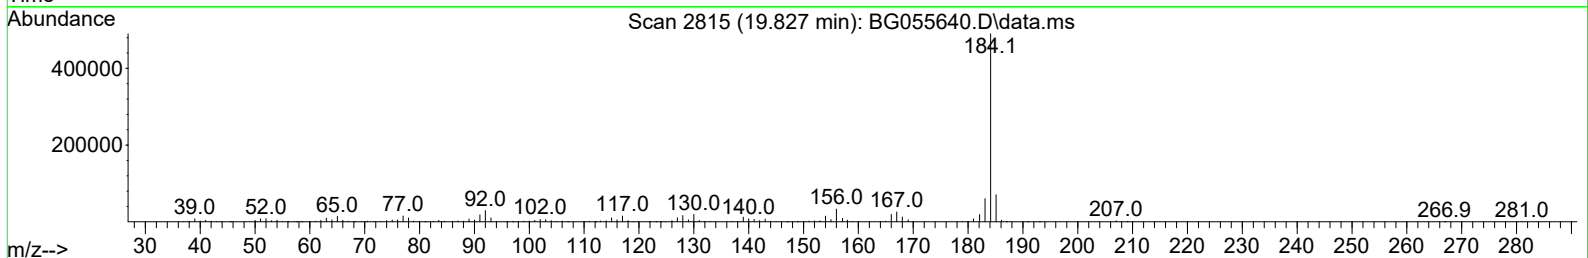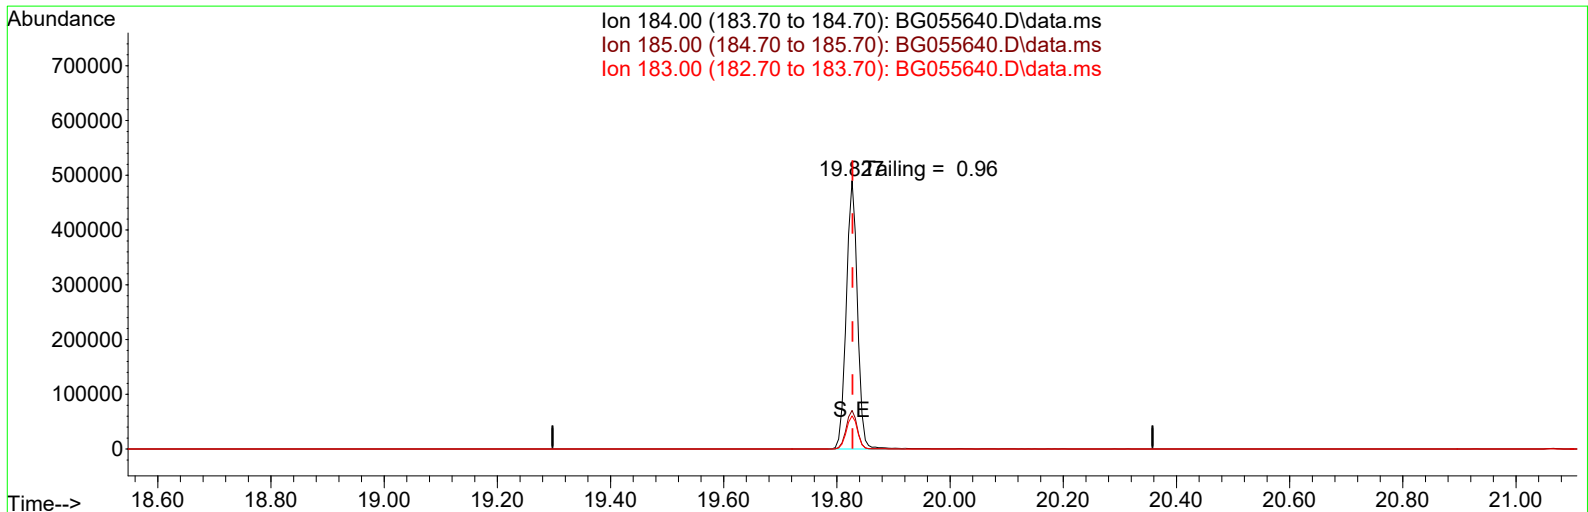

TIC: BG055640.D\data.ms

(77) Benzidine

19.827min (-0.001) 0.00 ng

response 668416

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.39
183.00	13.20	12.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/16/2022	BNA_G	BG055640.D
Compound Name	Response	Retention Time
DDT	312243	21.066
DDD	7911	20.608
DDE	409	20.114
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8320	320563	2.60

Instrument :
BNA_G
ClientSampleId :
DFTPP