

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111715\
 Data File : BG019665.D
 Acq On : 17 Nov 2015 18:28
 Operator : UM/NP
 Sample : PB86657BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK57

Quant Time: Nov 18 01:21:03 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 01:19:35 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	14770	20.00	ng/ul	0.00
18) Naphthalene-d8	10.97	136	64749	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.78	164	66505	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.52	188	224722	20.00	ng/ul	0.00
78) Chrysene-d12	21.79	240	310621	20.00	ng/ul	0.00
86) Perylene-d12	25.11	264	296714	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	2562	7.41	ng/uL	0.01
5) Phenol-d5	7.29	99	54989	36.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	39279	39.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.67	132	34787	35.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	46276	36.94	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	19672	37.00	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	24025	40.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	47032	36.35	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	59549	48.49	ng/ul	0.00
44) Dimethylphthalate-d6	14.18	166	203977	33.91	ng/ul	0.00
47) Acenaphthylene-d8	14.48	160	209294	32.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.96	143	32022	33.79	ng/ul	0.00
58) Fluorene-d10	15.77	176	182976	34.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.88	200	40313	27.77	ng/ul	0.00
71) Anthracene-d10	17.62	188	338847	31.06	ng/ul	0.00
79) Pyrene-d10	19.89	212	444181	31.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.88	264	499544	32.25	ng/ul	0.00


Target Compounds					Ovalue
15) N-Nitroso-di-n-propylamine	8.85	70	1560	1.12 ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111715\
Data File : BG019665.D
Acq On : 17 Nov 2015 18:28
Operator : UM/NP
Sample : PB86657BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK57

Quant Time: Nov 18 01:21:03 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 18 01:19:35 2015
Response via : Initial Calibration

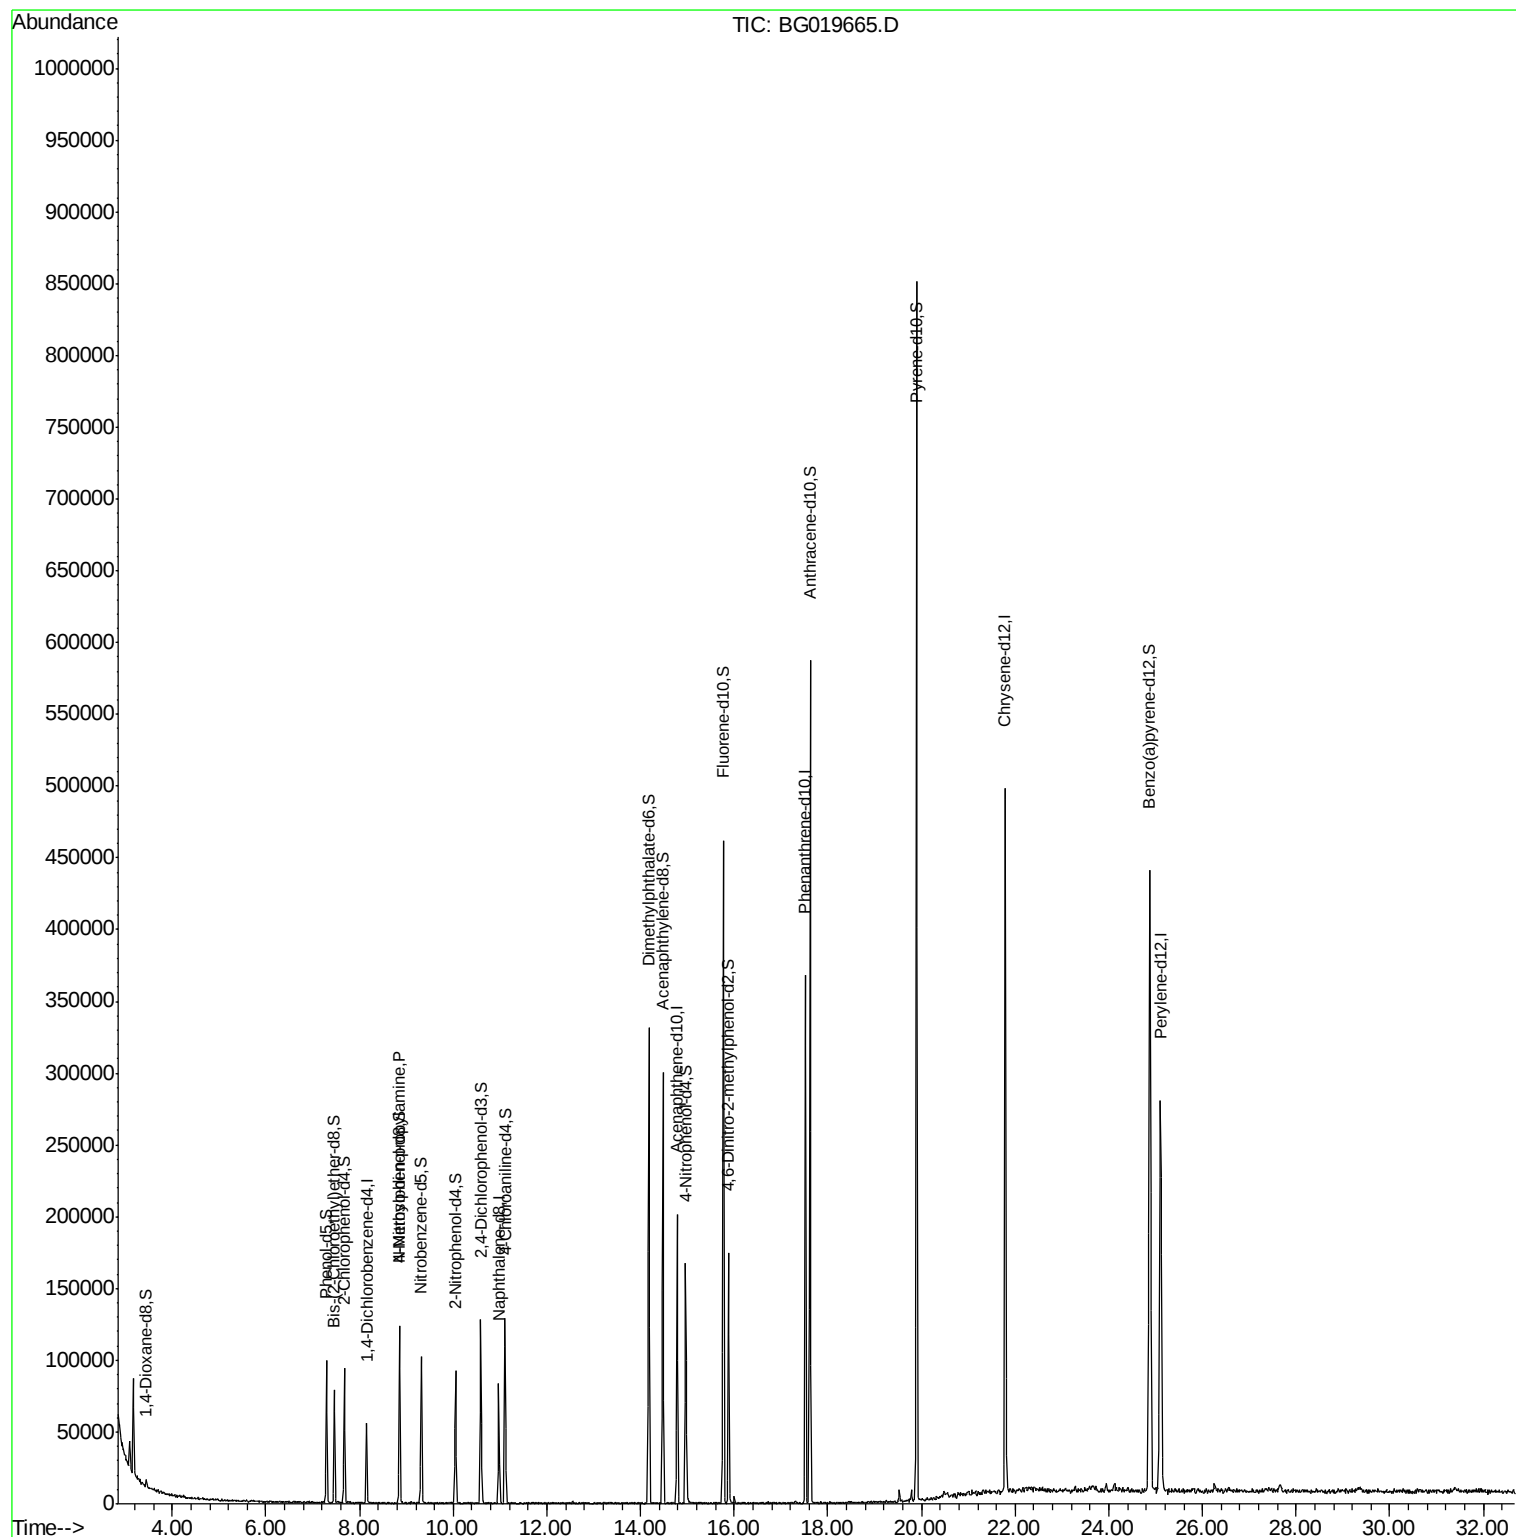

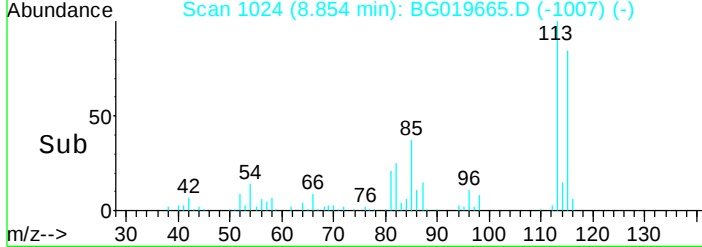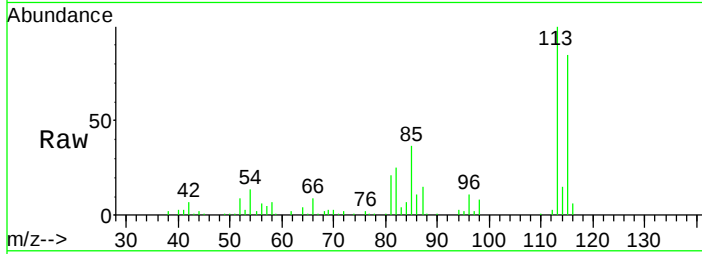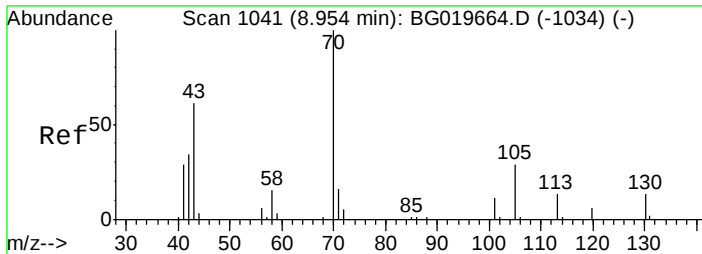

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.12 ng/ul
 RT: 8.85 min Scan# 1024
 Delta R.T. -0.10 min
 Lab File: BG019665.D
 Acq: 17 Nov 2015 18:28

Instrument :
 BNA_G
 ClientSampleId :
 SBLK57

Tot Ion: 70 Resp: 1560
 Ion Ratio Lower Upper
 70 100
 42 221.0 28.4 42.6#
 101 0.0 5.3 7.9#

Abundance Ion 70.000 (69.70 to 70.30): BG
 Ion 42.00 (41.70 to 42.70): BG
 Ion 101.00 (100.70 to 101.70):
 Ion 130.00 (129.70 to 130.70):

