

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111715\
 Data File : BG019670.D
 Acq On : 17 Nov 2015 21:39
 Operator : UM/NP
 Sample : G4427-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC798

Manual Integrations
 APPROVED

mohammad
 11/19/2015 8:26:53 AM

Quant Time: Nov 18 02:39:25 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 18 01:19:35 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	18687	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	85910	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.78	164	83094	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.52	188	244822	20.00	ng/ul	0.00
78) Chrysene-d12	21.79	240	328716	20.00	ng/ul	0.00
86) Perylene-d12	25.11	264	312409	20.00	ng/ul	0.00


System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	2570	5.87	ng/uL	0.00
5) Phenol-d5	7.29	99	60631	31.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	43287	34.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.67	132	40002	32.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	50381	31.79	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	21410	30.35	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	25569	32.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	47703	27.79	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	51539	31.63	ng/ul	0.00
44) Dimethylphthalate-d6	14.18	166	201688	26.84	ng/ul	0.00
47) Acenaphthylene-d8	14.48	160	163655	20.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.97	143	29130	24.60	ng/ul	0.00
58) Fluorene-d10	15.77	176	118158	17.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.88	200	32152	20.33	ng/ul	0.00
71) Anthracene-d10	17.62	188	201826	16.98	ng/ul	0.00
79) Pyrene-d10	19.89	212	191458	12.78	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.88	264	172193	10.56	ng/ul	0.00

Target Compounds

						Ovalue
6) Phenol	7.32	94	4755	2.30	ng/ul	93
45) Dimethylphthalate	14.23	163	183463	24.62	ng/ul	98
77) Fluoranthene	19.56	202	38947	2.33	ng/ul#	94
80) Pyrene	19.92	202	34433	1.79	ng/ul	97
83) Benzo(a)anthracene	21.77	228	22735	1.14	ng/ul	94
85) Chrysene	21.84	228	20509	1.09	ng/ul	96
91) Benzo(a)pyrene	24.94	252	20439m	1.10	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

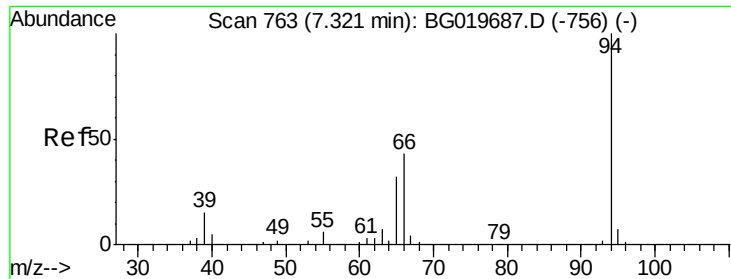

#6

Phenol

Concen: 2.30 ng/ul

RT: 7.32 min Scan# 762

Delta R.T. 0.00 min

Lab File: BG019670.D


Acq: 17 Nov 2015 21:39

Instrument :

BNA_G

ClientSampleId :

BC798

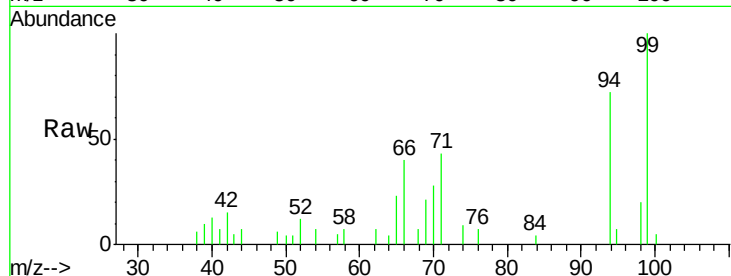

Tot Ion: 94 Resp: 4755

Ion Ratio Lower Upper

94 100

65 32.4 27.4 41.0




66 55.7 39.0 58.6

Manual Integrations

APPROVED

mohammad

11/19/2015 8:26:53 AM

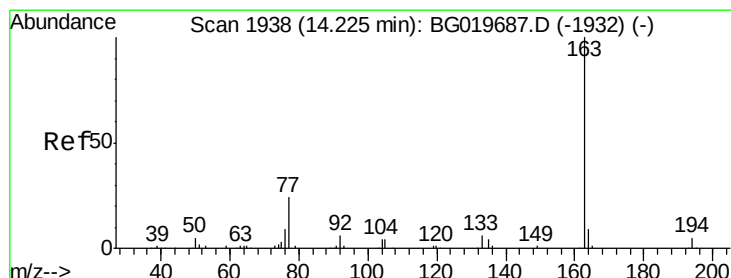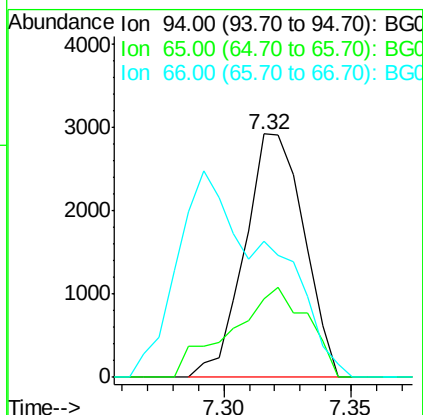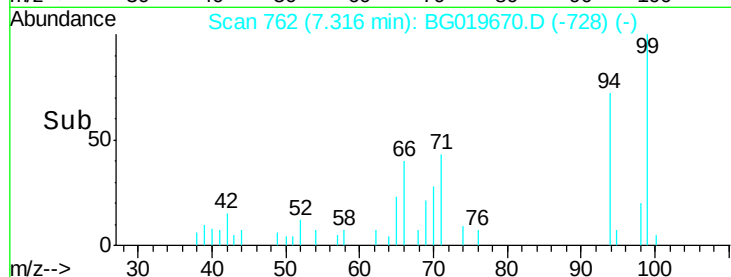

#45

Dimethylphthalate

Concen: 24.62 ng/ul

RT: 14.23 min Scan# 1938

Delta R.T. 0.00 min

Lab File: BG019670.D

Acq: 17 Nov 2015 21:39




Tgt Ion:163 Resp: 183463


Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 11.1 8.3 12.5

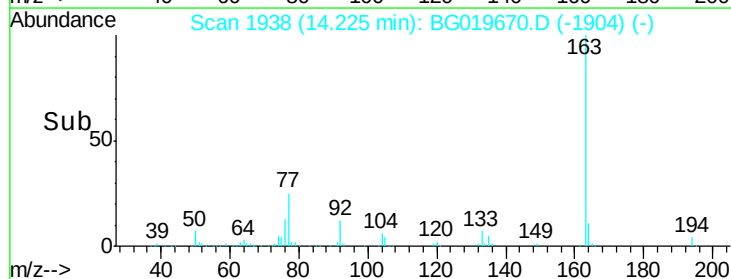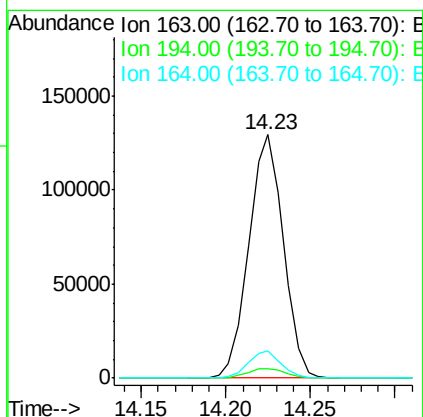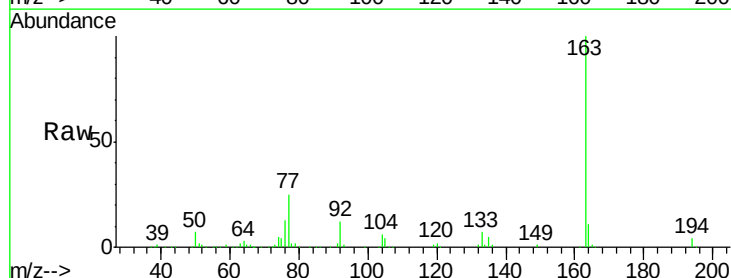

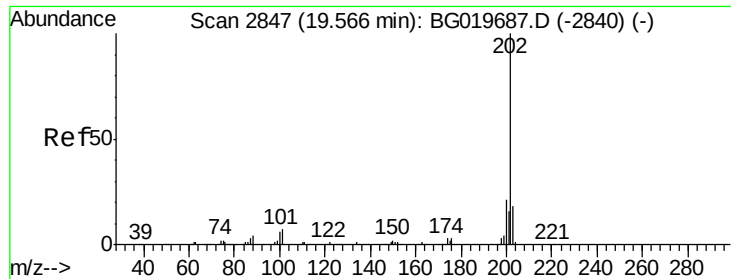

#77

Fluoranthene

Concen: 2.33 ng/ul

RT: 19.56 min Scan# 2846

Delta R.T. 0.00 min

Lab File: BG019670.D

Acq: 17 Nov 2015 21:39

Instrument :

BNA_G


ClientSampleId :

BC798

Tot Ion:	202	Resp:	38947
Ion Ratio	Lower	Upper	
202	100		
101	9.7	5.2	7.8#
100	5.4	5.0	7.4

Manual Integrations
APPROVED




mohammad
11/19/2015 8:26:53 AM

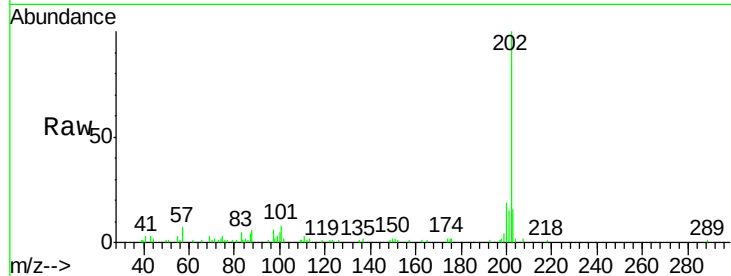

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

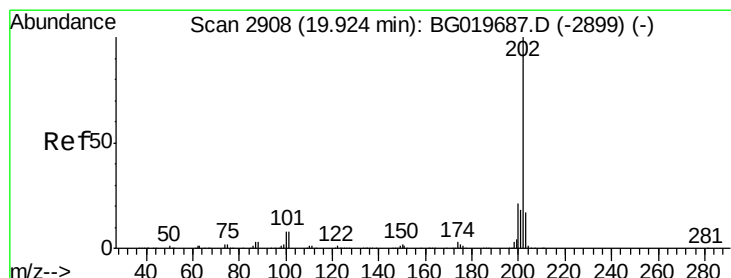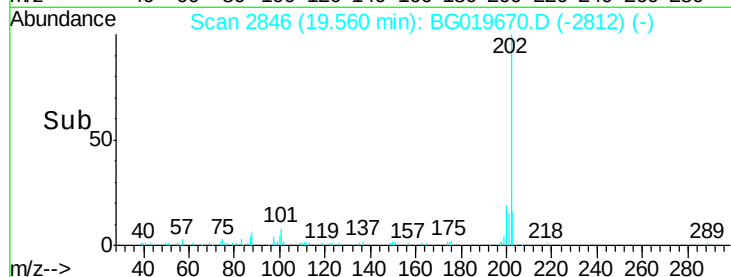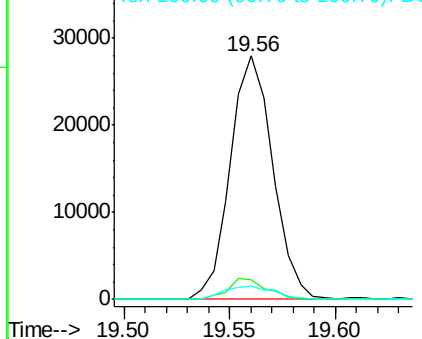

#80

Pyrene

Concen: 1.79 ng/ul

RT: 19.92 min Scan# 2907

Delta R.T. -0.01 min

Lab File: BG019670.D




Acq: 17 Nov 2015 21:39


Tgt Ion:	202	Resp:	34433
Ion Ratio	Lower	Upper	
202	100		
101	9.8	7.0	10.6
100	7.3	6.6	10.0

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

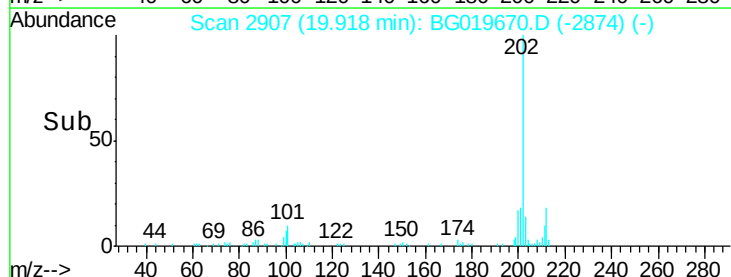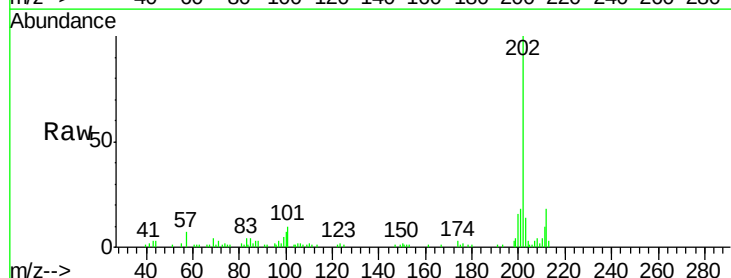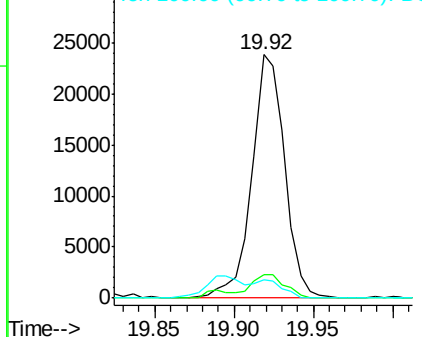

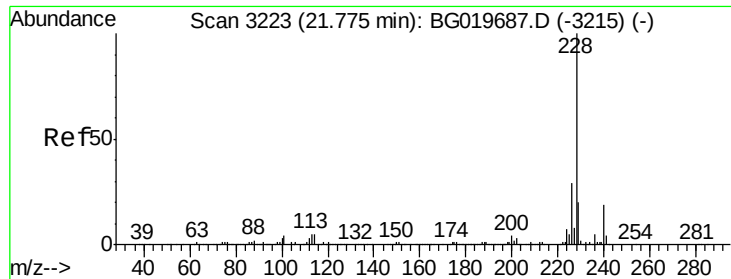





#83
Benzo(a)anthracene
Concen: 1.14 ng/ul
RT: 21.77 min Scan# 3222
Delta R.T. 0.00 min
Lab File: BG019670.D
Acq: 17 Nov 2015 21:39

Instrument :
BNA_G
ClientSampleId :
BC798

Tot Ion	Ratio	Lower	Upper
228	100		
229	19.4	15.7	23.5
226	33.5	22.6	33.8




Manual Integrations
APPROVED


mohammad
11/19/2015 8:26:53 AM

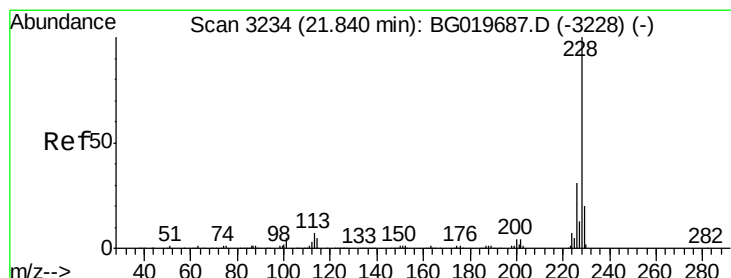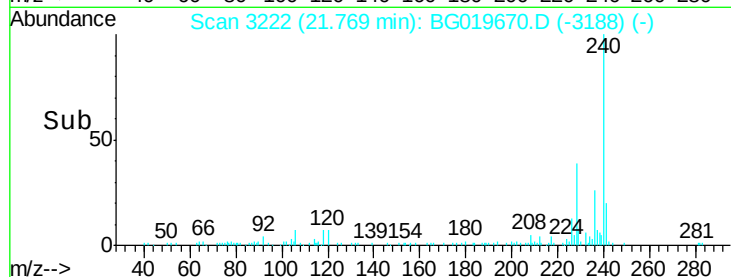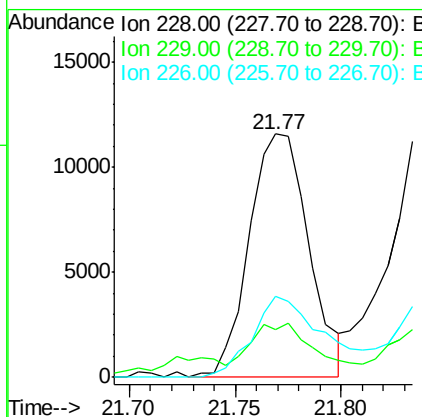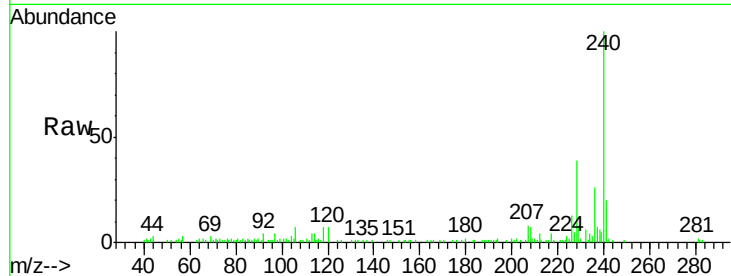

#85
Chrysene
Concen: 1.09 ng/ul
RT: 21.84 min Scan# 3234
Delta R.T. 0.00 min
Lab File: BG019670.D
Acq: 17 Nov 2015 21:39

Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.0	24.9	37.3
229	21.3	17.0	25.6

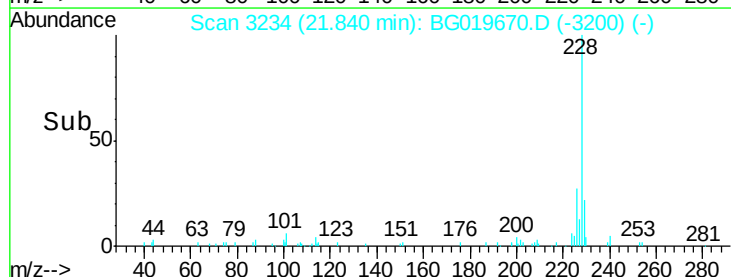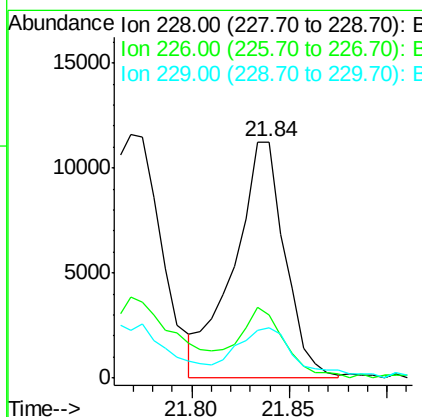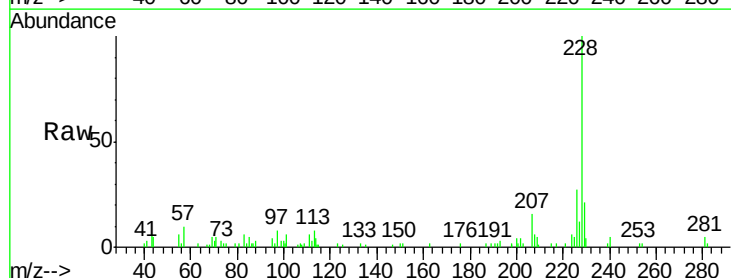

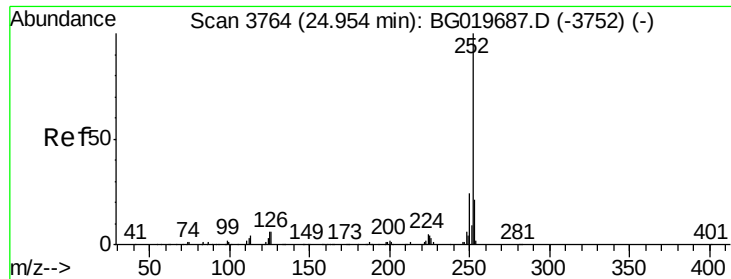

#91
 Benzo(a)pyrene
 Concen: 1.10 ng/ul m
 RT: 24.94 min Scan# 3762
 Delta R.T. -0.01 min
 Lab File: BG019670.D
 Acq: 17 Nov 2015 21:39

Instrument :
 BNA_G
 ClientSampleId :
 BC798

Tot Ion	Ratio	Lower	Upper
252	100		
253	17.0	16.9	25.3
125	5.2	5.4	8.0

Manual Integrations
 APPROVED

mohammad
 11/19/2015 8:26:53 AM

