

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111715\
 Data File : BG019695.D
 Acq On : 18 Nov 2015 19:02
 Operator : UM/NP
 Sample : G4427-09DL 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC7B0DL

Manual Integrations
 APPROVED

mohammad
 11/19/2015 8:27:54 AM

Quant Time: Nov 19 04:23:10 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Nov 19 03:06:25 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	21500	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	95762	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.79	164	78774	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.53	188	221513	20.00	ng/ul	0.00
78) Chrysene-d12	21.79	240	278411	20.00	ng/ul	0.00
86) Perylene-d12	25.11	264	270965	20.00	ng/ul	0.00


System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	218	0.43	ng/uL	0.00
5) Phenol-d5	7.29	99	7982	3.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	5201	3.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.67	132	5021	3.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	6926	3.80	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	2354	2.99	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	2740	3.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	6794	3.55	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	6189	3.41	ng/ul	0.01
44) Dimethylphthalate-d6	14.18	166	26306	3.69	ng/ul	0.00
47) Acenaphthylene-d8	14.48	160	27518	3.56	ng/ul	0.00
52) 4-Nitrophenol-d4	14.97	143	2920	2.60	ng/ul	0.00
58) Fluorene-d10	15.77	176	23331	3.66	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.88	200	1899	1.33	ng/ul	0.00
71) Anthracene-d10	17.62	188	40524m	3.77	ng/ul	0.00
79) Pyrene-d10	19.89	212	46213	3.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.88	264	50920	3.60	ng/ul	0.00

Target Compounds

						Ovalue
45) Dimethylphthalate	14.22	163	15505	2.19	ng/ul	96
70) Phenanthrene	17.57	178	156423	13.19	ng/ul	98
72) Anthracene	17.65	178	33547m	2.81	ng/ul	
75) Carbazole	17.92	167	11821	1.23	ng/ul#	90
77) Fluoranthene	19.56	202	258334	17.10	ng/ul	98
80) Pyrene	19.92	202	207242	12.75	ng/ul	98
81) Butylbenzylphthalate	20.79	149	201728	37.71	ng/ul	99
83) Benzo(a)anthracene	21.77	228	119678	7.09	ng/ul	98
84) Bis(2-ethylhexyl)phthalate	21.65	149	9176	1.17	ng/ul#	97
85) Chrysene	21.84	228	105298	6.63	ng/ul	97
88) Benzo(b)fluoranthene	24.05	252	125870	7.54	ng/ul	96
89) Benzo(k)fluoranthene	24.11	252	41152m	2.55	ng/ul	
91) Benzo(a)pyrene	24.95	252	83347	5.19	ng/ul	94
92) Indeno(1,2,3-cd)pyrene	28.90	276	55633	3.09	ng/ul#	93
94) Benzo(g,h,i)perylene	30.10	276	49161m	3.29	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

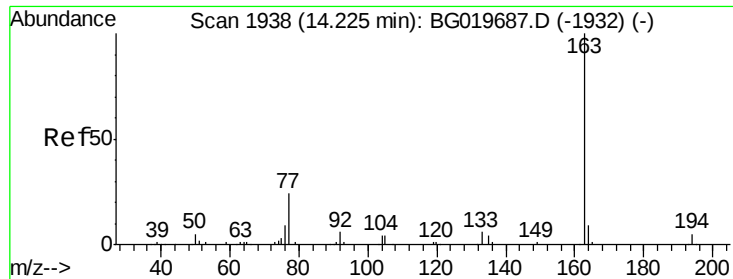





#45
Dimethylphthalate
Concen: 2.19 ng/ul
RT: 14.22 min Scan# 1938
Delta R.T. -0.00 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Instrument :
BNA_G
ClientSampleID :
BC7B0DL

Tot Ion	Ion	Ratio	Resp	Lower	Upper
163	100		15505		
194	3.6		3.5	5.3	
164	8.6		8.3	12.5	




Manual Integrations
APPROVED


mohammad
11/19/2015 8:27:54 AM

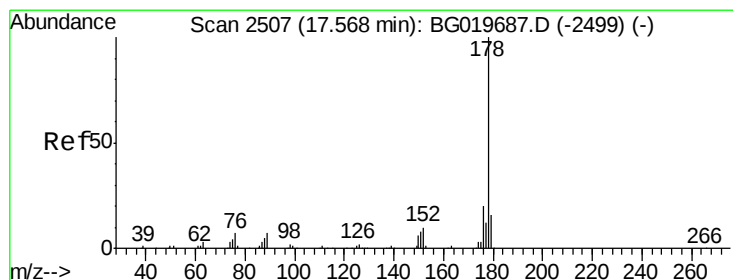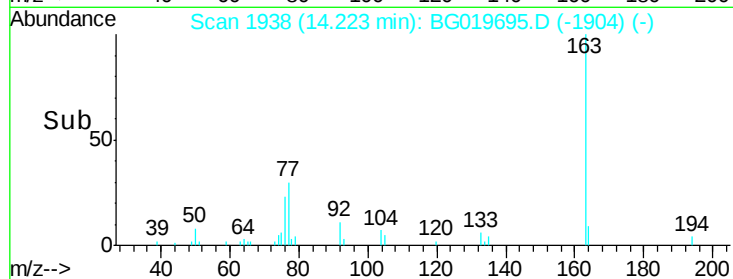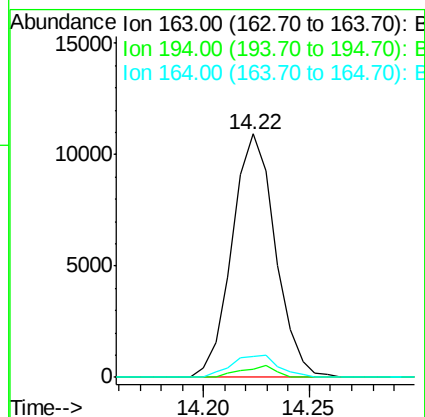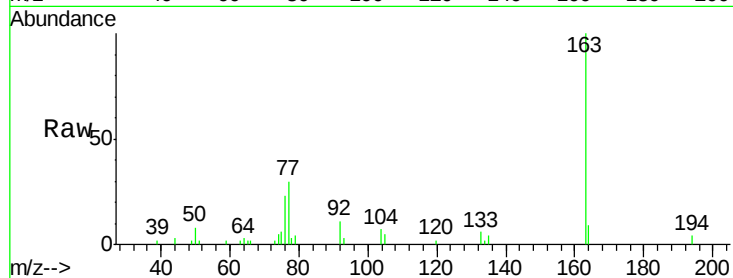

#70
Phenanthrene
Concen: 13.19 ng/ul
RT: 17.57 min Scan# 2507
Delta R.T. -0.00 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
178	100		156423		
179	15.1		12.2	18.2	
176	19.1		16.6	24.8	

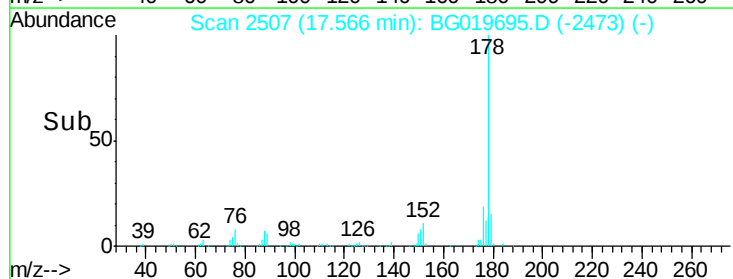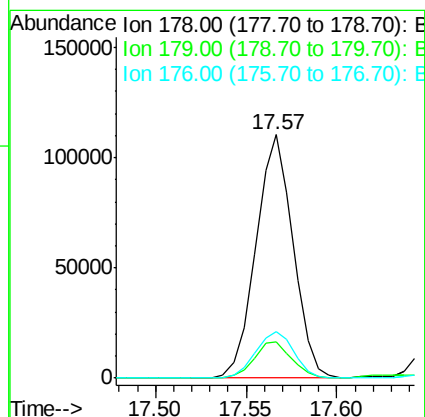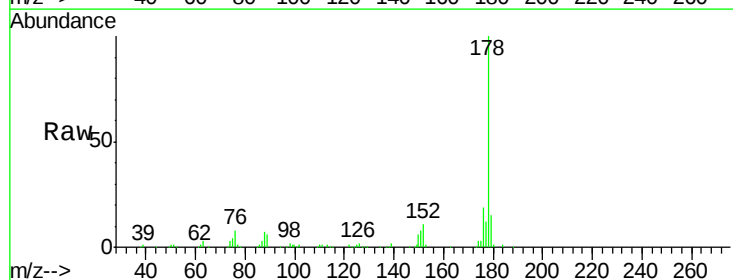



#72

Anthracene

Concen: 2.81 ng/ul m

RT: 17.65 min Scan# 2522

Delta R.T. -0.00 min

Lab File: BG019695.D

Acq: 18 Nov 2015 19:02

Instrument :

BNA_G


ClientSampleId :

BC7B0DL

Tot Ion	Ratio	Lower	Upper
178	100		
179	12.5	12.6	19.0#
176	19.0	15.0	22.4

Manual Integrations
APPROVED




mohammad
11/19/2015 8:27:54 AM

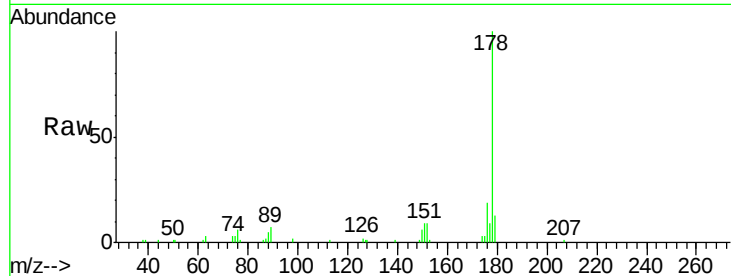

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

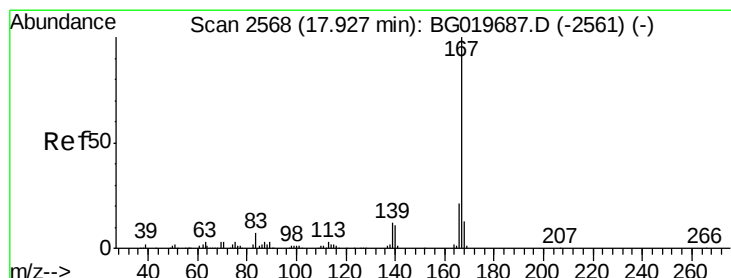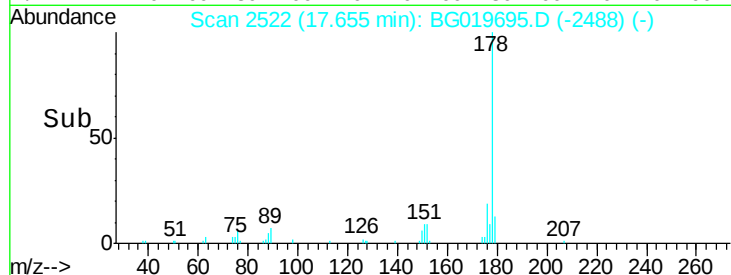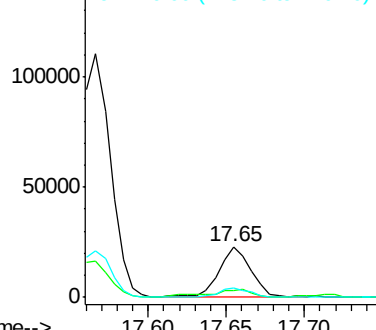

#75

Carbazole

Concen: 1.23 ng/ul


RT: 17.92 min Scan# 2567

Delta R.T. -0.01 min

Lab File: BG019695.D

Acq: 18 Nov 2015 19:02



Tgt Ion	Ratio	Lower	Upper
167	100		
166	16.3	18.1	27.1#
139	10.1	9.8	14.6

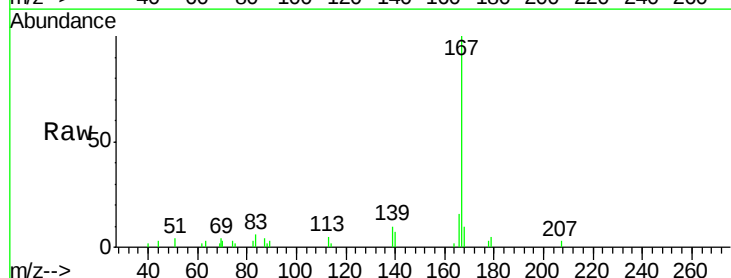


Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

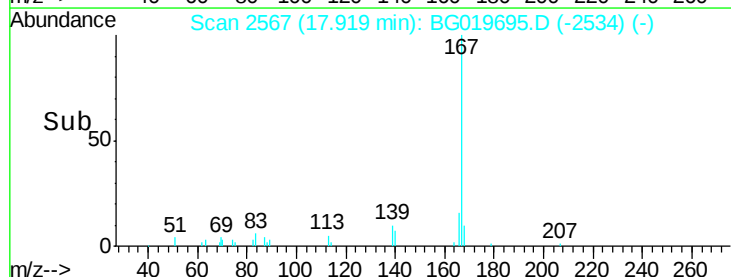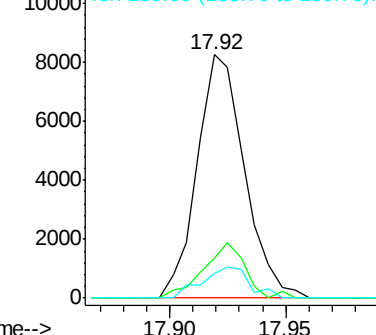







#77
Fluoranthene
Concen: 17.10 ng/ul
RT: 19.56 min Scan# 2847
Delta R.T. -0.00 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Instrument :
BNA_G
ClientSampleId :
BC7B0DL

Tot Ion	Ion:202	Resp:	258334
Ion	Ratio	Lower	Upper
202	100		
101	7.5	5.2	7.8
100	5.8	5.0	7.4




Manual Integrations
APPROVED


mohammad
11/19/2015 8:27:54 AM

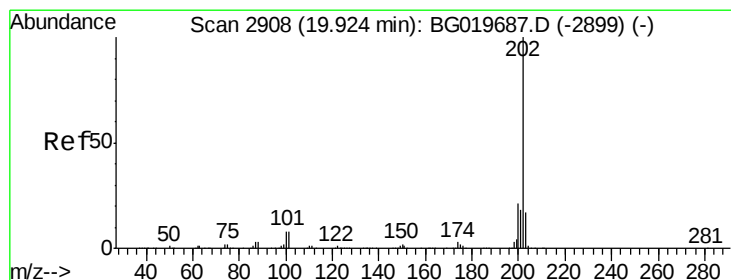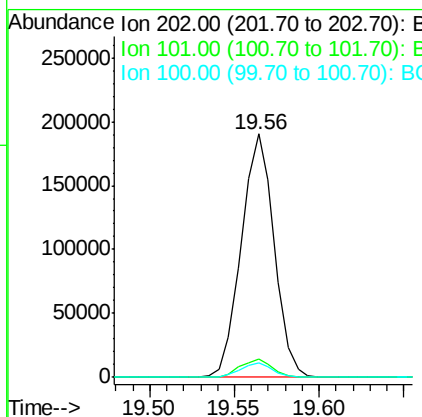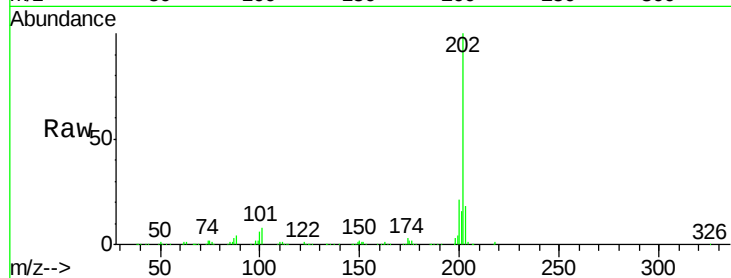

#80
Pyrene
Concen: 12.75 ng/ul
RT: 19.92 min Scan# 2908
Delta R.T. -0.00 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Tgt Ion	Ion:202	Resp:	207242
Ion	Ratio	Lower	Upper
202	100		
101	7.9	7.0	10.6
100	7.8	6.6	10.0

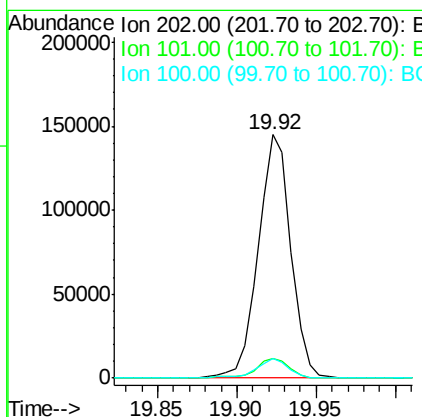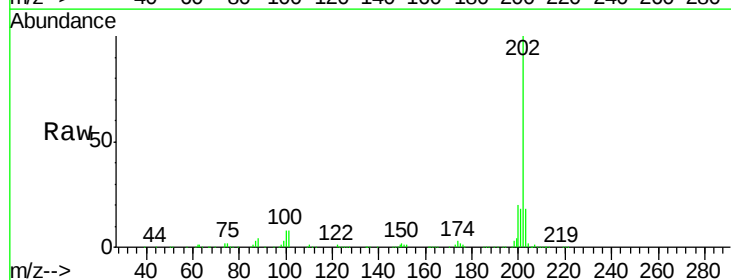







#81
Butylbenzylphthalate
Concen: 37.71 ng/ul
RT: 20.79 min Scan# 3056
Delta R.T. 0.00 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Instrument :
BNA_G
ClientSampleId :
BC7B0DL

Tot Ion	Ratio	Lower	Upper
149	100		
91	90.2	71.1	106.7
206	26.1	20.4	30.6




Manual Integrations
APPROVED


mohammad
11/19/2015 8:27:54 AM

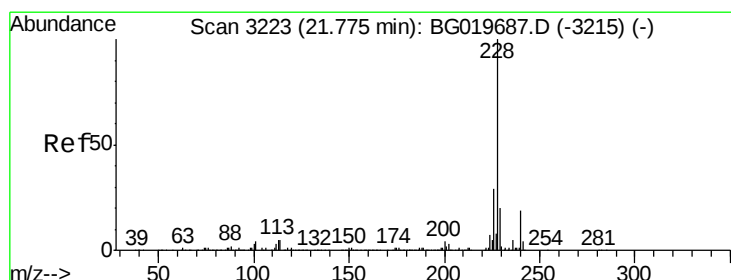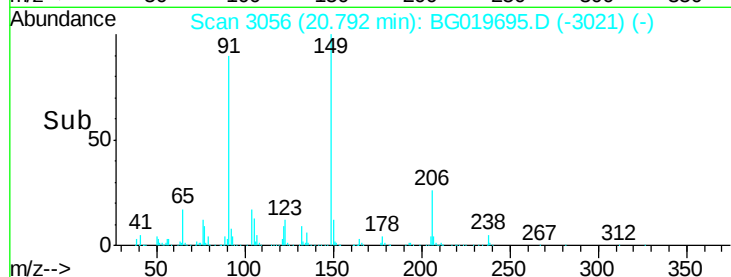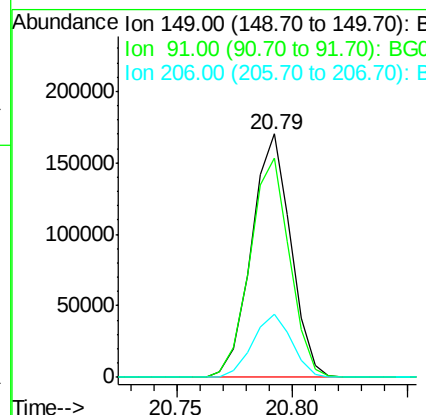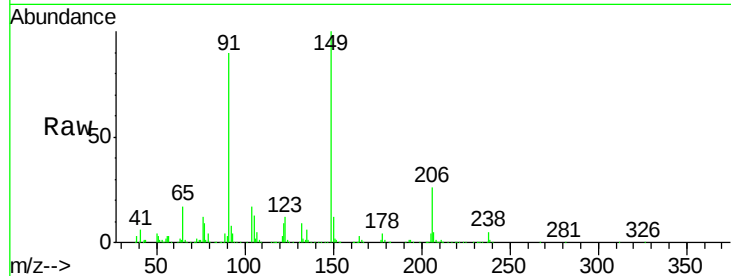

#83
Benzo(a)anthracene
Concen: 7.09 ng/ul
RT: 21.77 min Scan# 3223
Delta R.T. -0.00 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Tgt Ion	Ratio	Lower	Upper
228	100		
229	19.7	15.7	23.5
226	26.8	22.6	33.8

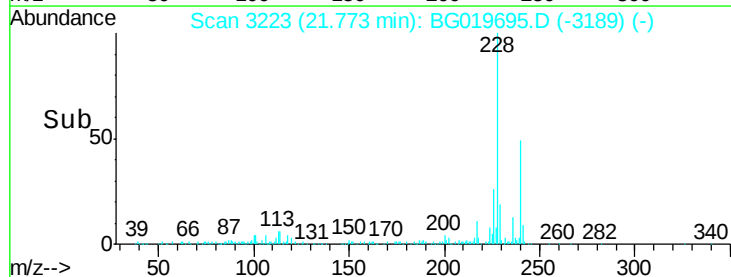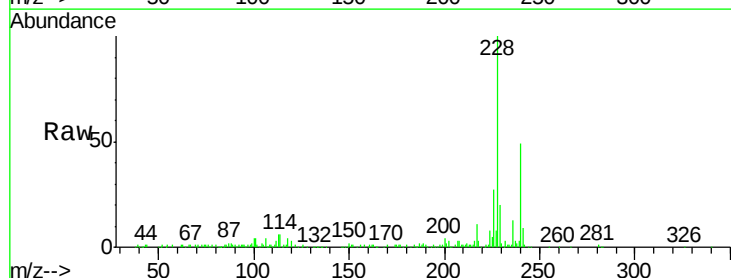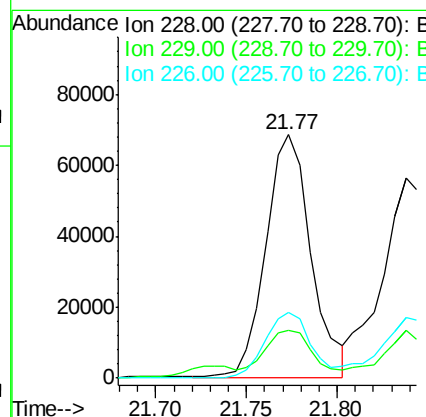







#84
 Bis(2-ethylhexyl)phthalate
 Concen: 1.17 ng/ul
 RT: 21.65 min Scan# 3202
 Delta R.T. -0.00 min
 Lab File: BG019695.D
 Acq: 18 Nov 2015 19:02

Instrument :
 BNA_G
 ClientSampled :
 BC7B0DL

Tot Ion	Ratio	Lower	Upper
149	100		
167	29.3	22.4	33.6
279	3.0	3.6	5.4




Manual Integrations
 APPROVED


mohammad
 11/19/2015 8:27:54 AM

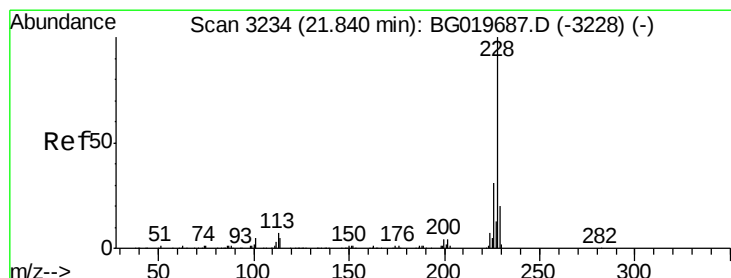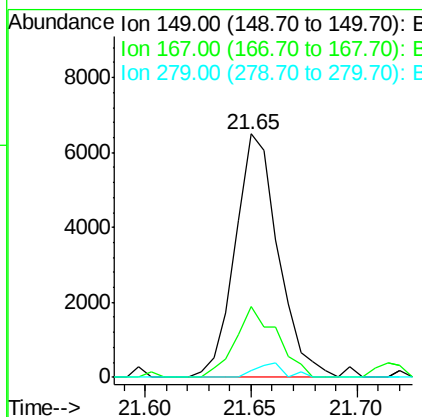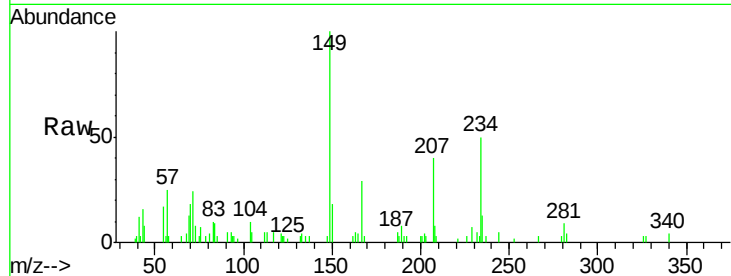

#85
 Chrysene
 Concen: 6.63 ng/ul
 RT: 21.84 min Scan# 3234
 Delta R.T. -0.00 min
 Lab File: BG019695.D
 Acq: 18 Nov 2015 19:02

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.2	24.9	37.3
229	24.1	17.0	25.6

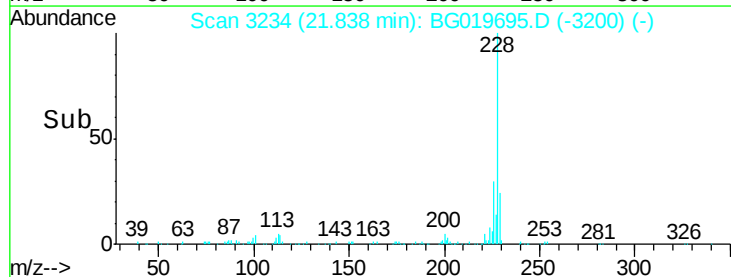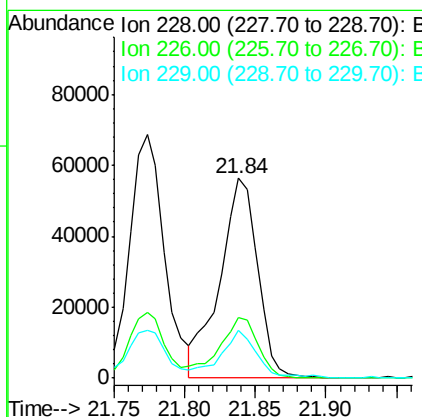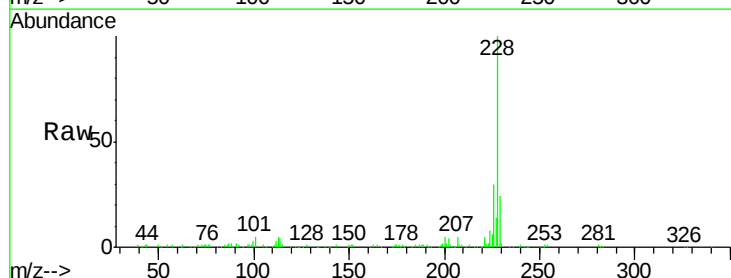

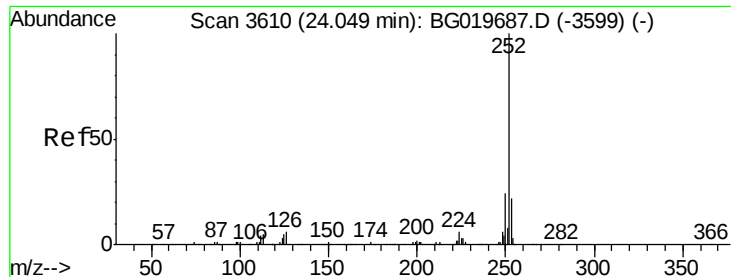

#88

Benzo(b)fluoranthene

Concen: 7.54 ng/ul

RT: 24.05 min Scan# 3611

Delta R.T. 0.00 min

Lab File: BG019695.D

Acq: 18 Nov 2015 19:02

Instrument :

BNA_G





ClientSampleId :

BC7B0DL

Tot Ion	Ratio	Resp	Lower	Upper
252	100	125870		
253	19.2		17.1	25.7
125	5.6		4.2	6.4

Manual Integrations
APPROVED

mohammad
11/19/2015 8:27:54 AM

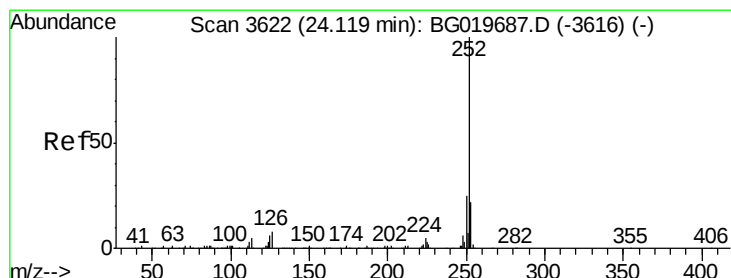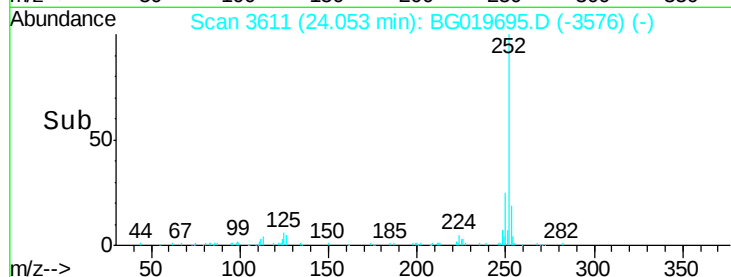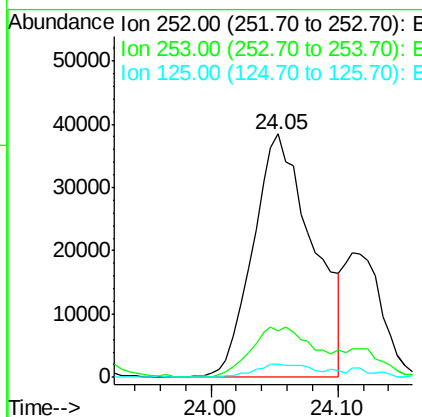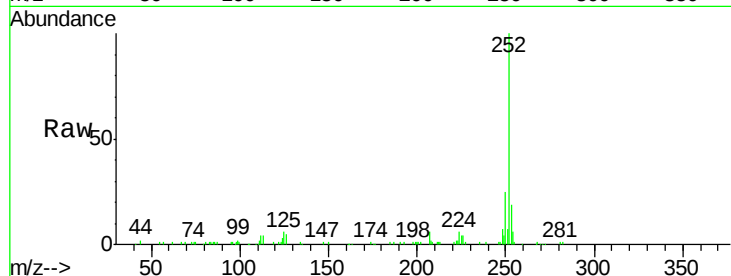

#89

Benzo(k)fluoranthene

Concen: 2.55 ng/ul m




RT: 24.11 min Scan# 3621


Delta R.T. -0.01 min

Lab File: BG019695.D

Acq: 18 Nov 2015 19:02

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	41152		
253	23.4		17.1	25.7
125	7.1		4.4	6.6#

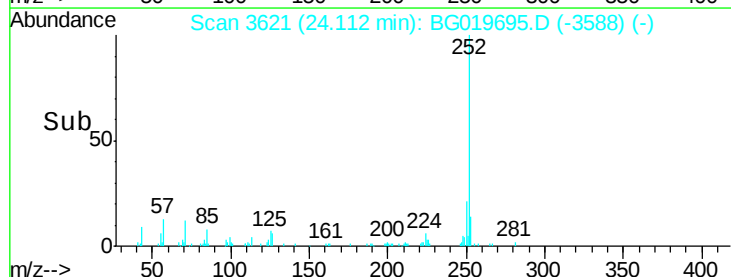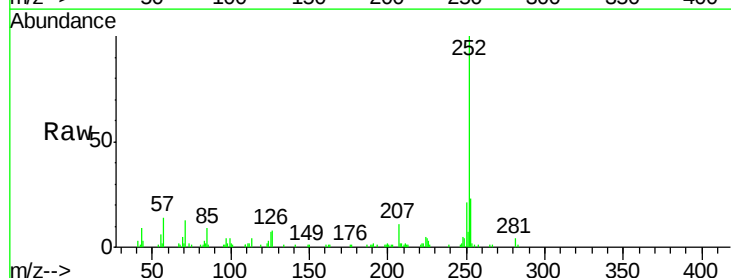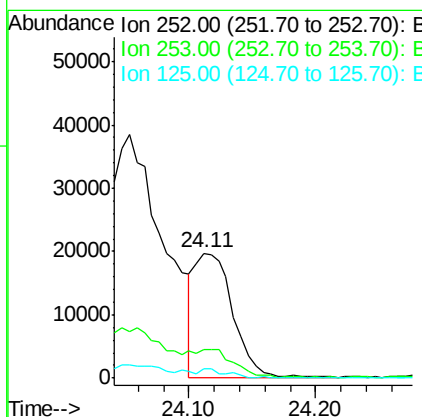







#91
Benzo(a)pyrene
Concen: 5.19 ng/ul
RT: 24.95 min Scan# 3763
Delta R.T. -0.01 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Instrument :
BNA_G
ClientSampleId :
BC7B0DL

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.5	16.9	25.3
125	6.1	5.4	8.0




Manual Integrations
APPROVED


mohammad
11/19/2015 8:27:54 AM

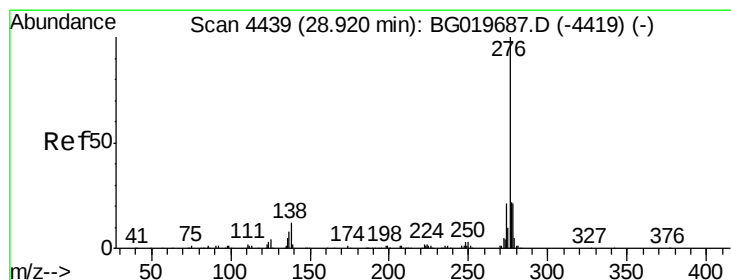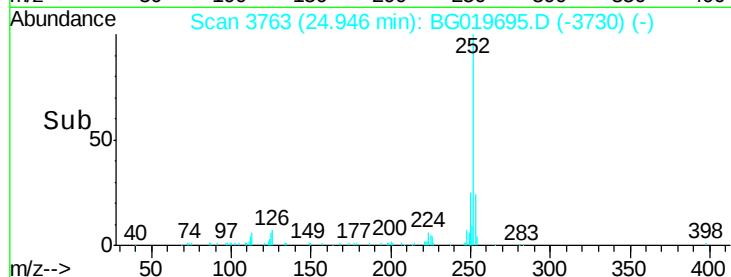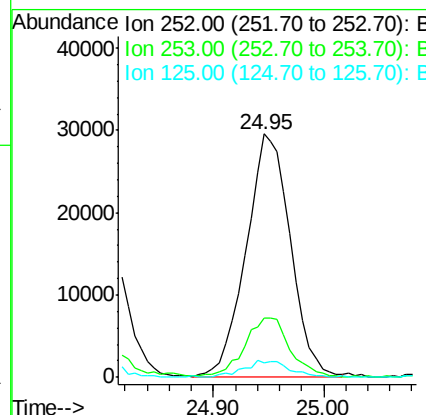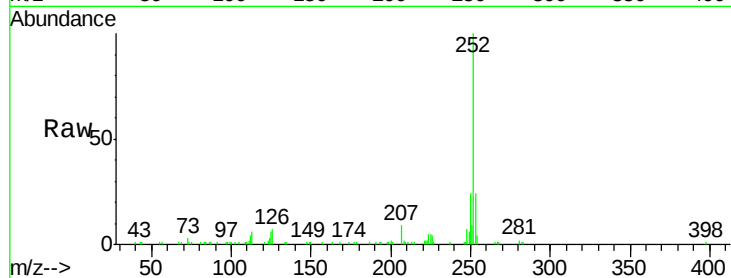

#92
Indeno(1,2,3-cd)pyrene
Concen: 3.09 ng/ul
RT: 28.90 min Scan# 4436
Delta R.T. -0.02 min
Lab File: BG019695.D
Acq: 18 Nov 2015 19:02

Tgt Ion	Ratio	Lower	Upper
276	100		
138	9.0	9.9	14.9#
277	23.4	21.3	31.9

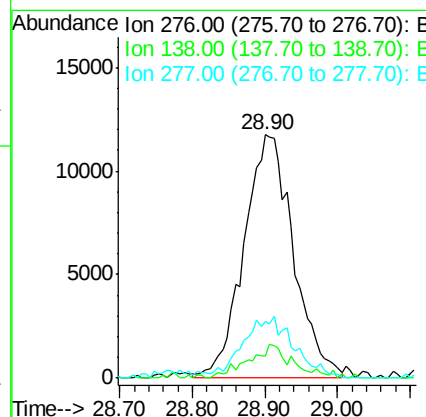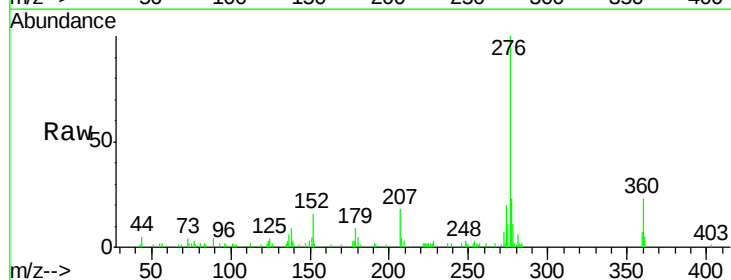



#94
 Benzo(a,h,i)perylene
 Concen: 3.29 ng/ul m
 RT: 30.10 min Scan# 4641
 Delta R.T. -0.01 min
 Lab File: BG019695.D
 Acq: 18 Nov 2015 19:02

Instrument :
 BNA_G
 ClientSampleId :
 BC7B0DL

Tot Ion	Ratio	Lower	Upper
276	100		
138	12.7	9.2	13.8
277	22.7	18.6	28.0

Manual Integrations
 APPROVED

mohammad
 11/19/2015 8:27:54 AM

