


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG111715\
Data File : BG019658.D
Acq On : 17 Nov 2015 8:41
Operator : UM/NP
Sample : DFTPP30
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP30

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111615.M
Title : SVOA CALIBRATION
Last Update : Thu Nov 19 03:06:25 2015

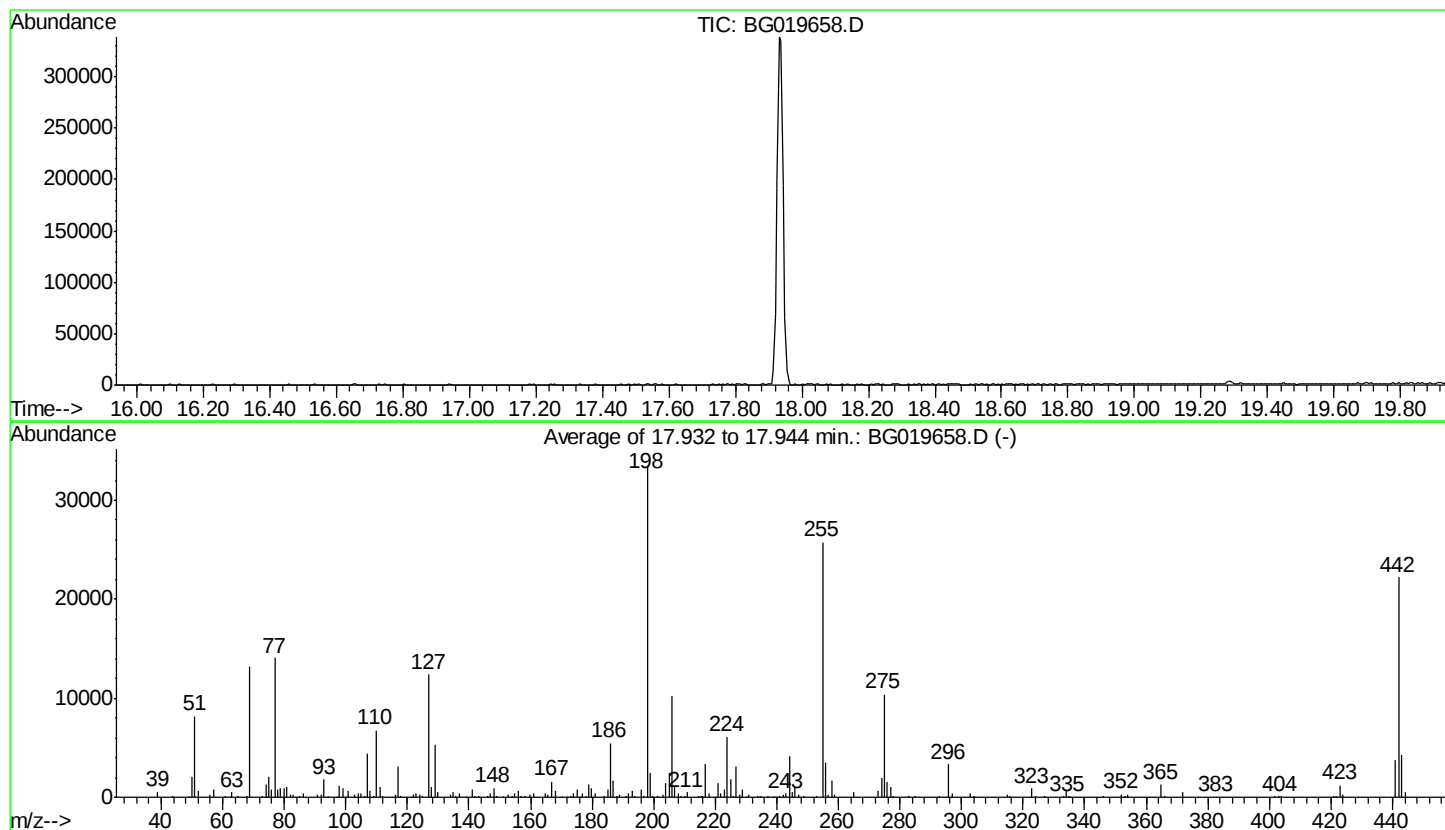

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	8161	PASS
68	69	0.00	2	1.2	154	PASS
69	198	0.00	100	39.2	13131	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.9	12367	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33498	PASS
199	198	5	9	7.4	2476	PASS
275	198	10	60	31.0	10397	PASS
365	198	1	100	3.8	1279	PASS
441	442	0.01	24	17.1	3802	PASS
442	198	50	100	66.4	22240	PASS
443	442	15	24	19.1	4239	PASS

m/z	Abundance
39.00	667.0
43.90	562.0
48.80	179.0
49.20	154.0
50.00	2689.0
51.00	11016.0
52.00	818.0
56.00	392.0
56.90	770.0
61.00	289.0
63.00	497.0
65.00	230.0
68.00	464.0
68.90	18280.0
73.00	302.0
73.90	1688.0
74.90	2719.0
75.90	964.0
77.00	18544.0
77.90	1098.0
78.90	1029.0
80.00	1038.0
81.00	1209.0
81.90	294.0
83.10	286.0
83.80	155.0
84.90	249.0
86.00	489.0
91.00	478.0
91.90	256.0
92.90	2294.0
93.90	200.0
96.80	153.0
98.00	1644.0
98.90	1207.0
99.90	179.0
100.90	623.0
102.90	295.0
103.90	423.0
105.00	578.0
105.90	190.0
106.90	5244.0
107.90	825.0
109.00	240.0
109.90	8912.0
111.00	1166.0
111.90	311.0
115.90	275.0
117.00	3705.0
117.90	206.0
121.90	401.0
122.90	454.0
123.90	407.0
127.00	16024.0
127.90	1314.0
129.00	6619.0
129.90	767.0
133.90	439.0
135.00	576.0
135.80	174.0
137.00	284.0
141.00	1136.0
143.00	251.0
146.80	638.0
147.90	1083.0
149.00	188.0
153.00	313.0
154.90	453.0
156.00	836.0
156.90	237.0
159.90	306.0
160.90	365.0
164.80	315.0
165.80	316.0
167.00	1963.0
168.00	810.0
170.00	159.0
172.90	241.0
173.90	279.0
175.00	872.0
176.90	219.0
178.00	248.0
178.90	1664.0
179.90	1083.0
181.00	557.0
184.10	246.0
185.00	835.0
185.90	6882.0
186.90	2032.0
188.00	240.0
188.90	210.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

191.10	248.0
191.90	459.0
192.90	638.0
193.90	208.0
195.90	808.0
196.60	498.0
197.90	38704.0
198.90	2946.0
200.00	293.0
202.80	227.0
203.90	1605.0
205.00	2819.0
206.00	12070.0
207.00	1569.0
208.00	232.0
209.00	251.0
211.00	585.0
214.90	158.0
215.70	348.0
216.90	3777.0
218.00	295.0
221.00	1641.0
221.90	417.0
222.90	937.0
224.00	6787.0
225.00	1745.0
226.00	459.0
226.90	3551.0
227.90	336.0
228.90	989.0
229.90	192.0
230.90	287.0
233.90	361.0
234.80	203.0
237.00	177.0
240.80	217.0
242.00	253.0
242.90	414.0
244.00	4542.0
245.00	589.0
245.90	953.0
246.90	213.0
248.90	207.0
253.10	259.0
254.90	28272.0
255.90	3891.0
256.80	207.0
258.00	1625.0
258.90	433.0
264.90	643.0
272.90	555.0
274.00	2056.0
274.90	11945.0
275.90	1905.0
276.90	1210.0
277.80	263.0
283.00	270.0
293.00	159.0
295.90	3276.0
296.90	462.0
302.90	310.0
304.00	218.0
314.90	345.0
315.90	253.0
322.90	946.0
323.90	270.0
326.80	156.0
333.90	589.0
335.10	192.0
345.90	160.0
351.90	343.0
353.00	271.0
354.00	280.0
364.90	1414.0
372.00	631.0
403.90	226.0
421.70	153.0
423.00	1250.0
423.80	304.0
441.00	4023.0
442.00	21288.0
443.00	3977.0
443.90	652.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

m/z	Abundance
39.00	613.0
39.90	283.0
43.90	319.0
50.00	2322.0
51.00	8946.0
51.90	818.0
55.90	264.0
56.90	969.0
61.00	188.0
62.30	154.0
63.10	483.0
64.90	284.0
68.90	13876.0
72.80	183.0
74.00	1598.0
74.90	2345.0
75.90	798.0
77.00	15091.0
78.00	838.0
78.90	1069.0
79.90	885.0
80.90	1297.0
82.00	411.0
83.00	301.0
84.80	275.0
86.00	363.0
90.90	414.0
92.00	357.0
93.00	2058.0
97.90	1115.0
98.90	964.0
100.90	946.0
102.90	220.0
103.90	447.0
105.00	503.0
106.00	165.0
106.90	5054.0
107.90	712.0
109.00	170.0
109.90	7128.0
111.00	1304.0
112.00	232.0
115.90	283.0
116.90	3716.0
122.00	322.0
123.00	622.0
123.90	296.0
124.80	221.0
127.00	13641.0
128.00	1313.0
128.90	6028.0
129.90	400.0
133.90	235.0
134.90	660.0
135.90	282.0
136.90	425.0
138.90	188.0
141.00	666.0
141.90	233.0
142.90	168.0
145.90	251.0
146.90	417.0
148.00	966.0
148.80	208.0
150.90	168.0
152.90	336.0
153.90	244.0
155.00	621.0
156.00	762.0
158.00	221.0
160.00	282.0
160.90	427.0
164.90	584.0
165.80	369.0
167.00	1695.0
167.90	806.0
171.80	187.0
172.90	151.0
174.00	450.0
175.00	1064.0
176.00	192.0
177.00	399.0
179.00	1803.0
179.90	905.0
180.80	371.0
184.90	985.0
186.00	6030.0
187.00	1846.0
188.80	357.0
192.00	627.0
192.90	764.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

193.80	176.0
196.00	1090.0
197.90	39104.0
198.90	2982.0
199.80	225.0
201.00	160.0
201.40	193.0
202.90	374.0
204.00	2105.0
204.90	2978.0
206.00	11785.0
206.90	1303.0
207.90	717.0
208.90	265.0
210.10	252.0
210.90	562.0
214.80	201.0
216.00	247.0
216.90	3638.0
218.00	418.0
220.90	1432.0
221.90	524.0
223.00	730.0
224.00	7704.0
225.00	2475.0
226.90	3666.0
227.80	331.0
229.00	860.0
230.90	337.0
234.00	226.0
234.80	287.0
236.90	298.0
238.80	171.0
240.90	210.0
242.00	353.0
243.00	346.0
244.00	5256.0
245.00	474.0
245.90	1390.0
247.00	216.0
248.90	195.0
252.90	175.0
254.90	31216.0
256.00	4242.0
256.90	320.0
257.90	2057.0
258.90	313.0
265.00	670.0
272.90	911.0
273.90	1978.0
275.00	11504.0
275.90	1937.0
276.90	1199.0
277.90	241.0
285.00	243.0
293.00	419.0
296.00	4411.0
296.90	471.0
303.00	631.0
303.80	286.0
314.80	291.0
315.90	215.0
323.00	913.0
326.70	224.0
333.00	268.0
334.00	712.0
334.80	166.0
345.80	212.0
351.90	270.0
354.00	262.0
364.90	1506.0
366.00	247.0
372.00	764.0
382.80	184.0
401.80	226.0
403.00	231.0
420.80	234.0
423.00	1467.0
424.00	436.0
441.00	4373.0
442.00	25432.0
443.00	5254.0
444.00	410.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

m/z	Abundance
39.00	372.0
40.00	321.0
43.90	504.0
50.00	1173.0
51.00	4522.0
51.90	220.0
55.90	241.0
57.00	484.0
63.00	401.0
68.90	7238.0
74.00	705.0
74.90	1243.0
75.90	409.0
77.00	8488.0
78.00	458.0
79.00	569.0
79.90	799.0
80.90	654.0
82.90	256.0
85.10	178.0
85.90	177.0
92.90	956.0
94.10	153.0
97.90	731.0
98.90	624.0
100.90	417.0
102.80	232.0
104.00	230.0
105.00	211.0
107.00	2760.0
108.00	412.0
110.00	4322.0
110.90	654.0
116.00	303.0
117.00	1812.0
117.90	182.0
122.00	174.0
122.90	270.0
123.90	196.0
127.00	7437.0
127.90	573.0
129.00	3120.0
129.90	218.0
134.00	159.0
134.90	208.0
136.90	179.0
137.10	167.0
140.80	701.0
146.00	161.0
146.90	273.0
147.90	696.0
152.80	165.0
154.90	242.0
155.90	530.0
159.90	258.0
160.90	218.0
164.70	210.0
165.90	186.0
166.90	1094.0
168.00	463.0
172.90	195.0
173.90	272.0
175.00	496.0
176.90	428.0
179.00	599.0
180.00	557.0
180.90	294.0
185.00	526.0
185.90	3500.0
187.00	1095.0
189.00	197.0
190.80	200.0
192.00	177.0
193.00	536.0
195.90	508.0
197.90	22688.0
198.90	1502.0
201.20	159.0
202.90	336.0
203.90	637.0
204.90	1529.0
206.00	6764.0
207.00	1251.0
207.90	362.0
210.80	232.0
215.70	186.0
215.90	192.0
216.90	2843.0
217.90	348.0
220.10	189.0
220.90	1019.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

221.70	329.0
222.90	629.0
224.00	3918.0
225.00	1049.0
227.00	1937.0
228.80	512.0
230.90	241.0
235.00	168.0
239.10	160.0
242.00	259.0
243.10	335.0
243.90	2704.0
244.90	520.0
245.90	616.0
246.90	254.0
248.90	158.0
254.90	17872.0
255.90	2363.0
256.90	231.0
257.90	1189.0
258.90	210.0
264.90	409.0
273.00	545.0
274.00	1626.0
275.00	7742.0
276.00	1007.0
276.90	612.0
284.90	193.0
296.00	2289.0
296.90	316.0
303.00	262.0
314.90	276.0
323.00	730.0
327.00	159.0
334.00	575.0
334.80	174.0
352.00	170.0
352.90	228.0
354.00	338.0
364.80	918.0
365.90	167.0
371.90	296.0
403.80	150.0
420.90	181.0
421.90	213.0
422.90	880.0
424.00	240.0
441.00	3012.0
442.00	20000.0
443.00	3486.0
444.10	524.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

Scan 2563 (17.897 min): BG019658.D
DFTPP30

m/z	Abundance
39.90	218.0
44.00	352.0
207.00	196.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30