
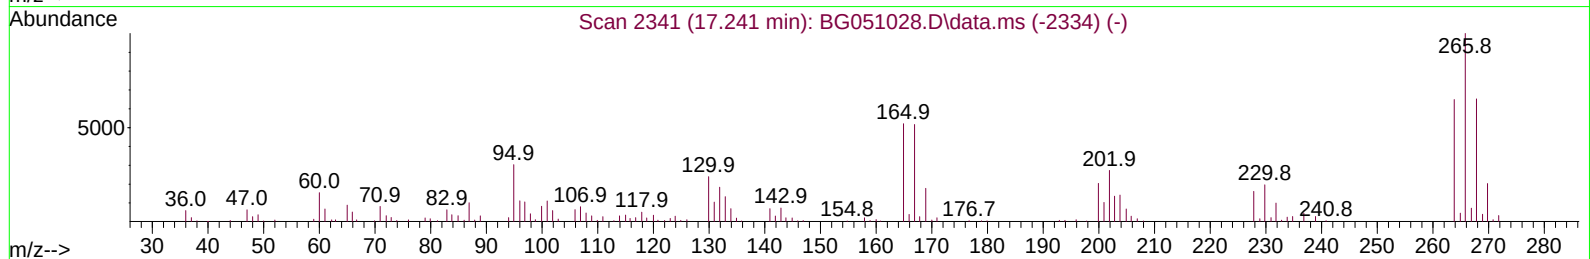
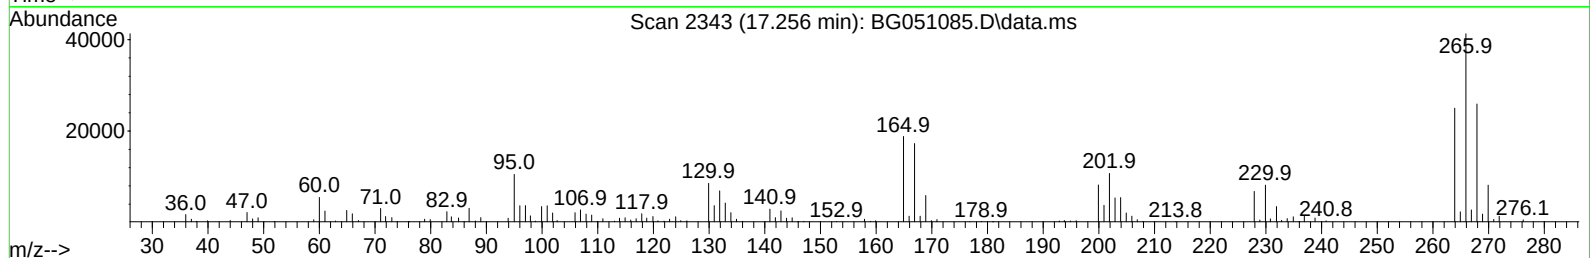


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
Data File : BG051085.D
Acq On : 17 Nov 2021 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 10:31:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

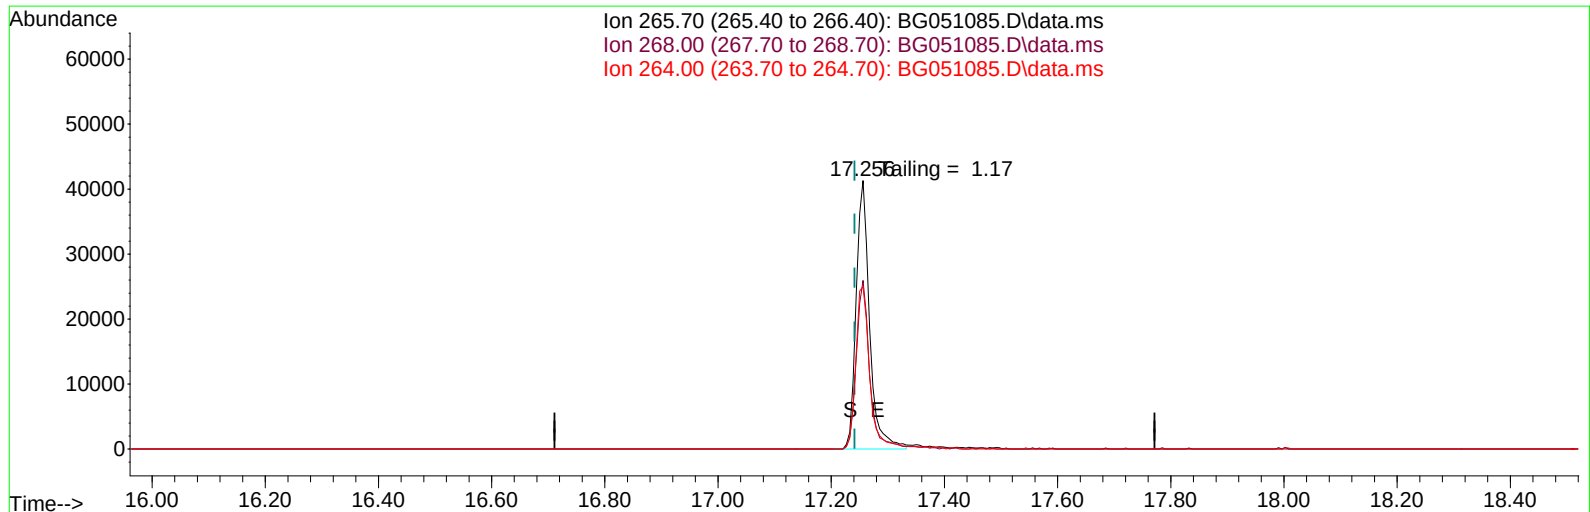

TIC: BG051085.D\data.ms

(70) Pentachlorophenol (C)




17.256min (+ 0.015) 30151.00 ng

response 68626

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.79
264.00	61.30	60.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
 Data File : BG051085.D
 Acq On : 17 Nov 2021 9:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 10:31:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 03:55:35 2021
 Response via : Initial Calibration

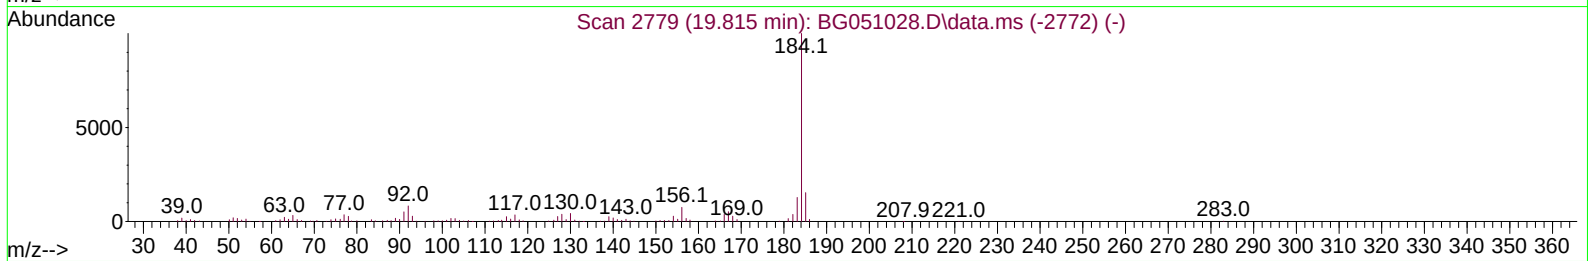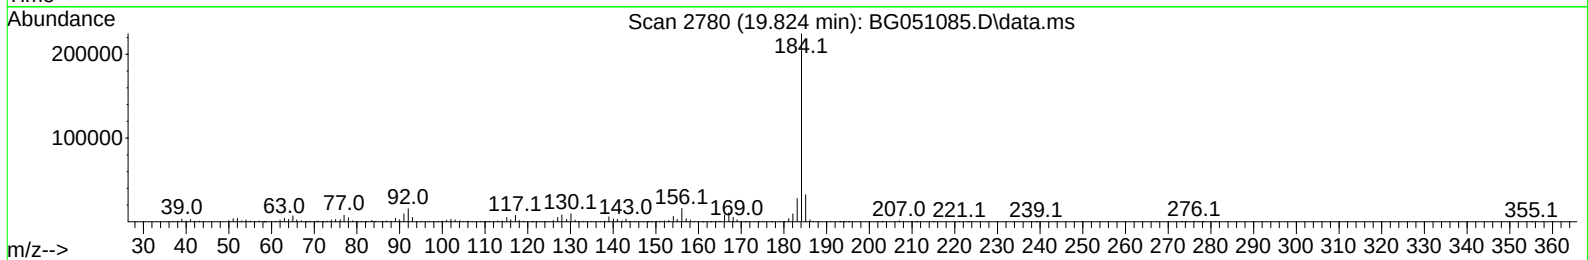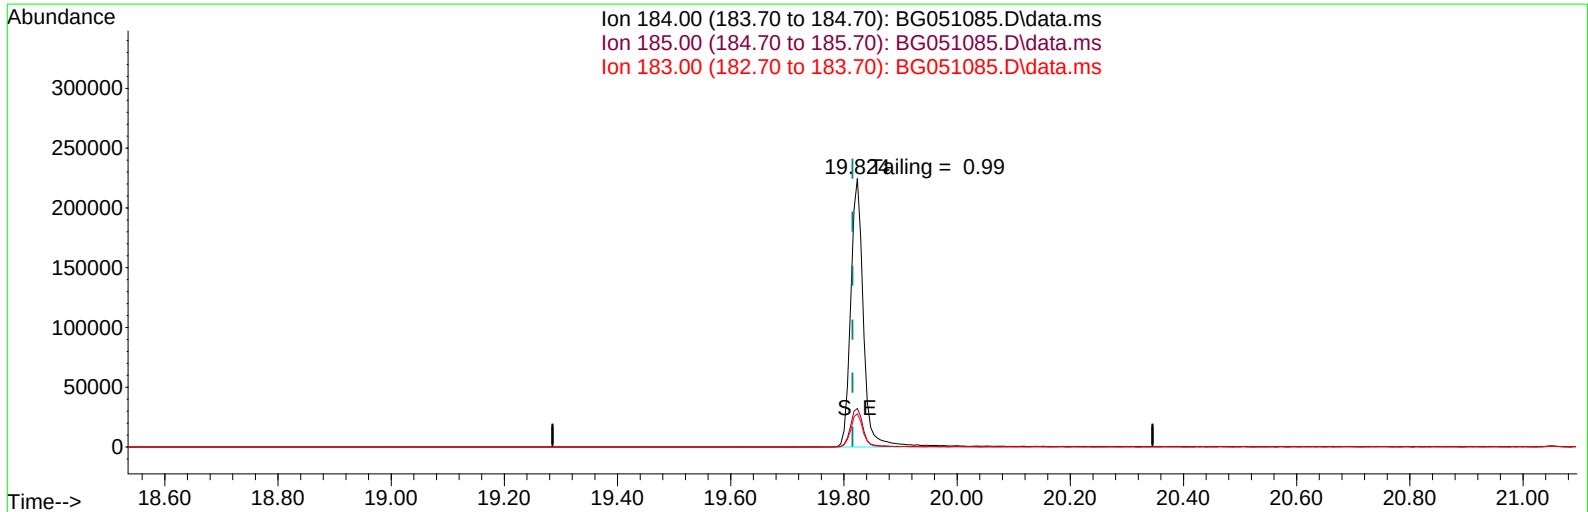

TIC: BG051085.D\data.ms

(77) Benzidine**19.824min (+ 0.009) 330243.18 ng****response 349571**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.41
183.00	11.70	12.43
0.00	0.00	0.00