

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
 Data File : BG051101.D
 Acq On : 17 Nov 2021 21:06
 Operator : CG/JU
 Sample : M4700-01 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 IMPOUND-LOT-SP-JC-11-15-21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG051101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.770	380	388	396	rBV	205909	366110	37.97%	4.500%
2	7.380	653	662	675	rBV	220728	412580	42.79%	5.072%
3	8.226	799	806	818	rVB	131849	231346	23.99%	2.844%
4	9.407	997	1007	1016	rBV	135005	262825	27.26%	3.231%
5	10.453	1176	1185	1194	rBV2	34981	65167	6.76%	0.801%
6	10.806	1238	1245	1253	rBV3	12035	25258	2.62%	0.310%
7	11.058	1280	1288	1294	rBV	181444	343995	35.68%	4.229%
8	11.111	1294	1297	1304	rVB2	9144	14610	1.52%	0.180%
9	12.416	1514	1519	1523	rBV4	6234	9710	1.01%	0.119%
10	12.698	1562	1567	1572	rVB	10454	15078	1.56%	0.185%
11	12.915	1599	1604	1609	rVB3	6015	10572	1.10%	0.130%
12	13.473	1692	1699	1706	rBV	357577	557826	57.85%	6.857%
13	13.644	1717	1728	1732	rBV6	12276	28261	2.93%	0.347%
14	13.714	1733	1740	1743	rBV7	6061	12130	1.26%	0.149%
15	14.172	1812	1818	1823	rVB5	10357	17672	1.83%	0.217%
16	14.266	1830	1834	1836	rBV2	8725	11934	1.24%	0.147%
17	14.578	1883	1887	1893	rBV4	15543	30245	3.14%	0.372%
18	14.672	1899	1903	1906	rBV5	9170	12600	1.31%	0.155%
19	14.813	1920	1927	1928	rBV7	8617	13879	1.44%	0.171%
20	14.854	1928	1934	1940	rVV	279340	452169	46.89%	5.558%
21	14.918	1940	1945	1952	rVB2	21968	40456	4.20%	0.497%
22	15.071	1965	1971	1977	rVB9	5677	13058	1.35%	0.161%
23	15.248	1997	2001	2008	rVB2	16473	26264	2.72%	0.323%
24	15.629	2060	2066	2068	rBV6	14673	25572	2.65%	0.314%
25	15.735	2078	2084	2086	rBV6	6168	12633	1.31%	0.155%
26	15.900	2106	2112	2116	rBV3	17086	27507	2.85%	0.338%
27	16.340	2181	2187	2195	rBV2	229698	388964	40.34%	4.781%
28	16.540	2214	2221	2227	rBV6	24236	59446	6.17%	0.731%
29	17.263	2340	2344	2348	rVB2	19050	29033	3.01%	0.357%
30	17.604	2396	2402	2405	rBV	295439	461286	47.84%	5.670%
31	17.645	2405	2409	2415	rVB	383941	575388	59.67%	7.073%
32	17.739	2421	2425	2432	rVB	63010	92553	9.60%	1.138%
33	18.526	2556	2559	2564	rVB2	83049	115700	12.00%	1.422%
34	19.648	2745	2750	2755	rBV	673490	964244	100.00%	11.853%
35	20.013	2807	2812	2818	rVB	652771	956696	99.22%	11.760%
36	20.189	2838	2842	2849	rBV	475296	657509	68.19%	8.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
Data File : BG051101.D
Acq On : 17 Nov 2021 21:06
Operator : CG/JU
Sample : M4700-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IMPOUND-LOT-SP-JC-11-15-21

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.899	3128	3133	3139	rBV2	321879	794858	82.43%	9.771%
----	--------	------	------	------	------	--------	--------	--------	--------




Sum of corrected areas: 8135134

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
Data File : BG051101.D
Acq On : 17 Nov 2021 21:06
Operator : CG/JU
Sample : M4700-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IMPOUND-LOT-SP-JC-11-15-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

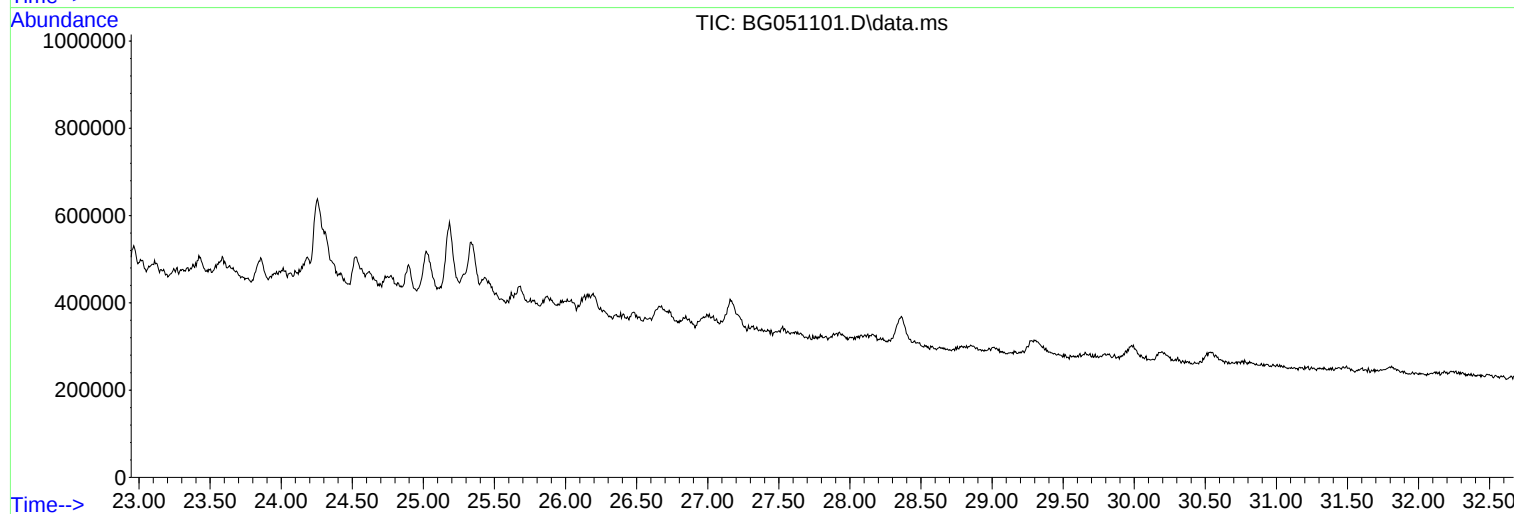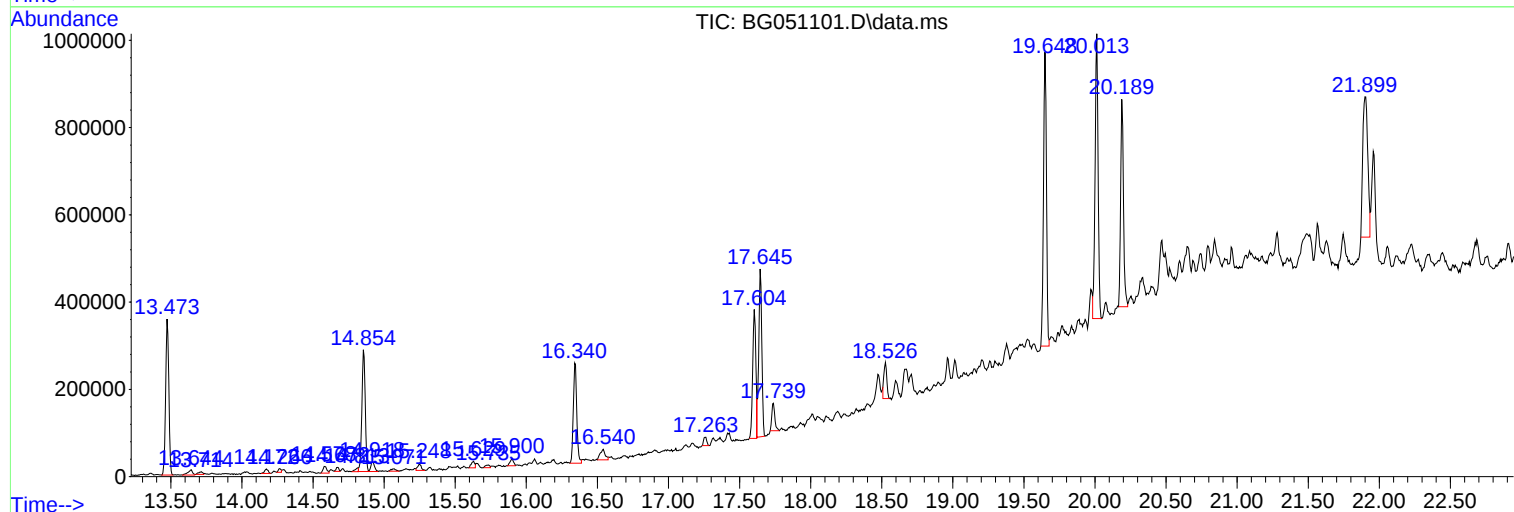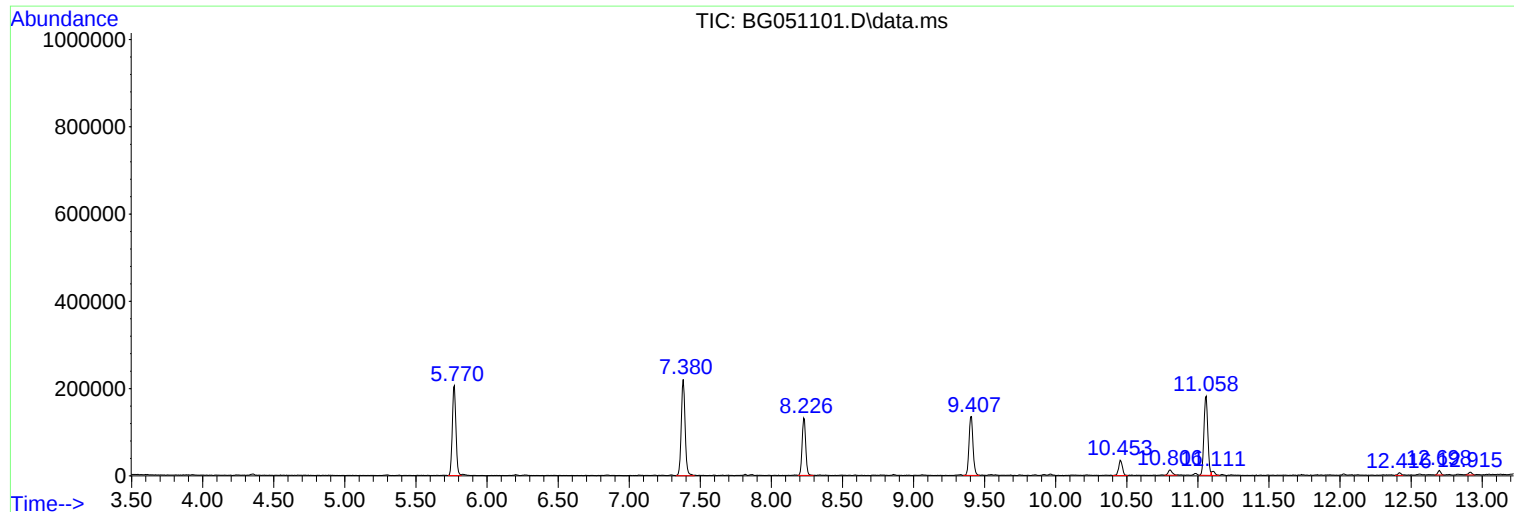

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
Data File : BG051101.D
Acq On : 17 Nov 2021 21:06
Operator : CG/JU
Sample : M4700-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IMPOUND-LOT-SP-JC-11-15-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
Data File : BG051101.D
Acq On : 17 Nov 2021 21:06
Operator : CG/JU
Sample : M4700-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IMPOUND-LOT-SP-JC-11-15-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc