
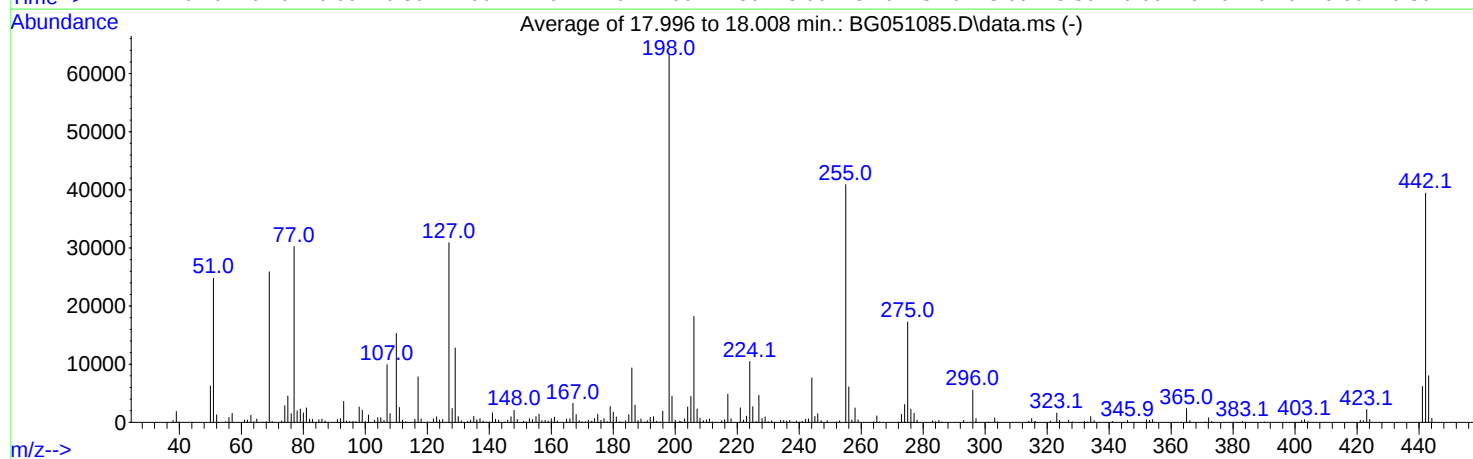


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
 Data File : BG051085.D
 Acq On : 17 Nov 2021 9:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 15 03:55:35 2021

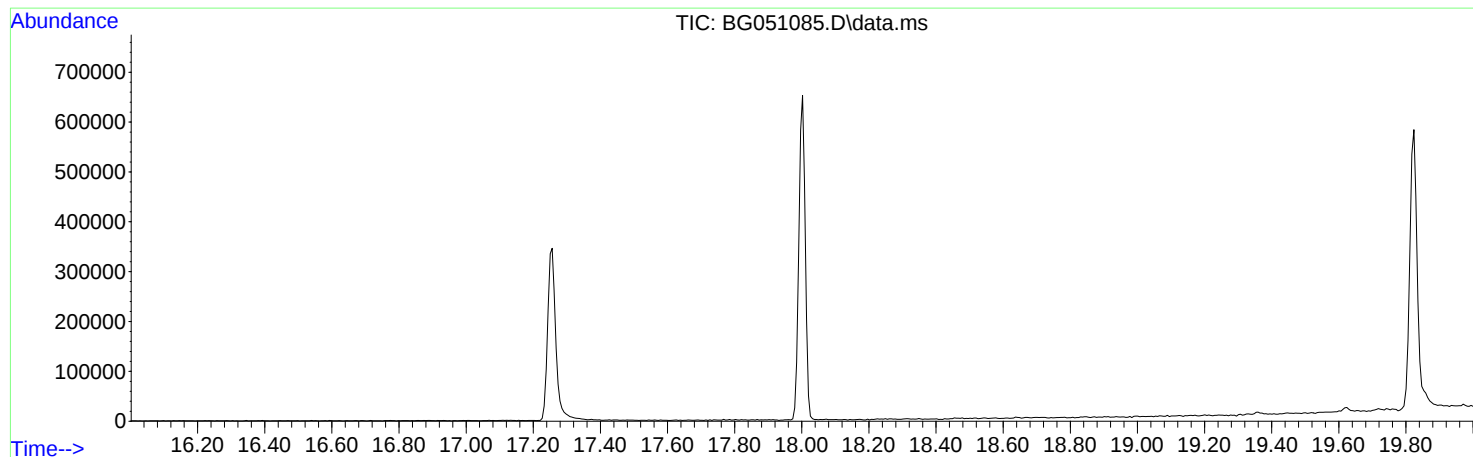




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	24789	PASS
68	69	0.00	2	0.6	151	PASS
69	198	0.00	100	40.9	25913	PASS
70	69	0.00	2	0.8	196	PASS
127	198	10	80	48.8	30915	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63288	PASS
199	198	5	9	7.1	4485	PASS
275	198	10	60	27.3	17274	PASS
365	198	1	100	3.7	2363	PASS
441	198	0.01	100	9.8	6176	PASS
442	442	50	100	100.0	39435	PASS
443	442	15	24	20.3	8013	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
Data File : BG051085.D
Acq On : 17 Nov 2021 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 17 10:31:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

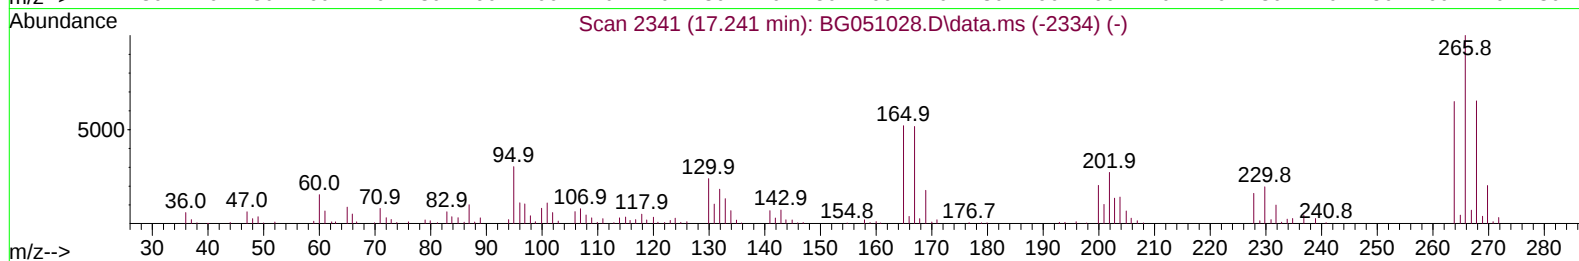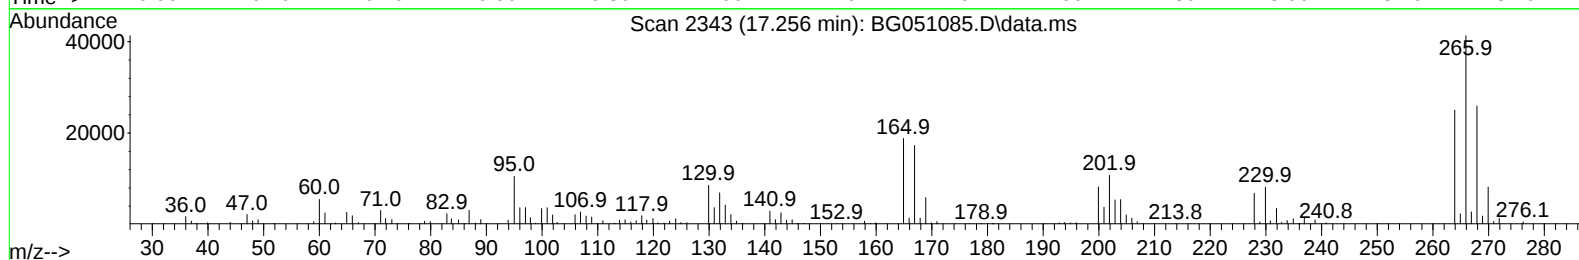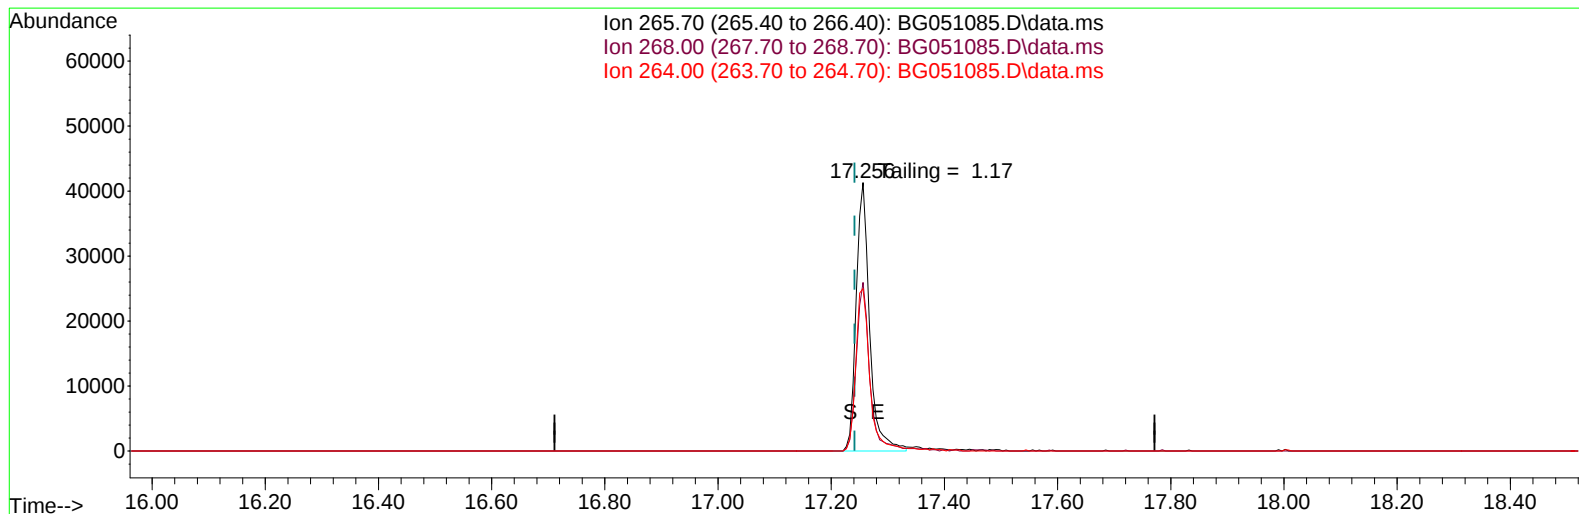

TIC: BG051085.D\data.ms

(70) Pentachlorophenol (C)

17.256min (+ 0.015) 30151.00 ng




response 68626

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.79
264.00	61.30	60.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111721\
Data File : BG051085.D
Acq On : 17 Nov 2021 9:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 17 10:31:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

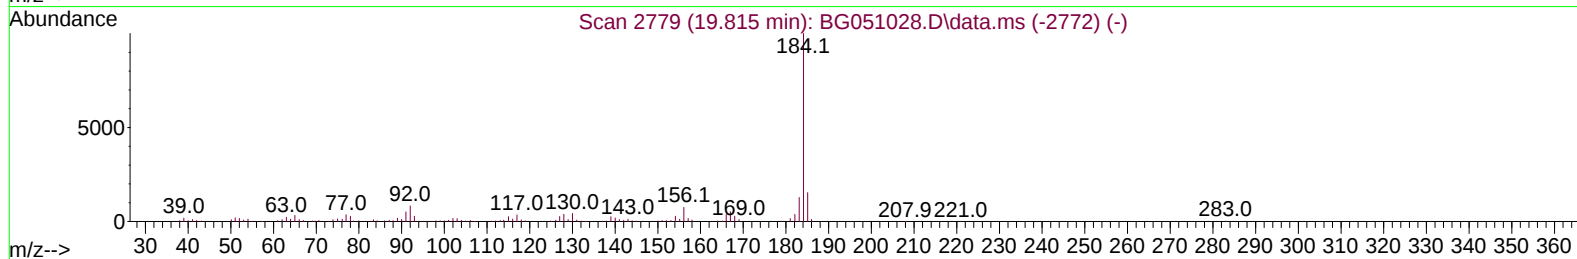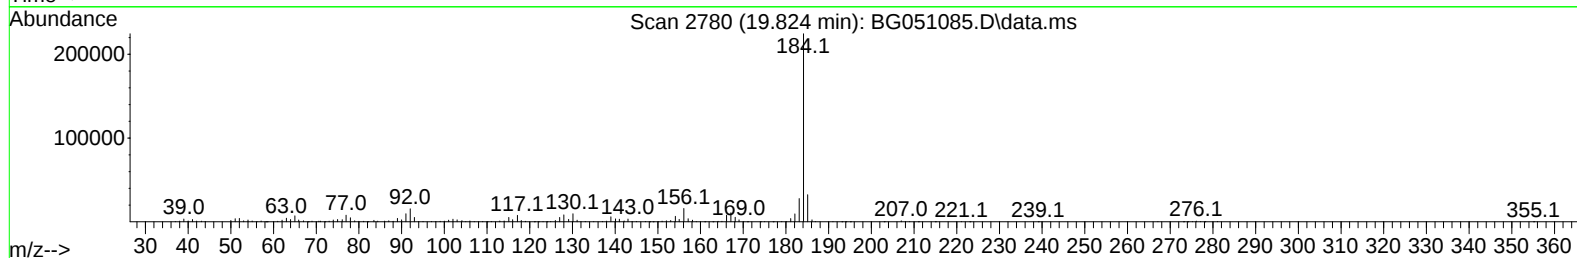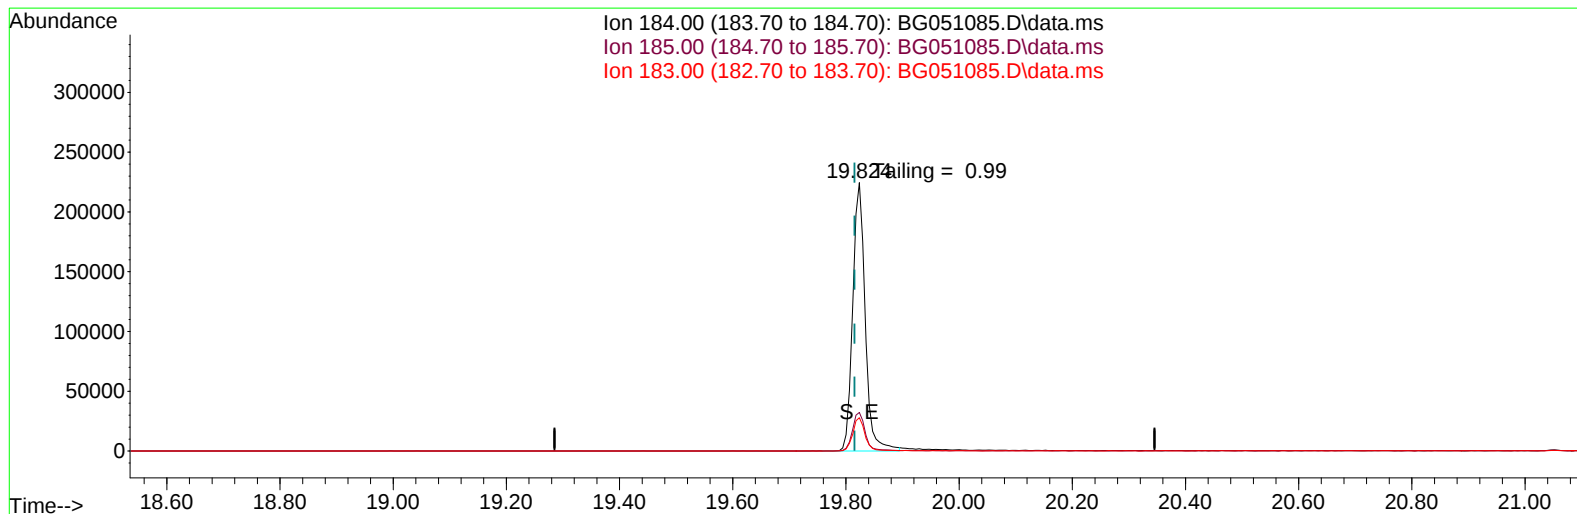

TIC: BG051085.D\data.ms

(77) Benzdine

19.824min (+ 0.009) 330243.18 ng

response 349571

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.41
183.00	11.70	12.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2021	BNA_G	BG051085.D
Compound Name	Response	Retention Time
DDT	182333	21.05
DDD	11617	20.6
DDE	0	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11617	193950	5.99

Instrument :
BNA_G
ClientSampleId :
DFTPP