
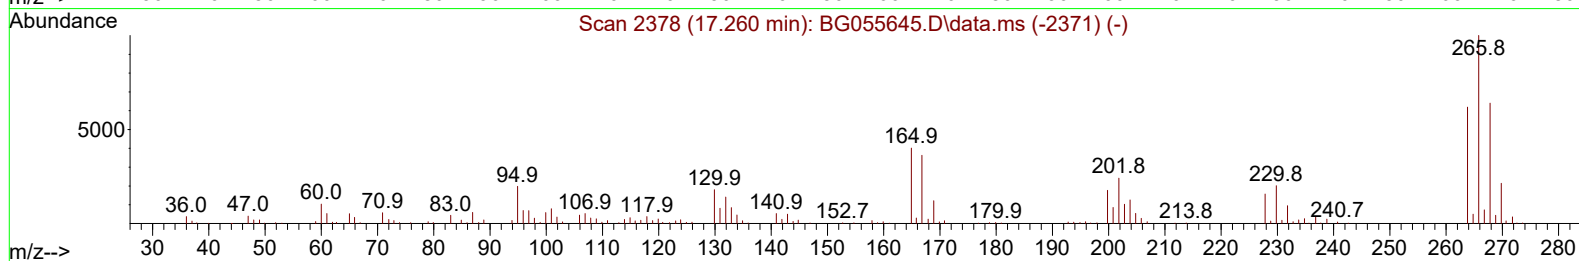
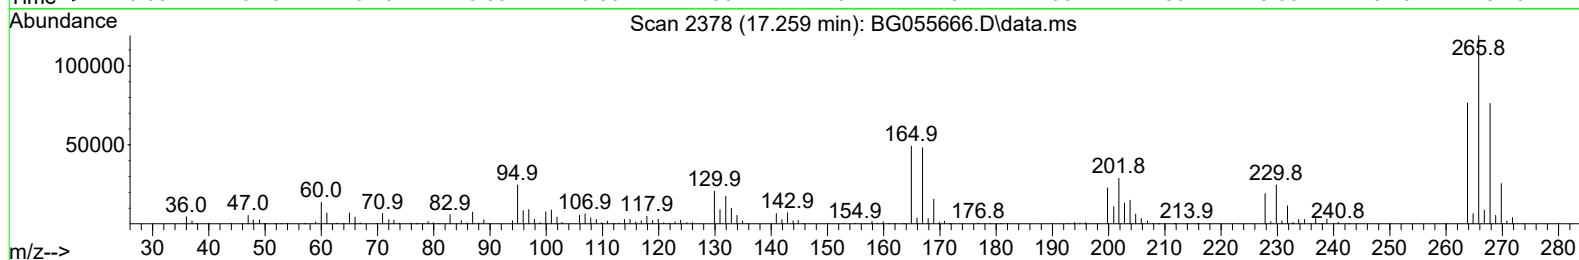


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
Data File : BG055666.D
Acq On : 17 Nov 2022 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 05:41:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

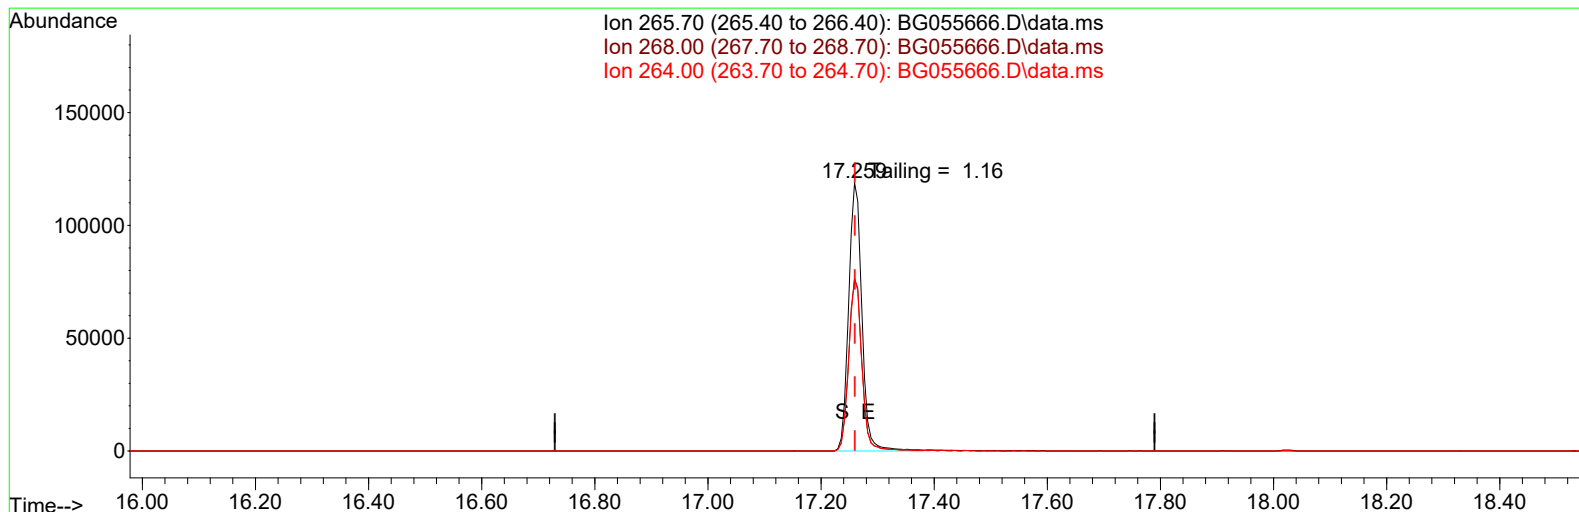

TIC: BG055666.D\data.ms

(70) Pentachlorophenol (C)




17.259min (-0.001) 27923.46 ng

response 194227

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.08
264.00	61.90	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
Data File : BG055666.D
Acq On : 17 Nov 2022 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 05:41:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

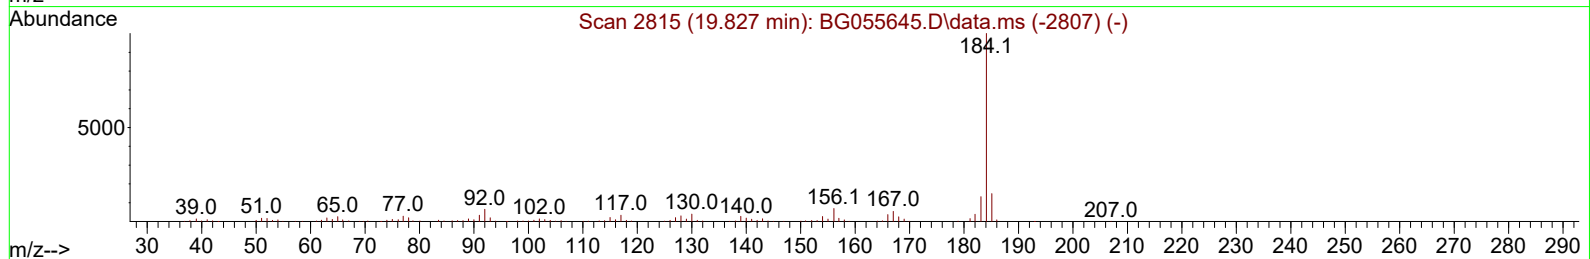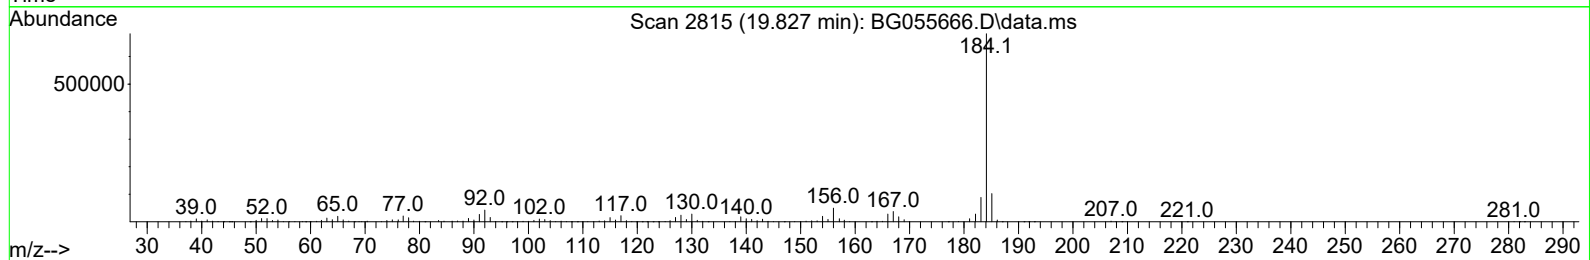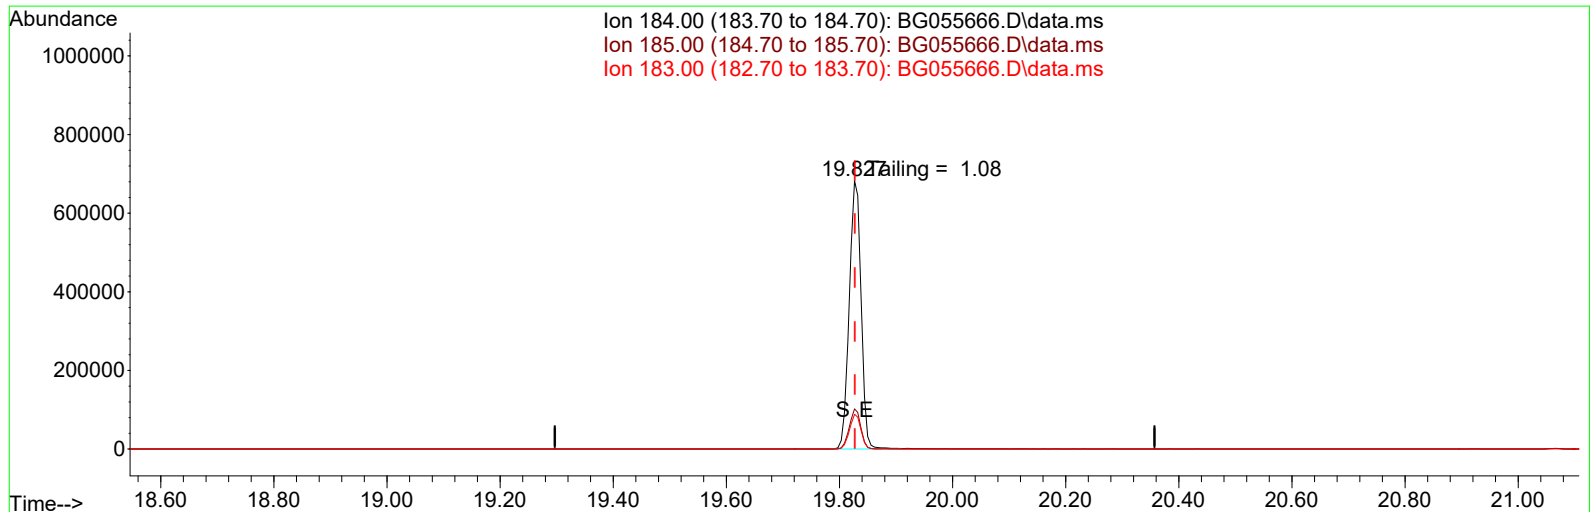

TIC: BG055666.D\data.ms

(77) Benzidine

19.827min (-0.001) 0.00 ng

response 995657

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.00
183.00	13.20	12.96
0.00	0.00	0.00