
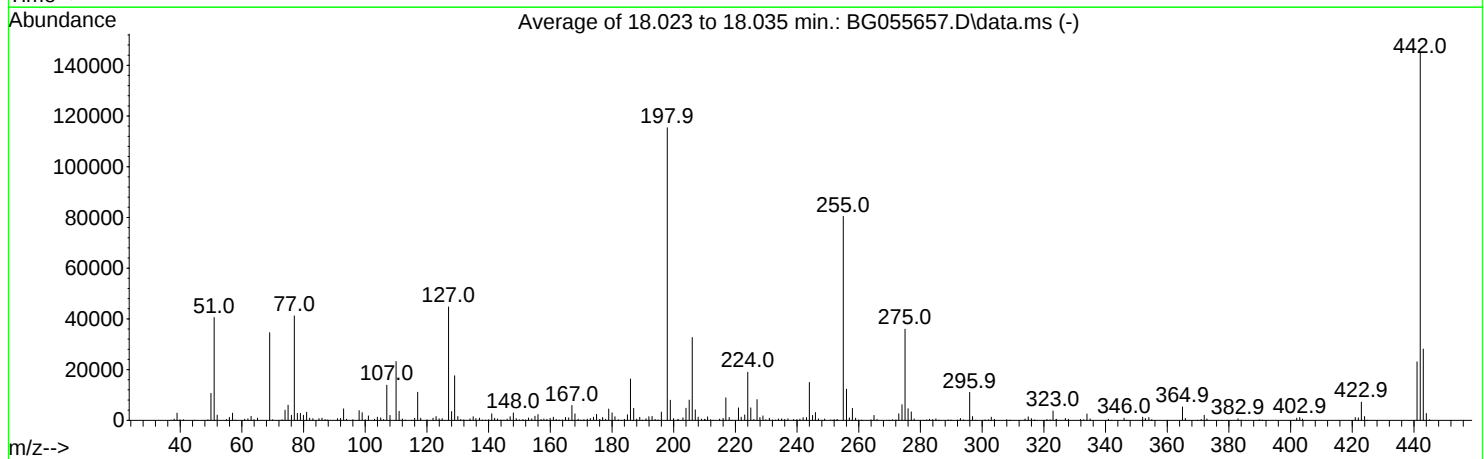


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
Data File : BG055657.D
Acq On : 17 Nov 2022 8:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 17 02:02:46 2022

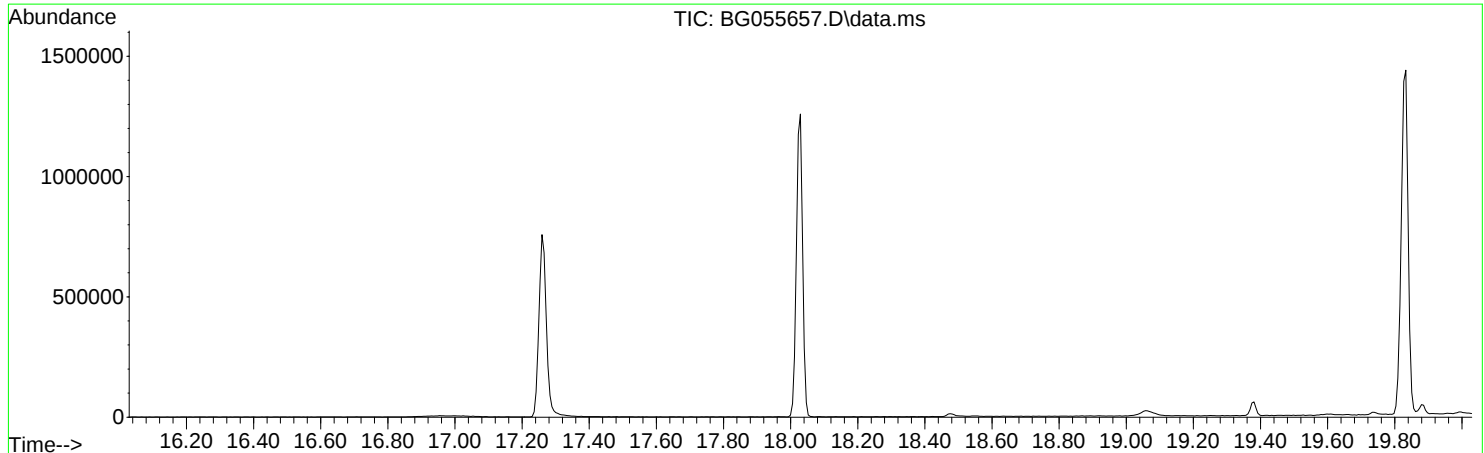




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	40557	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.0	34581	PASS
70	69	0.00	2	0.6	223	PASS
127	198	10	80	38.8	44725	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	115387	PASS
199	198	5	9	6.9	7926	PASS
275	198	10	60	31.1	35936	PASS
365	198	1	100	4.6	5258	PASS
441	198	0.01	100	20.0	23099	PASS
442	442	50	100	100.0	145088	PASS
443	442	15	24	19.4	28091	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
Data File : BG055657.D
Acq On : 17 Nov 2022 8:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 05:40:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

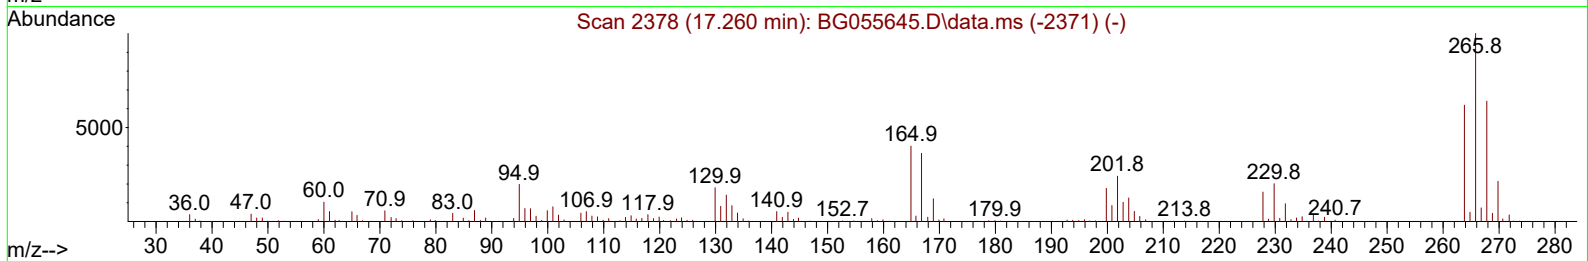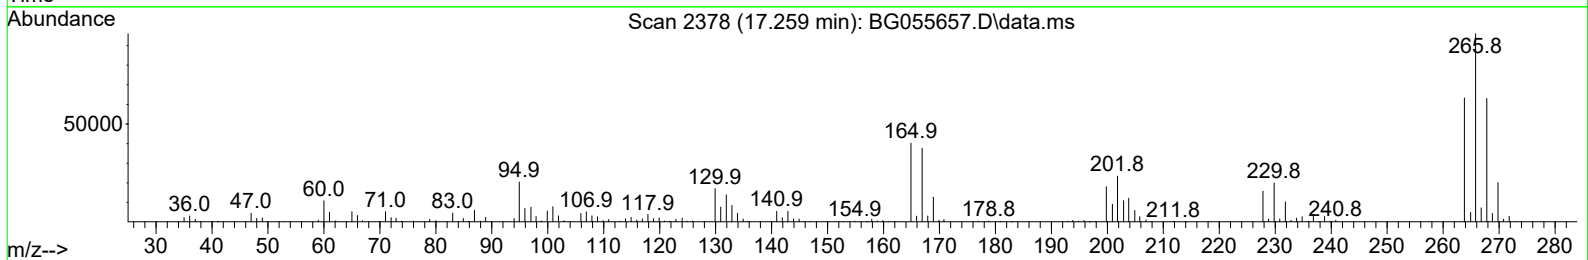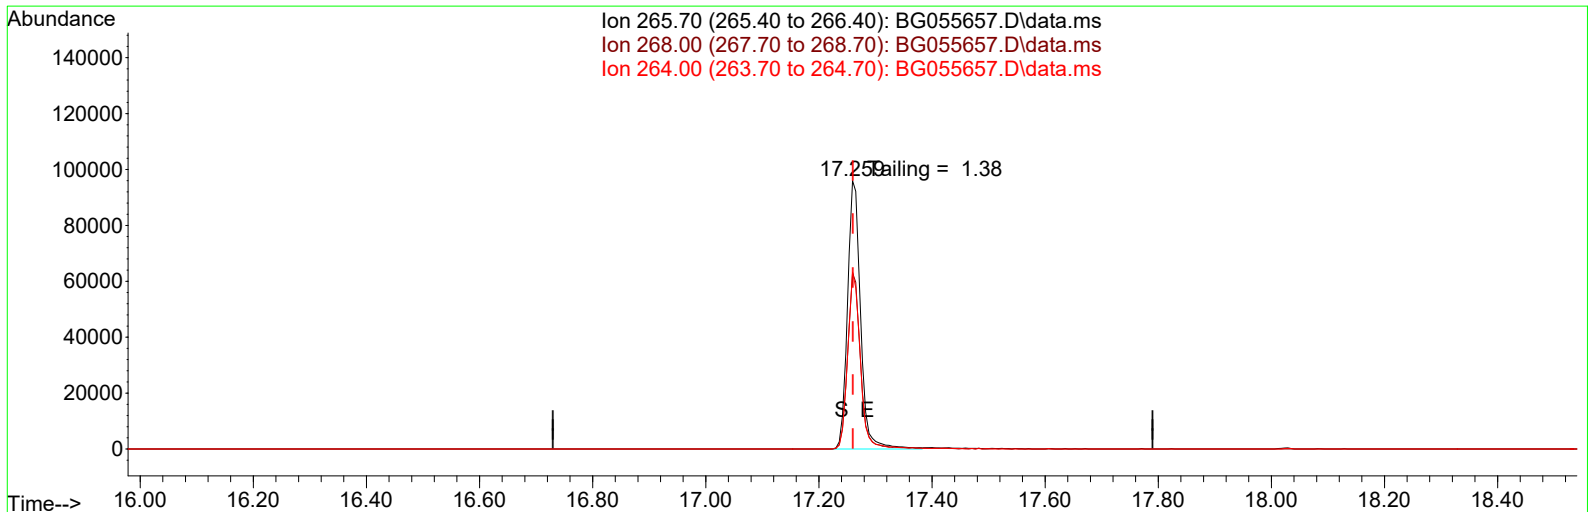

TIC: BG055657.D\data.ms

(70) Pentachlorophenol (C)

17.259min (-0.001) 28063.21 ng




response 154641

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	65.66
264.00	61.90	65.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
Data File : BG055657.D
Acq On : 17 Nov 2022 8:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 05:40:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

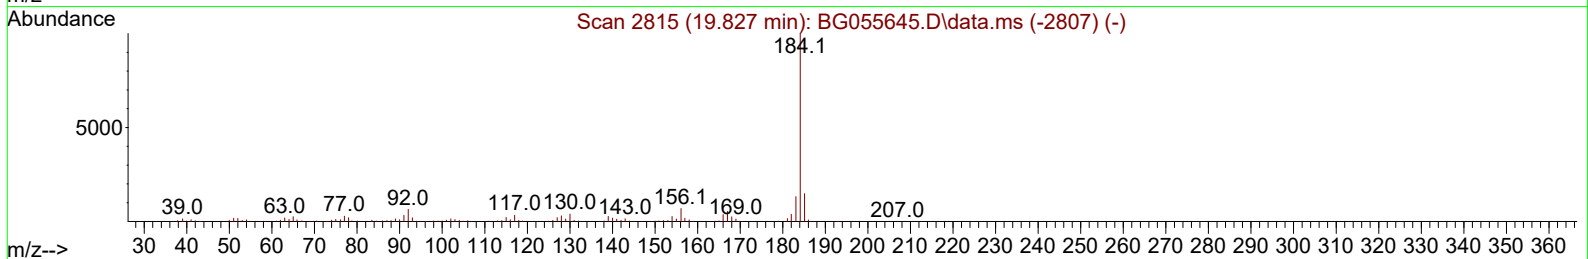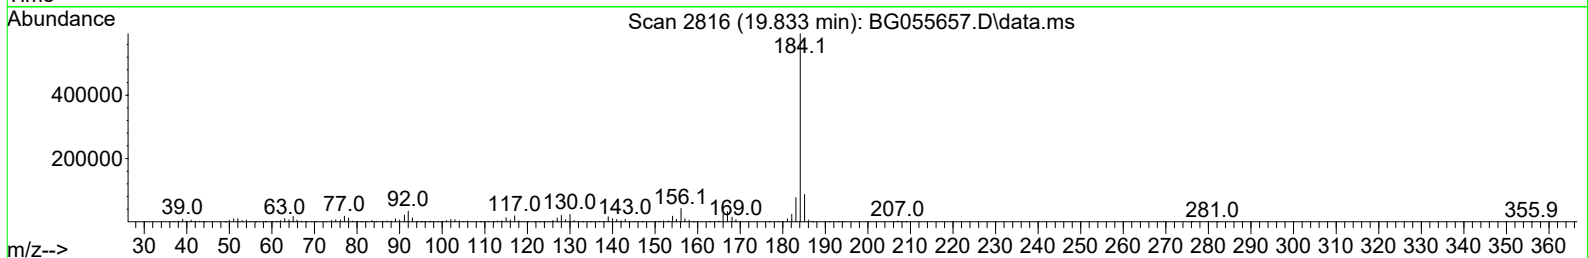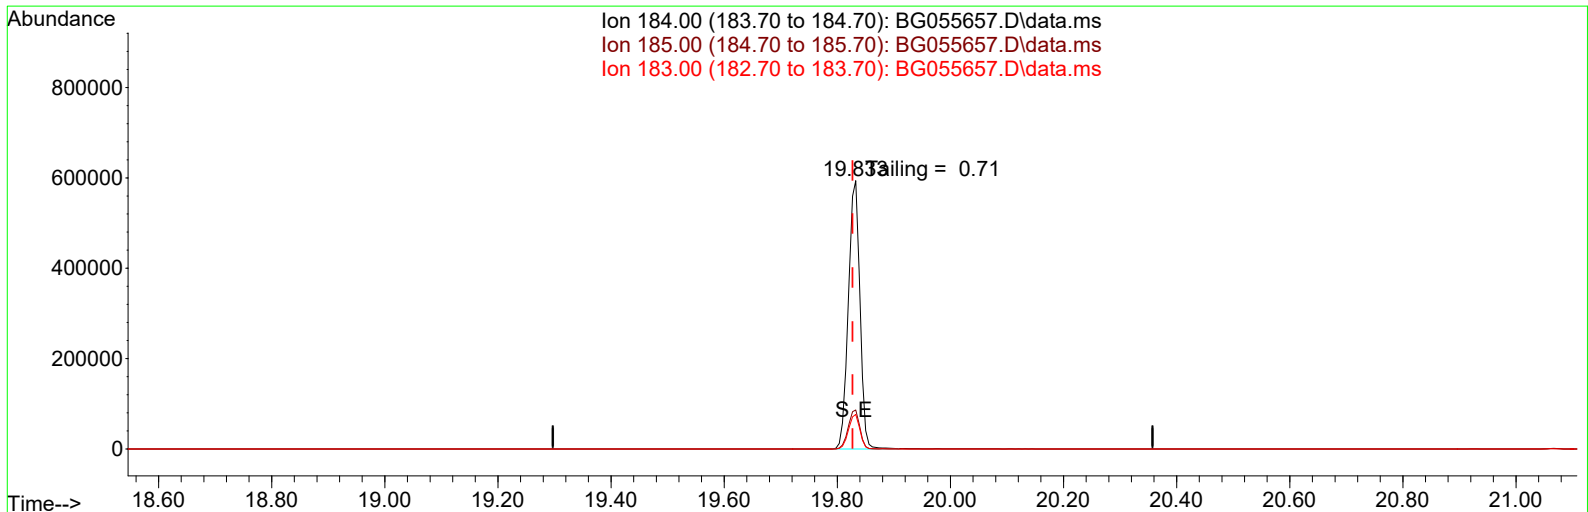

TIC: BG055657.D\data.ms

(77) Benzidine

19.833min (+ 0.005) 593525.46 ng

response 851316

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.56
183.00	13.20	12.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2022	BNA_G	BG055657.D
Compound Name	Response	Retention Time
DDT	415587	21.067
DDD	9337	20.14
DDE	60	20.103
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9397	424984	2.21

Instrument :
BNA_G
ClientSampleId :
DFTPP