
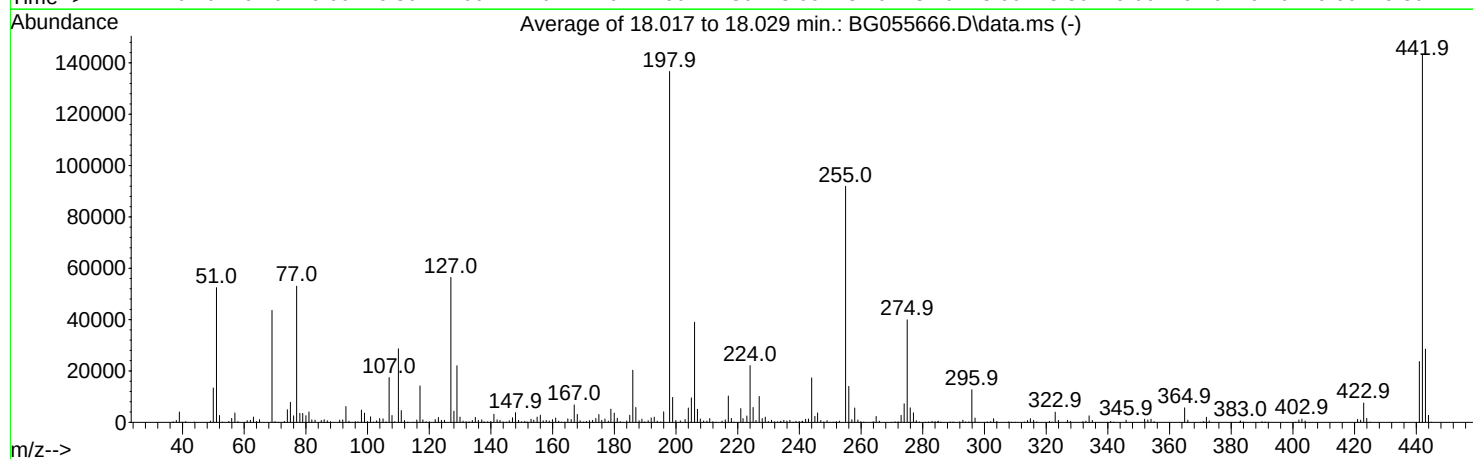


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
 Data File : BG055666.D
 Acq On : 17 Nov 2022 15:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 17 02:02:46 2022

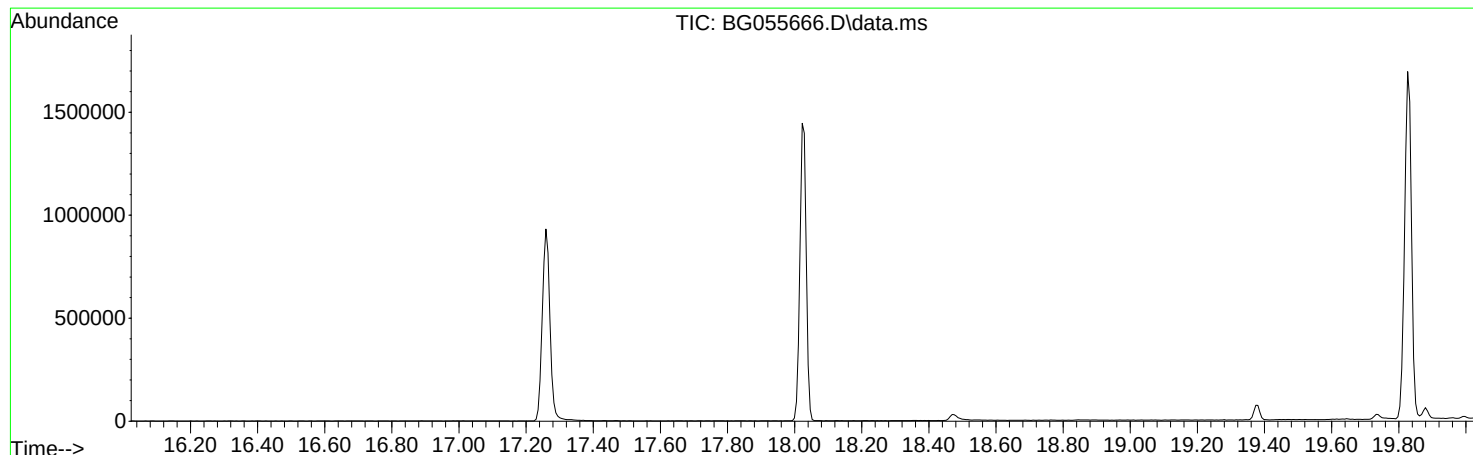




AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	52475	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.9	43576	PASS
70	69	0.00	2	0.7	307	PASS
127	198	10	80	41.3	56469	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136691	PASS
199	198	5	9	7.1	9706	PASS
275	198	10	60	29.2	39931	PASS
365	198	1	100	4.1	5629	PASS
441	198	0.01	100	17.3	23684	PASS
442	442	50	100	100.0	143299	PASS
443	442	15	24	19.9	28547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
Data File : BG055666.D
Acq On : 17 Nov 2022 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 05:41:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

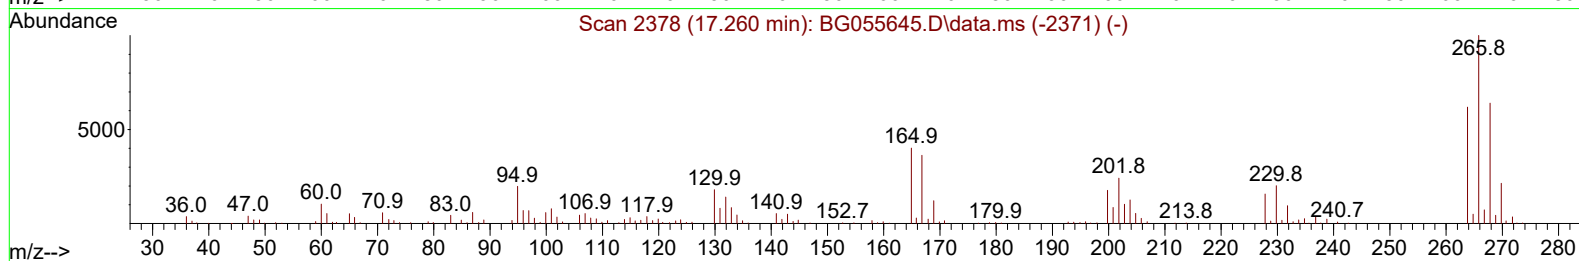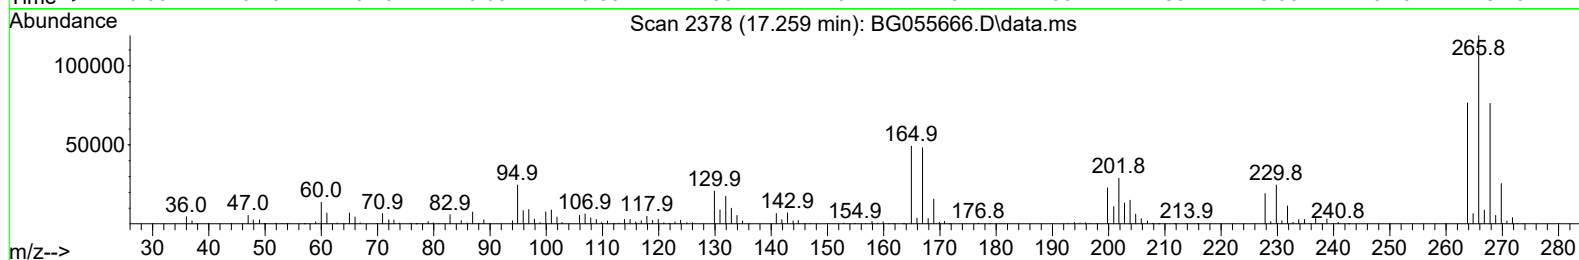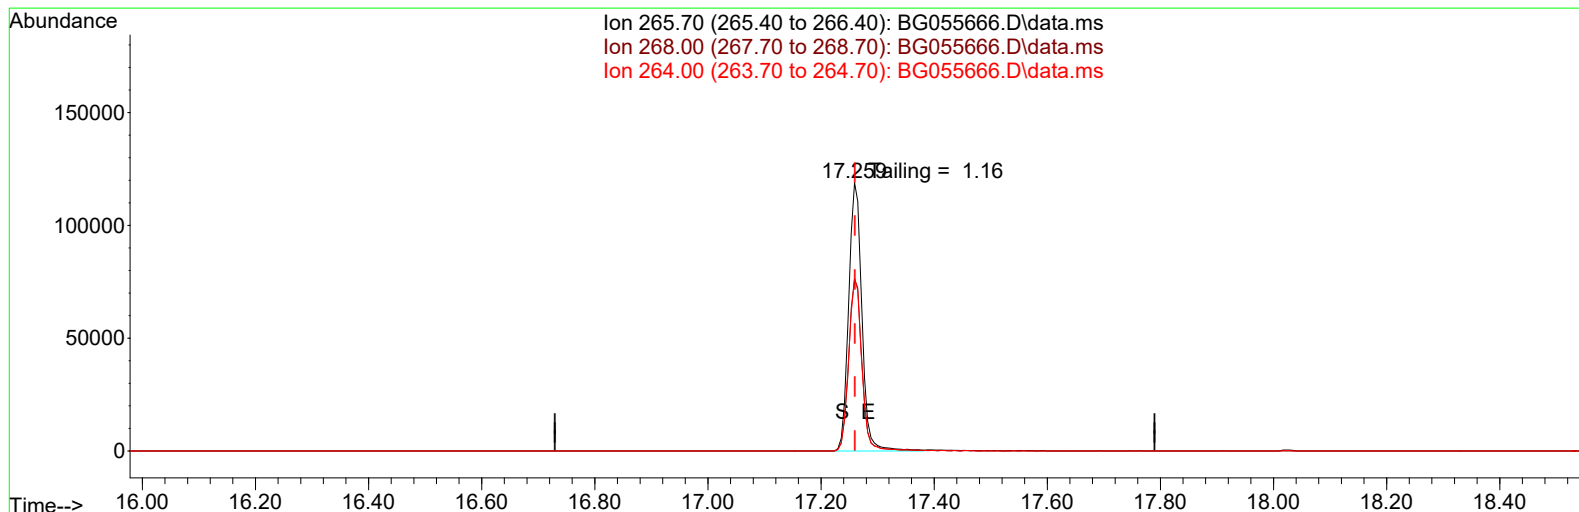

TIC: BG055666.D\data.ms

(70) Pentachlorophenol (C)

17.259min (-0.001) 27923.46 ng




response 194227

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.08
264.00	61.90	64.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111722\
Data File : BG055666.D
Acq On : 17 Nov 2022 15:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 05:41:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

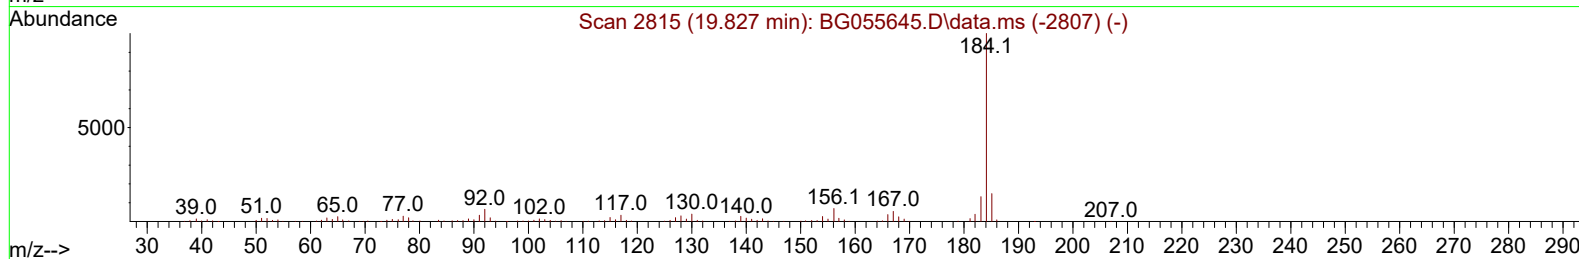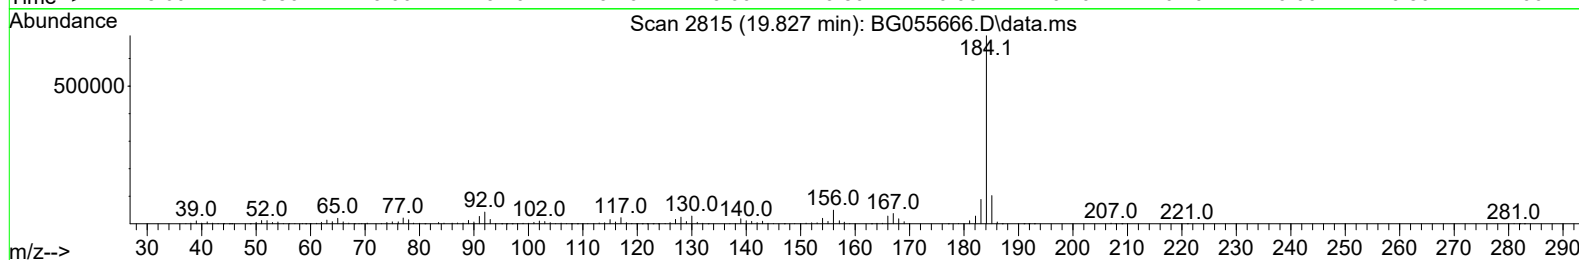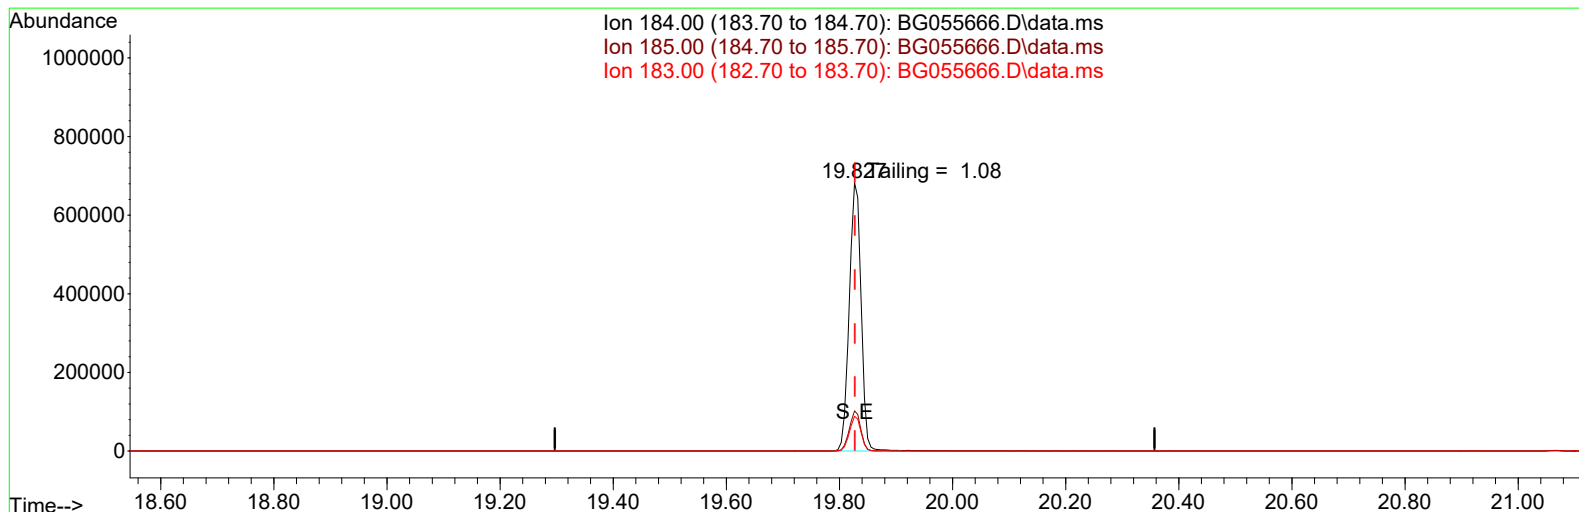

TIC: BG055666.D\data.ms

(77) Benzidine

19.827min (-0.001) 0.00 ng

response 995657

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.00
183.00	13.20	12.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/17/2022	BNA_G	<u>BG055666.D</u>
Compound Name	Response	Retention Time
DDT	496874	21.066
DDD	10965	20.608
DDE	198	20.109
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11163	508037	2.20

Instrument :
BNA_G
ClientSampleId :
DFTPP