
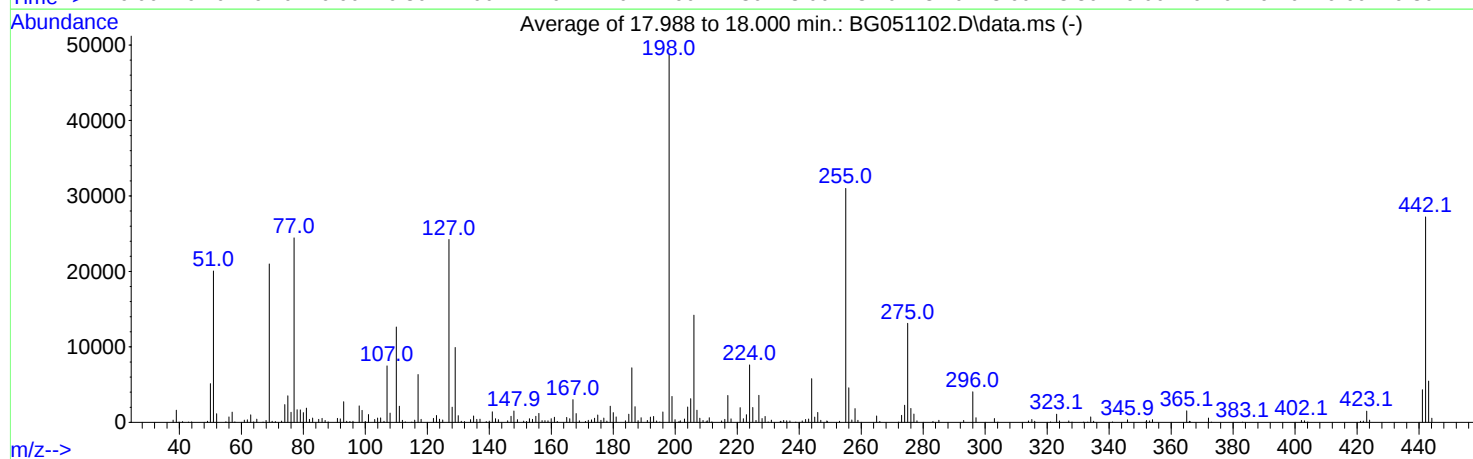


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111821\
 Data File : BG051102.D
 Acq On : 18 Nov 2021 11:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 19 01:16:08 2021

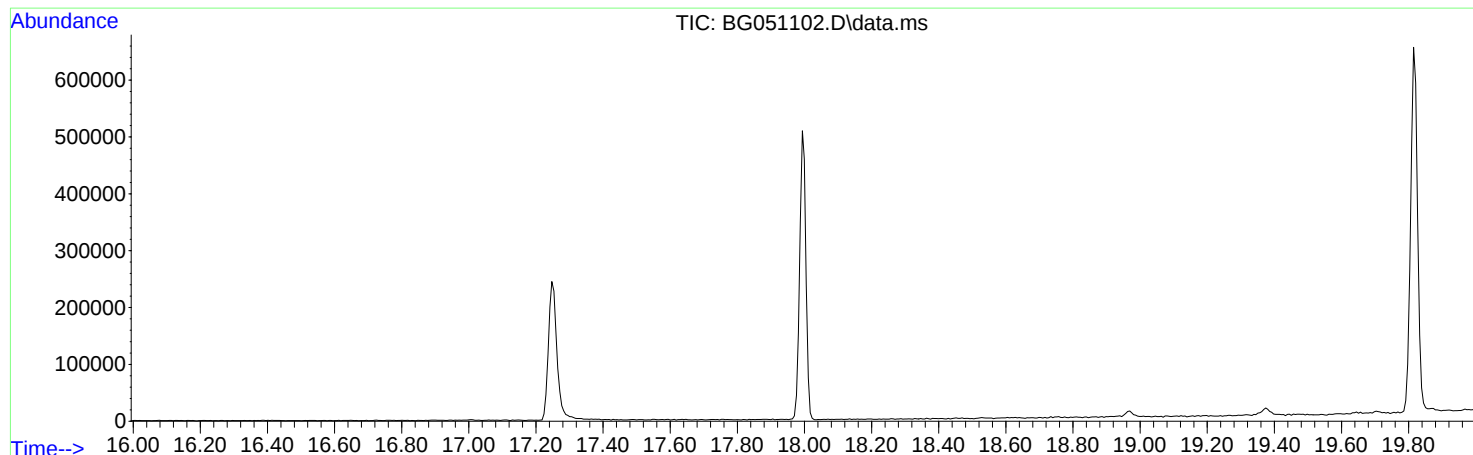




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	20064	PASS
68	69	0.00	2	1.3	264	PASS
69	198	0.00	100	43.0	20979	PASS
70	69	0.00	2	0.7	157	PASS
127	198	10	80	49.7	24237	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48739	PASS
199	198	5	9	7.0	3433	PASS
275	198	10	60	26.9	13117	PASS
365	198	1	100	3.1	1521	PASS
441	198	0.01	100	8.9	4319	PASS
442	442	50	100	100.0	27229	PASS
443	442	15	24	20.1	5478	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111821\
Data File : BG051102.D
Acq On : 18 Nov 2021 11:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 14:30:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

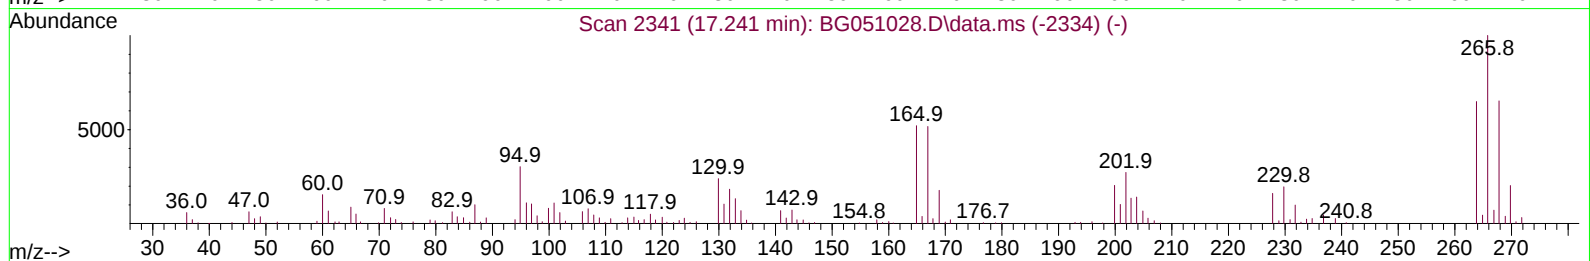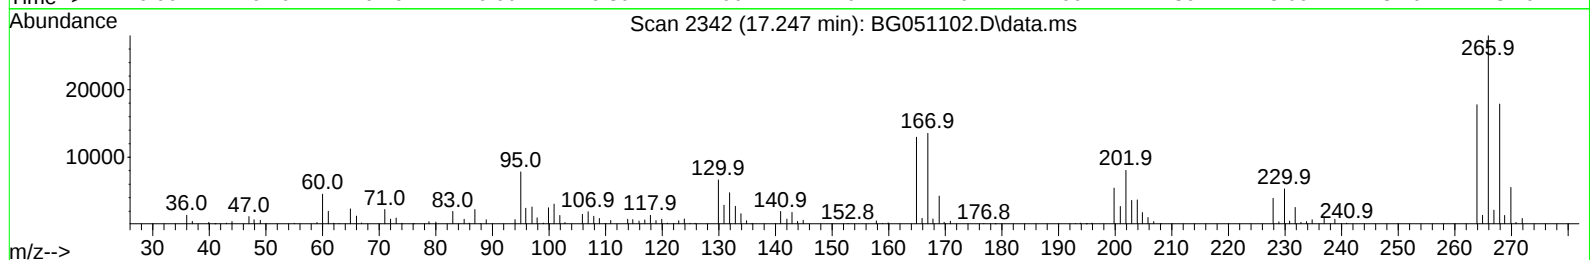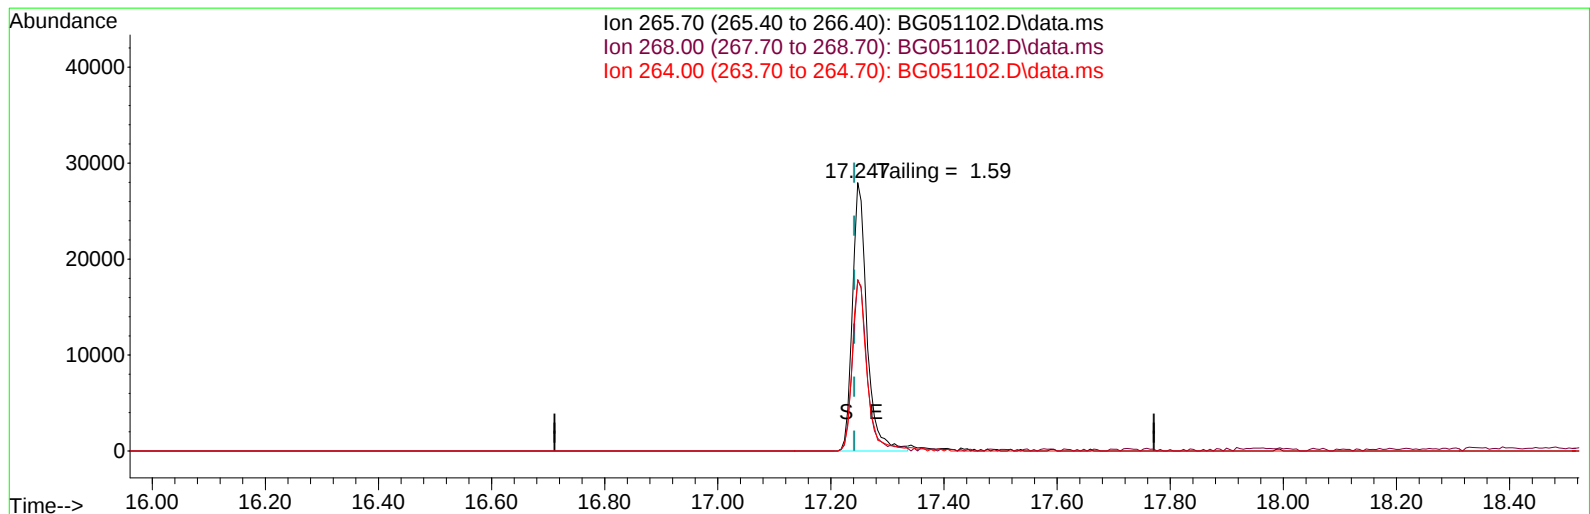

TIC: BG051102.D\data.ms

(70) Pentachlorophenol (C)

17.247min (+ 0.006) 34856.81 ng




response 49560

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.84
264.00	61.30	63.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111821\
Data File : BG051102.D
Acq On : 18 Nov 2021 11:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 18 14:30:58 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 03:55:35 2021
Response via : Initial Calibration

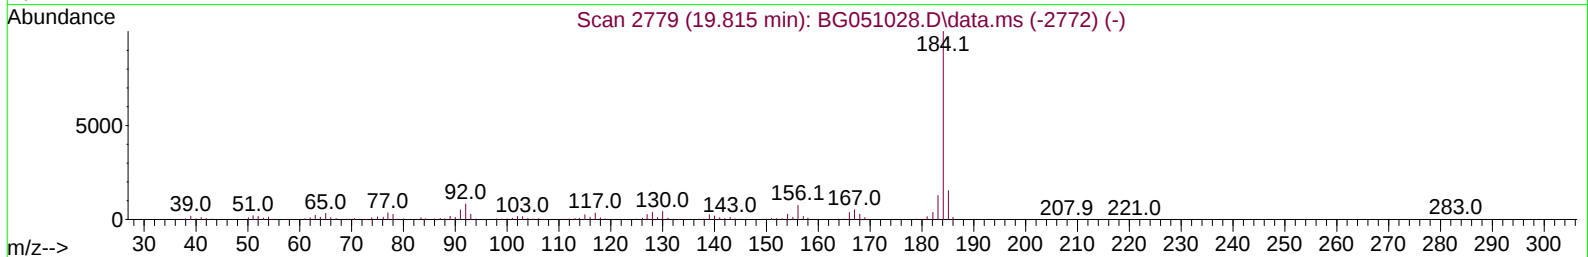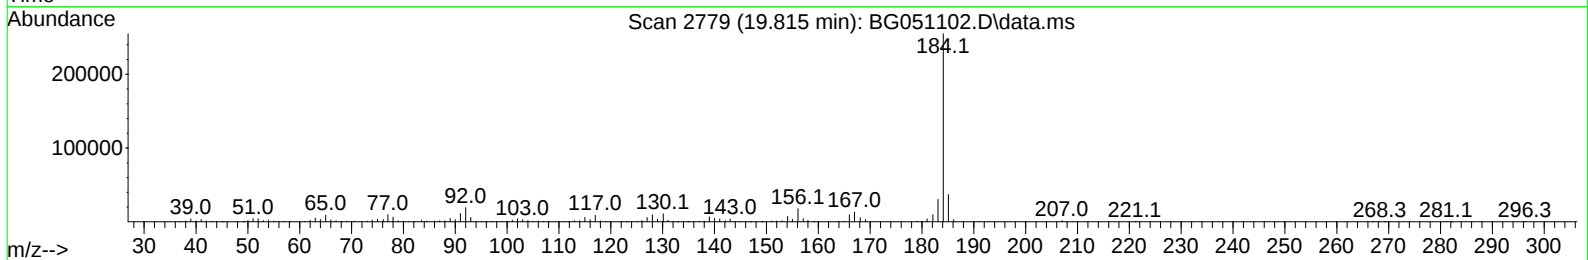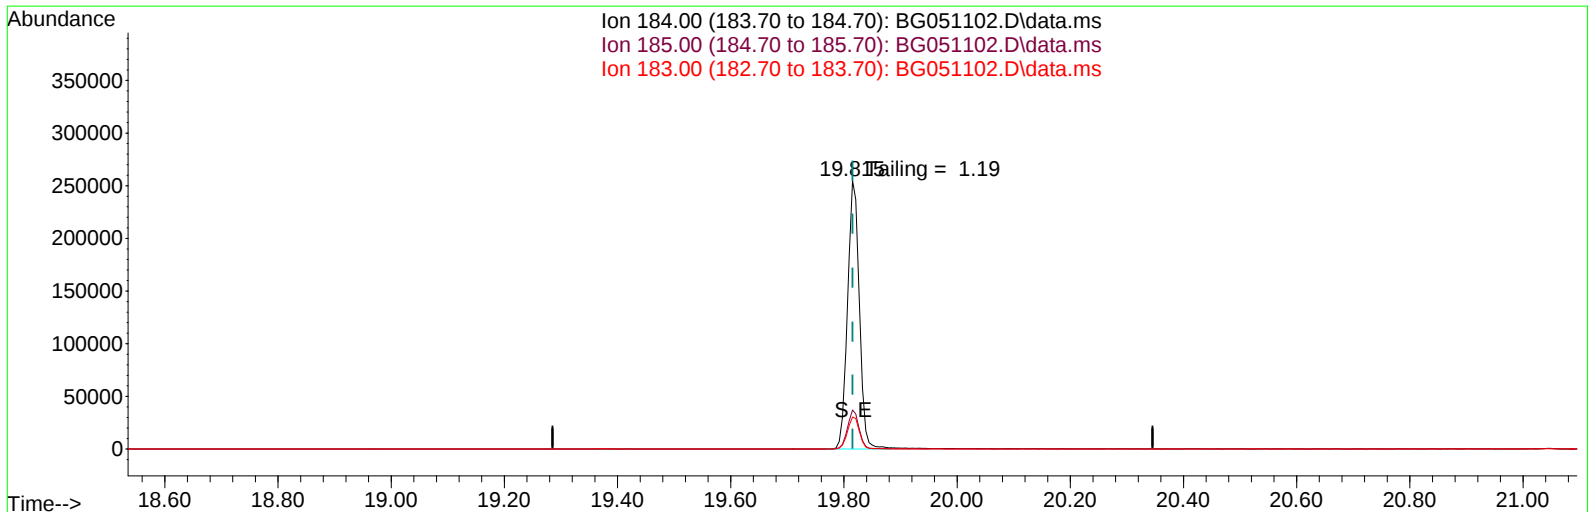

TIC: BG051102.D\data.ms

(77) Benzidine

19.815min (+ 0.000) 345739.02 ng

response 372509

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.55
183.00	11.70	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/18/2021	BNA_G	<u>BG051102.D</u>
Compound Name	Response	Retention Time
DDT	161635	21.04
DDD	2317	20.59
DDE	68	20.08
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2385	164020	1.45

Instrument :
BNA_G
ClientSampleId :
DFTPP