
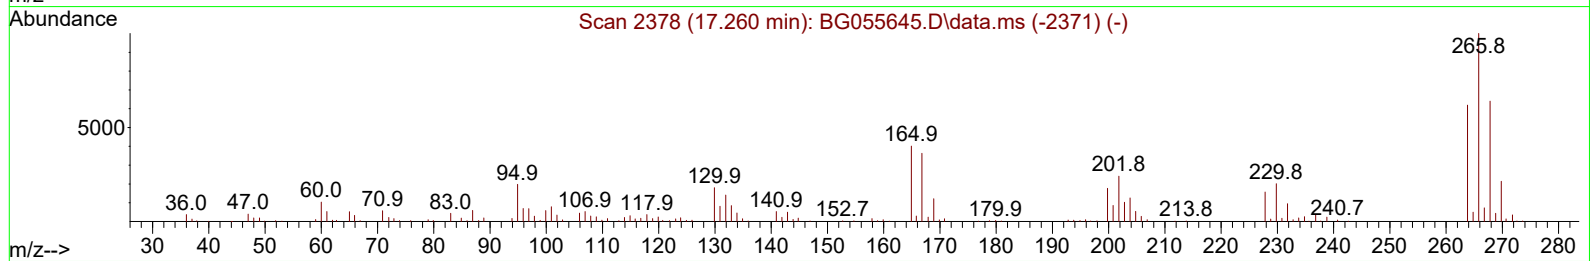
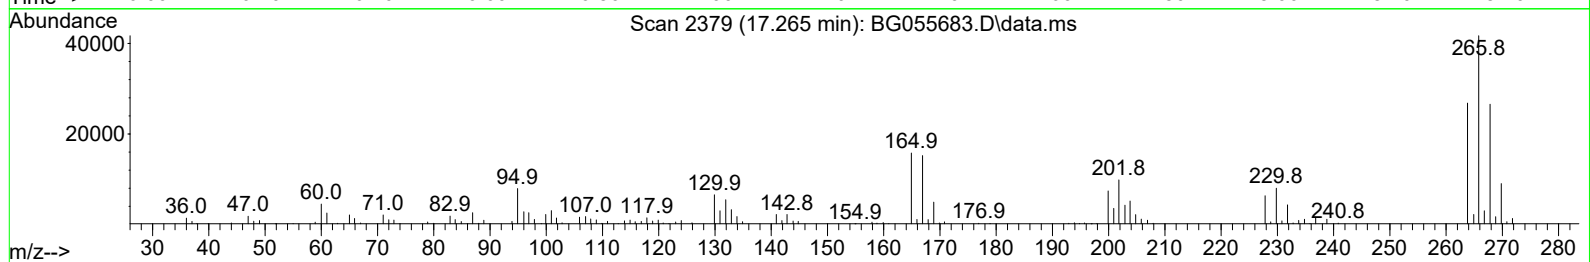


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
 Data File : BG055683.D
 Acq On : 18 Nov 2022 9:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 04:40:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 02:02:46 2022
 Response via : Initial Calibration

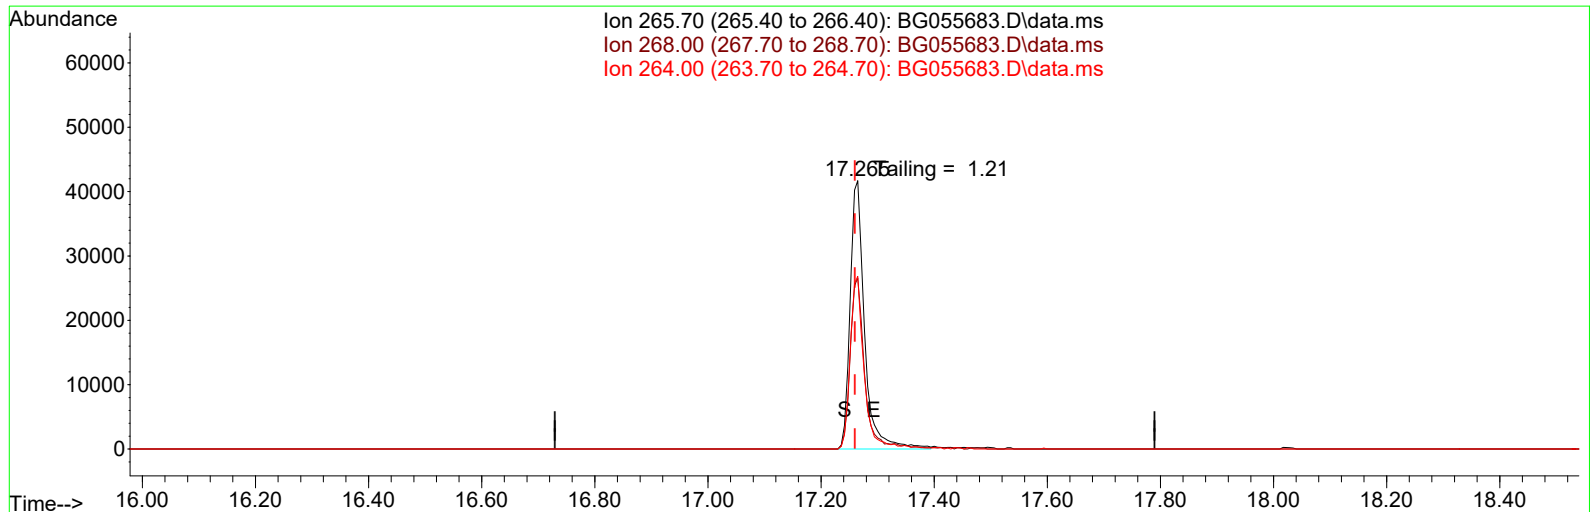

TIC: BG055683.D\data.ms

(70) Pentachlorophenol (C)




17.265min (+ 0.005) 86364.65 ng

response 74757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.74
264.00	61.90	64.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
Data File : BG055683.D
Acq On : 18 Nov 2022 9:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 04:40:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

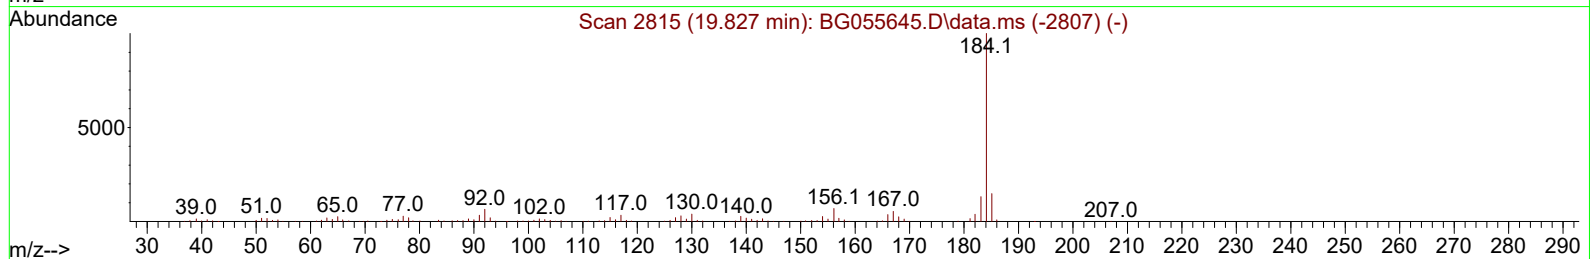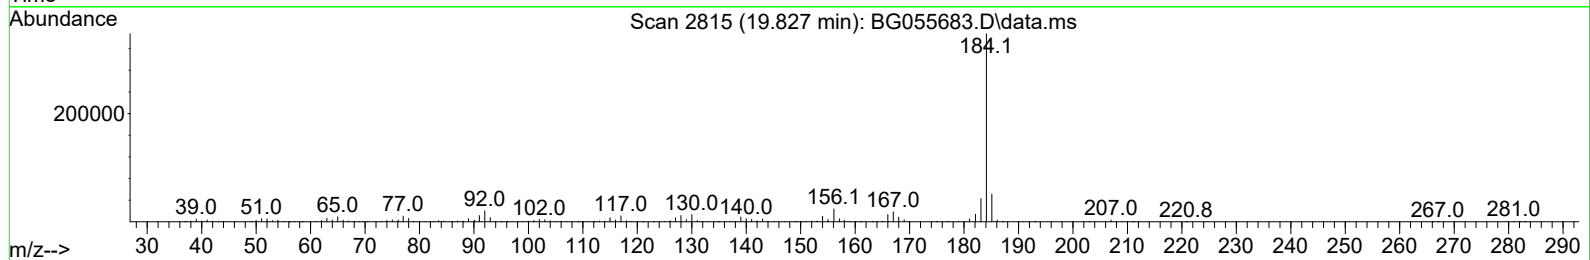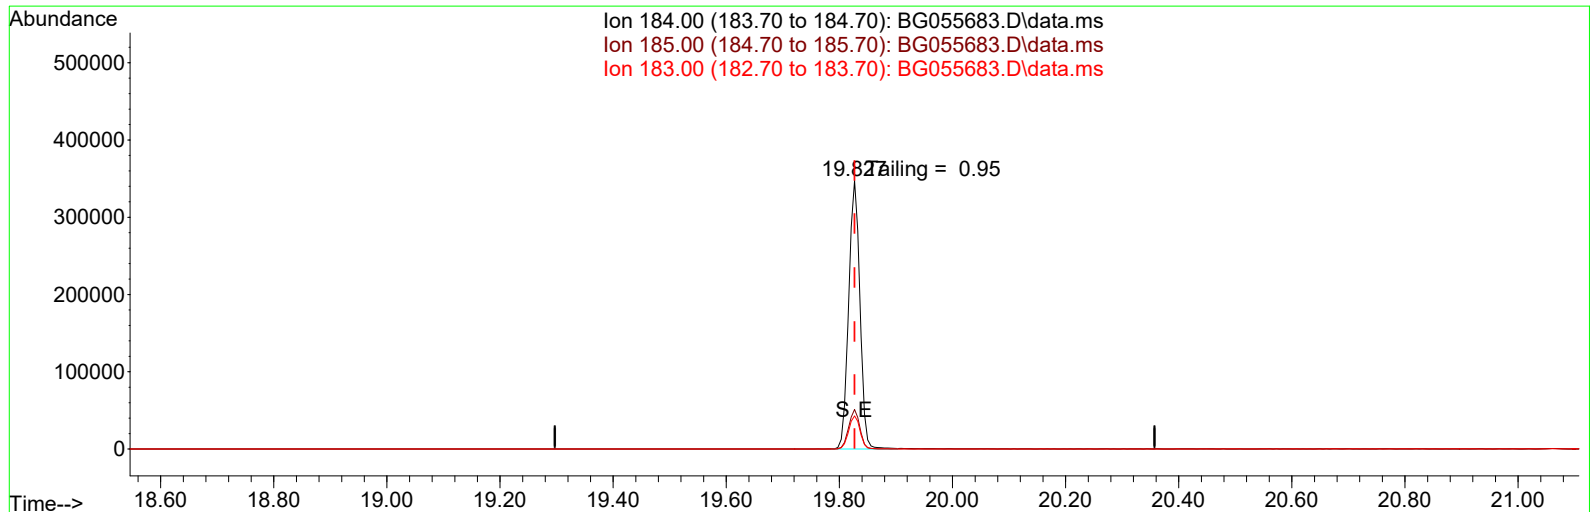

TIC: BG055683.D\data.ms

(77) Benzidine**19.827min (-0.001) 353313.70 ng****response 482250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.74
183.00	13.20	12.38
0.00	0.00	0.00