
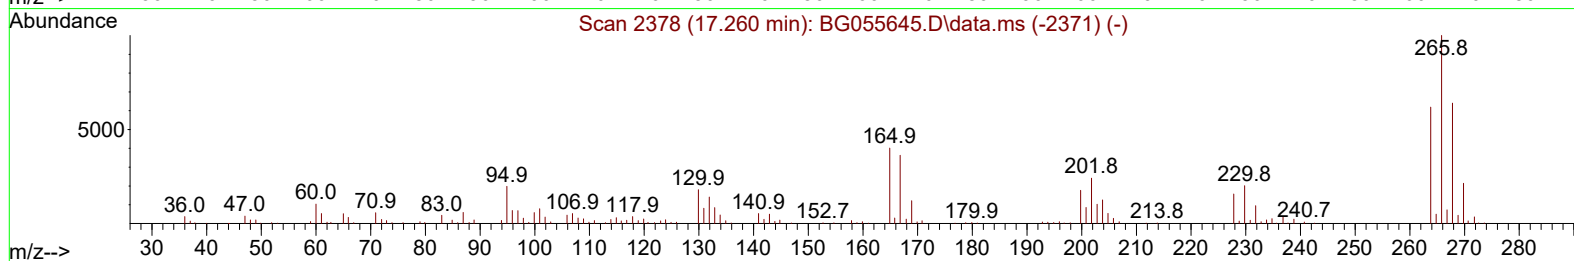
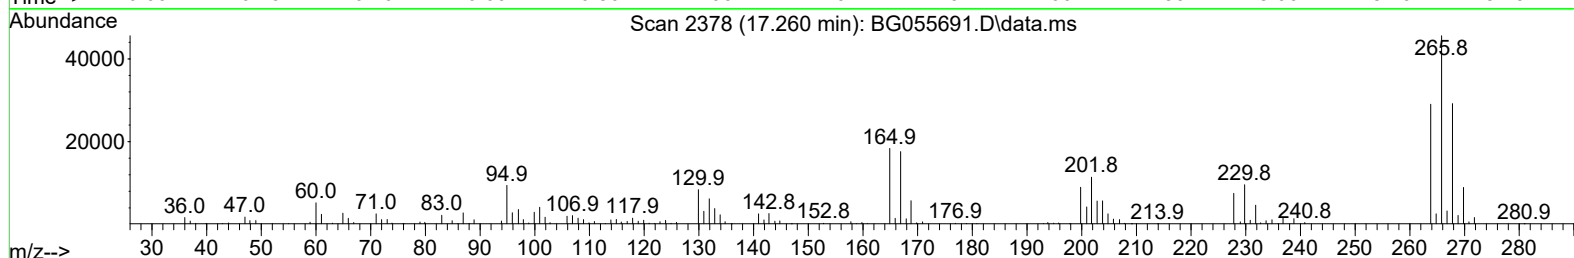


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
Data File : BG055691.D
Acq On : 18 Nov 2022 15:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 04:43:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

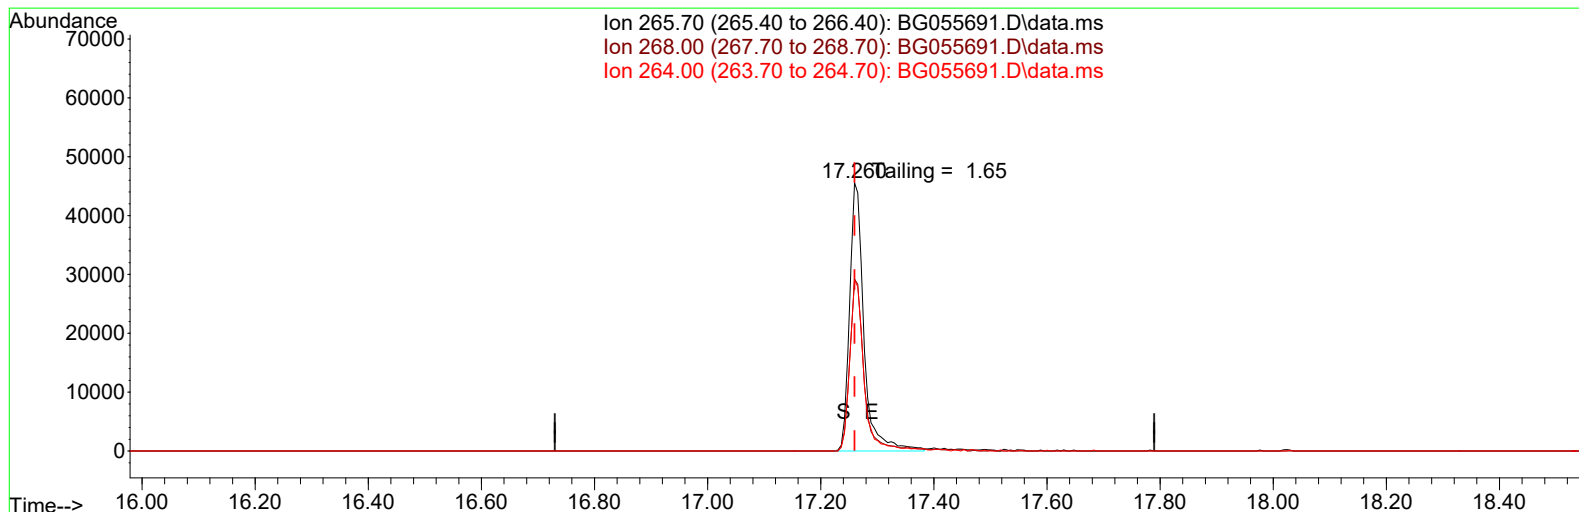

TIC: BG055691.D\data.ms

(70) Pentachlorophenol (C)




17.260min (-0.000) 26251.99 ng

response 80953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.03
264.00	61.90	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
 Data File : BG055691.D
 Acq On : 18 Nov 2022 15:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 04:43:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 02:02:46 2022
 Response via : Initial Calibration

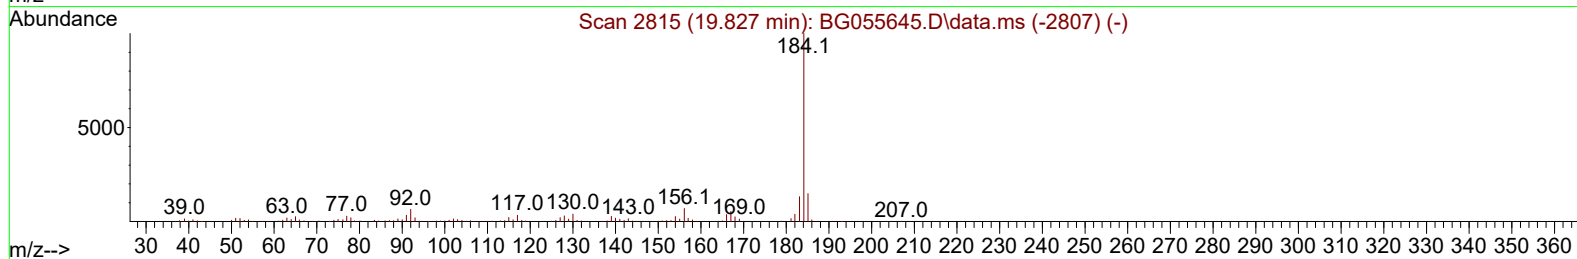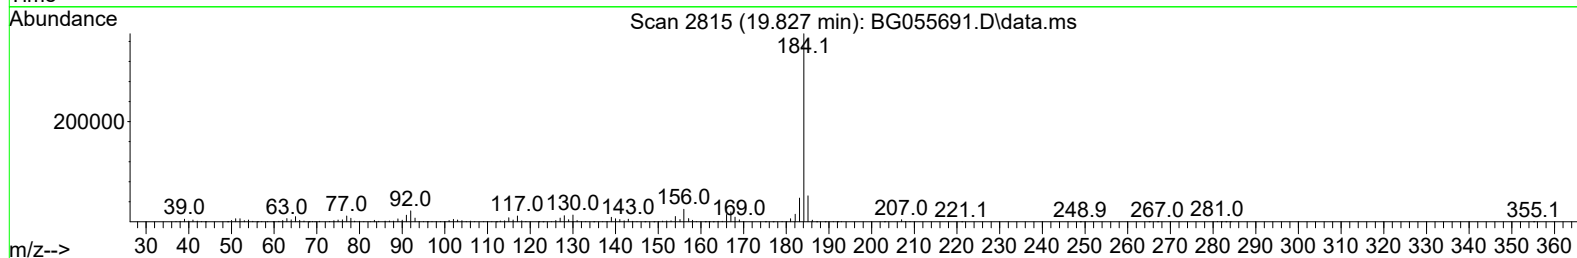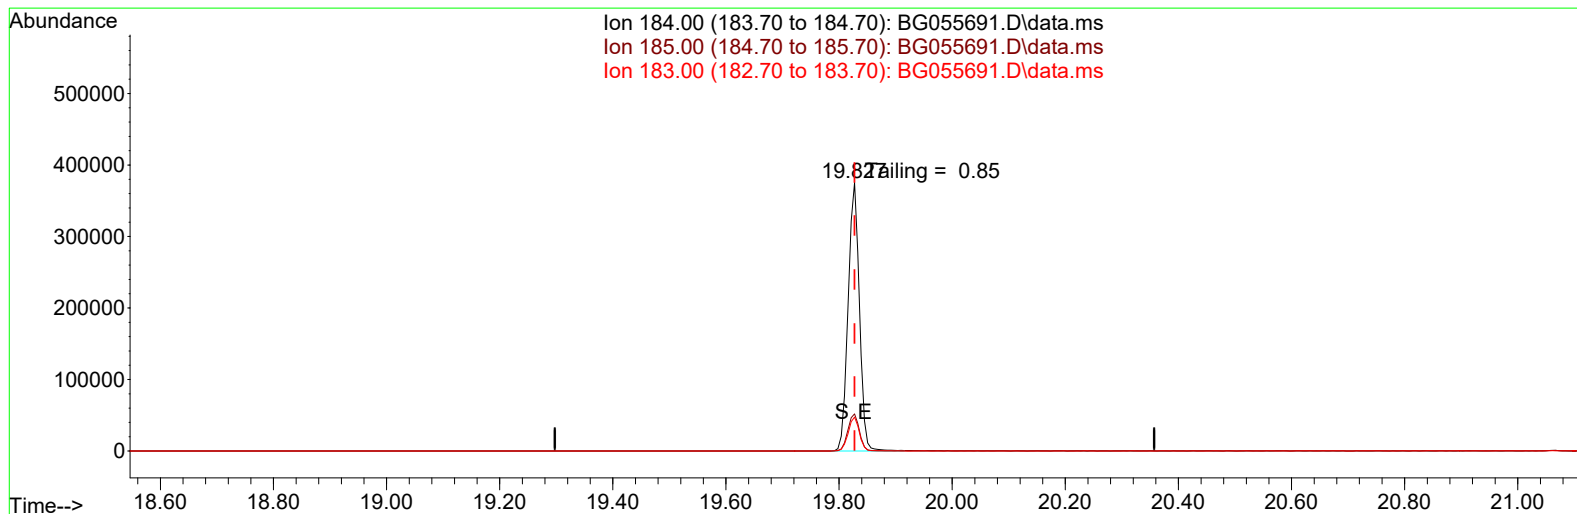

TIC: BG055691.D\data.ms

(77) Benzidine**19.827min (-0.000) 410725.77 ng****response 522606**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.84
183.00	13.20	12.67
0.00	0.00	0.00