


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
 Data File : BG055683.D
 Acq On : 18 Nov 2022 9:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 17 02:02:46 2022

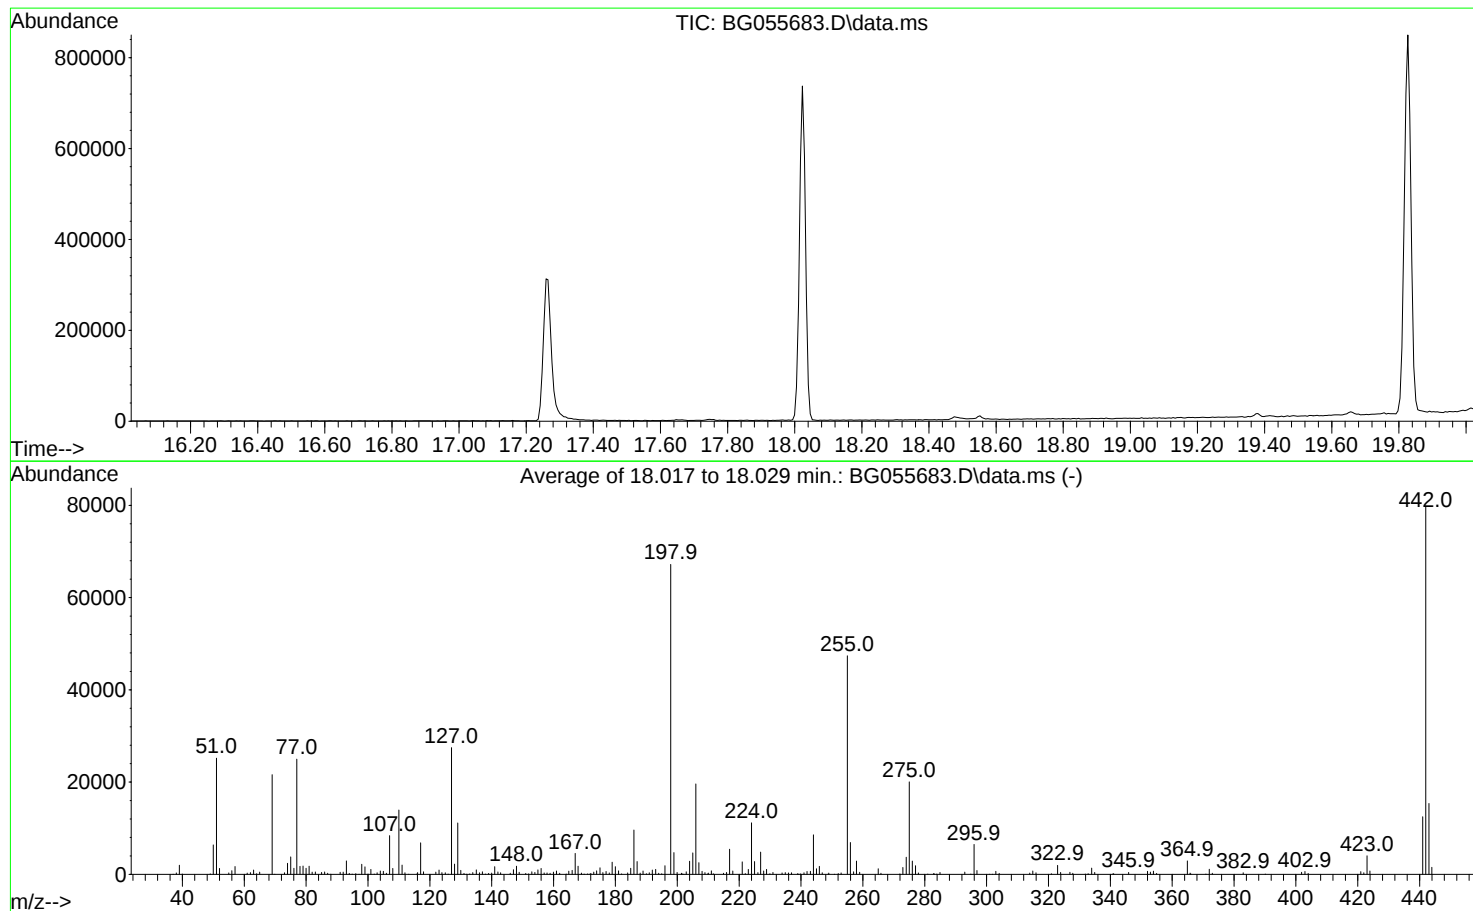

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	25179	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.2	21616	PASS
70	69	0.00	2	0.3	55	PASS
127	198	10	80	40.9	27491	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67203	PASS
199	198	5	9	7.0	4737	PASS
275	198	10	60	29.8	20059	PASS
365	198	1	100	4.3	2912	PASS
441	198	0.01	100	18.6	12482	PASS
442	442	50	100	100.0	79752	PASS
443	442	15	24	19.3	15385	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/18/2022	BNA_G	BG055683.D
Compound Name	Response	Retention Time
DDT	217075	21.066
DDD	6393	20.608
DDE	0	20.109
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6393	223468	2.86

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
Data File : BG055683.D
Acq On : 18 Nov 2022 9:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 19 04:40:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

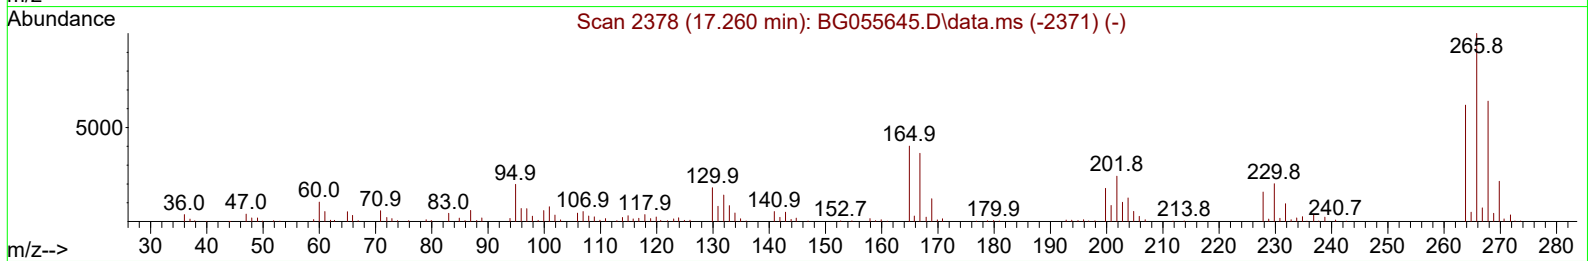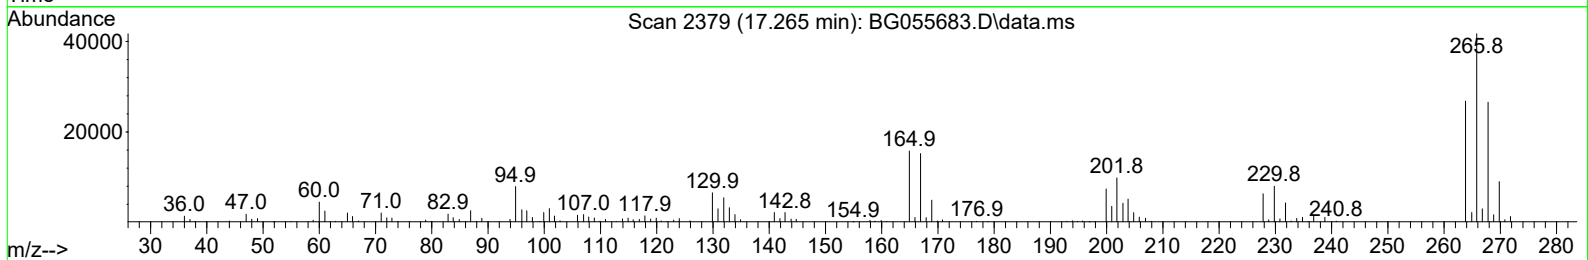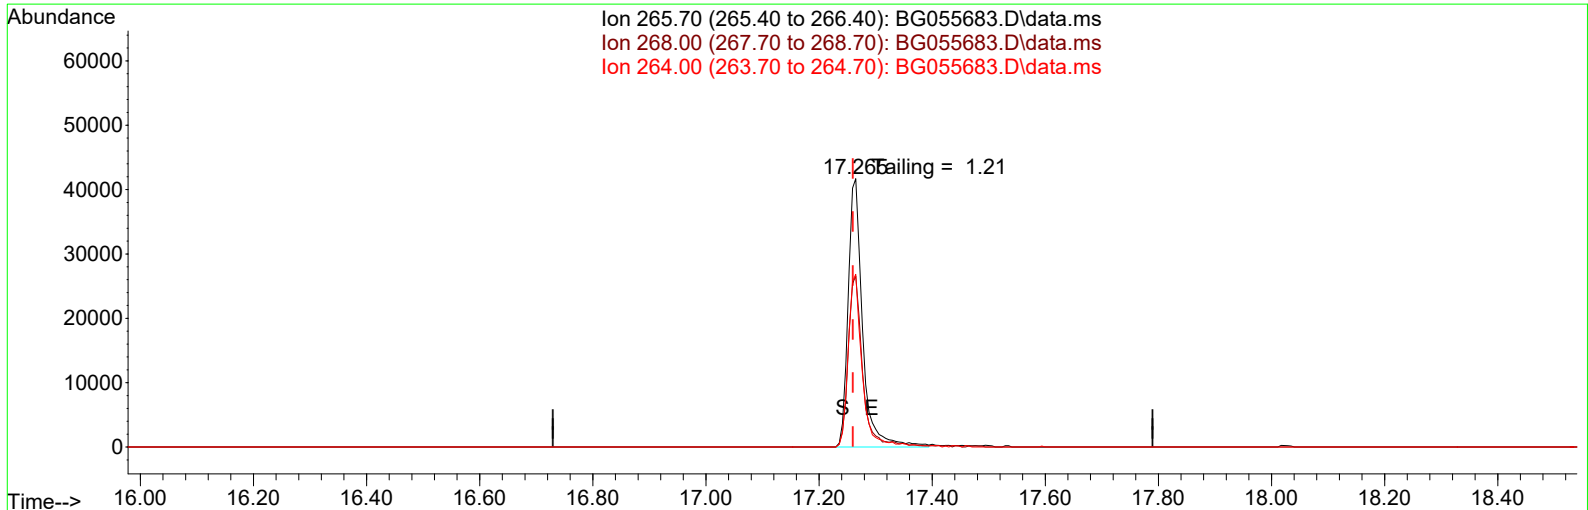

TIC: BG055683.D\data.ms

(70) Pentachlorophenol (C)

17.265min (+ 0.005) 86364.65 ng




response 74757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.74
264.00	61.90	64.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
Data File : BG055683.D
Acq On : 18 Nov 2022 9:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 19 04:40:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

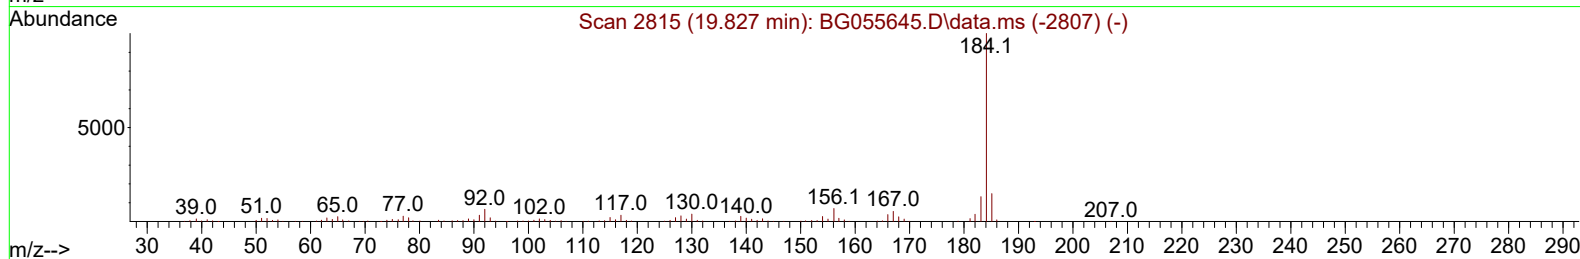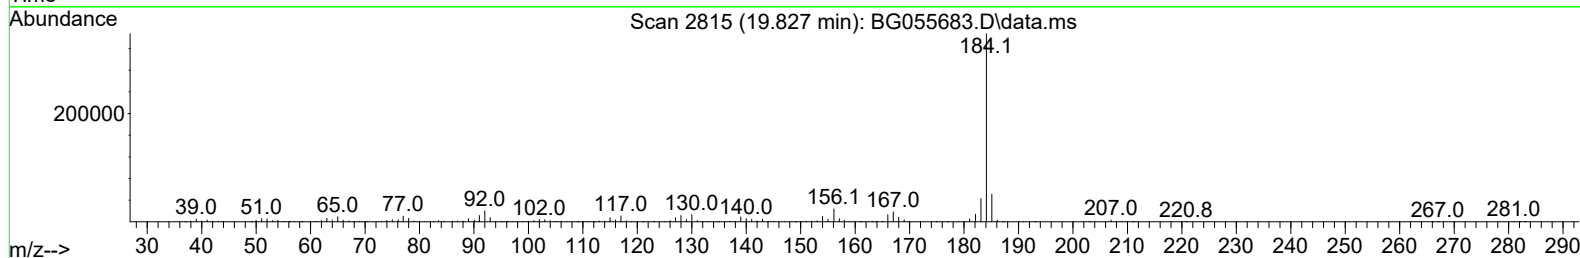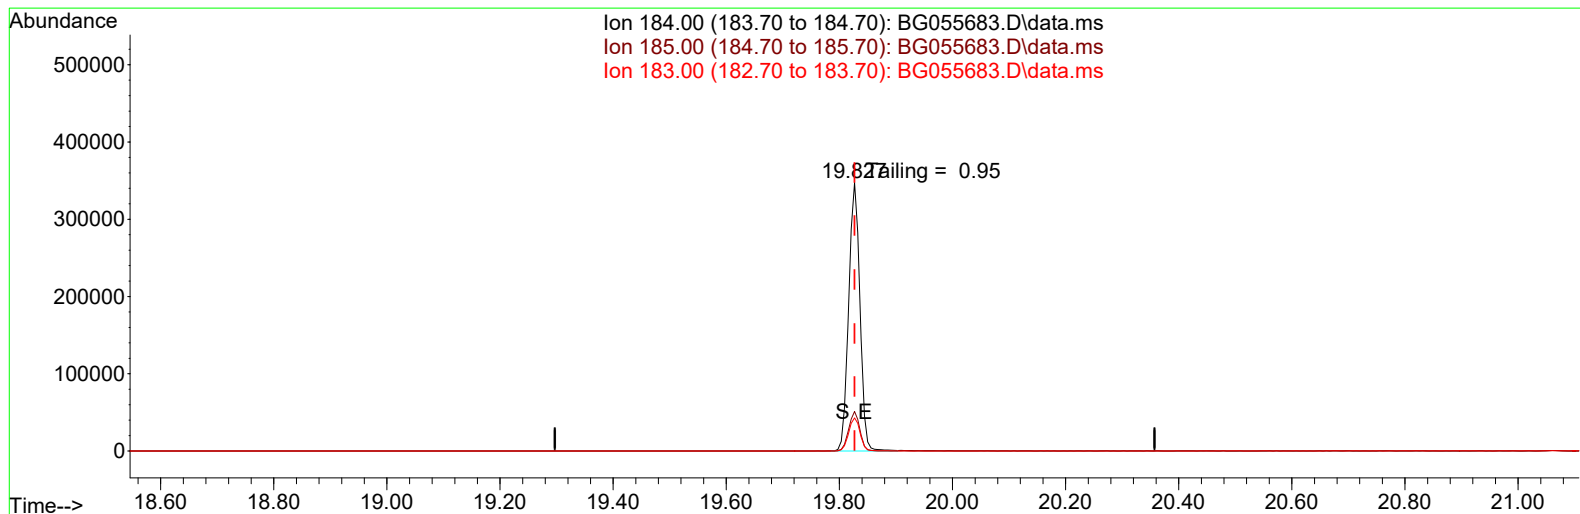

TIC: BG055683.D\data.ms

(77) Benzidine

19.827min (-0.001) 353313.70 ng

response 482250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.74
183.00	13.20	12.38
0.00	0.00	0.00