
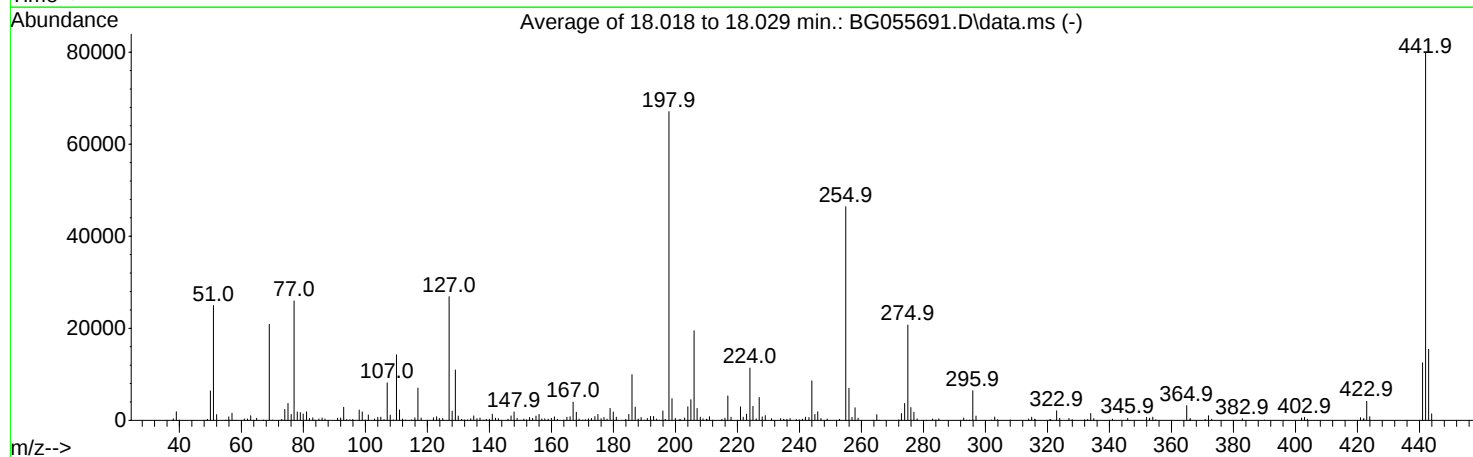


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
 Data File : BG055691.D
 Acq On : 18 Nov 2022 15:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 17 02:02:46 2022

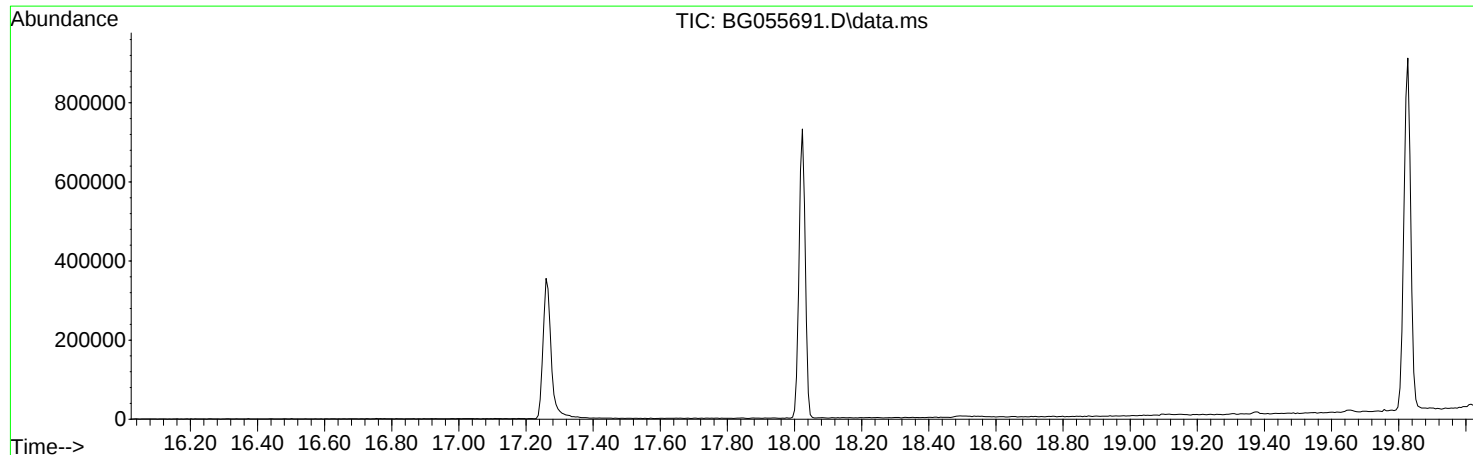

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	24957	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.1	20845	PASS
70	69	0.00	2	0.3	71	PASS
127	198	10	80	40.0	26861	PASS
197	198	0.00	2	0.3	230	PASS
198	198	100	100	100.0	67093	PASS
199	198	5	9	7.1	4739	PASS
275	198	10	60	30.9	20725	PASS
365	198	1	100	4.8	3216	PASS
441	198	0.01	100	18.6	12504	PASS
442	442	50	100	100.0	79923	PASS
443	442	15	24	19.3	15440	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/18/2022	BNA_G	BG055691.D
Compound Name	Response	Retention Time
DDT	240917	21.061
DDD	7503	20.609
DDE	373	20.109
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7876	248793	3.17

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
Data File : BG055691.D
Acq On : 18 Nov 2022 15:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 19 04:43:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 02:02:46 2022
Response via : Initial Calibration

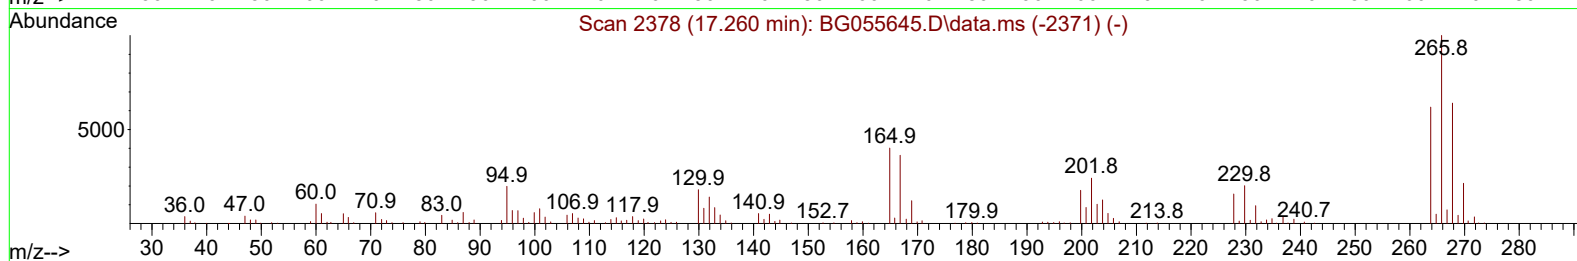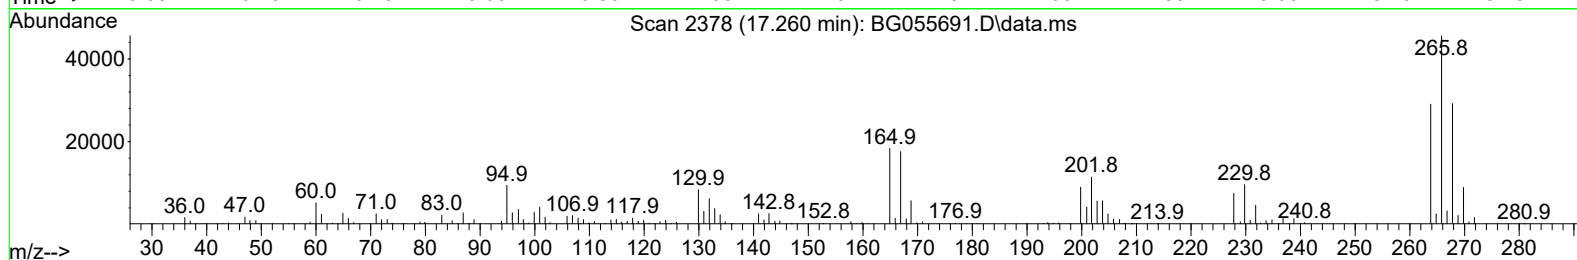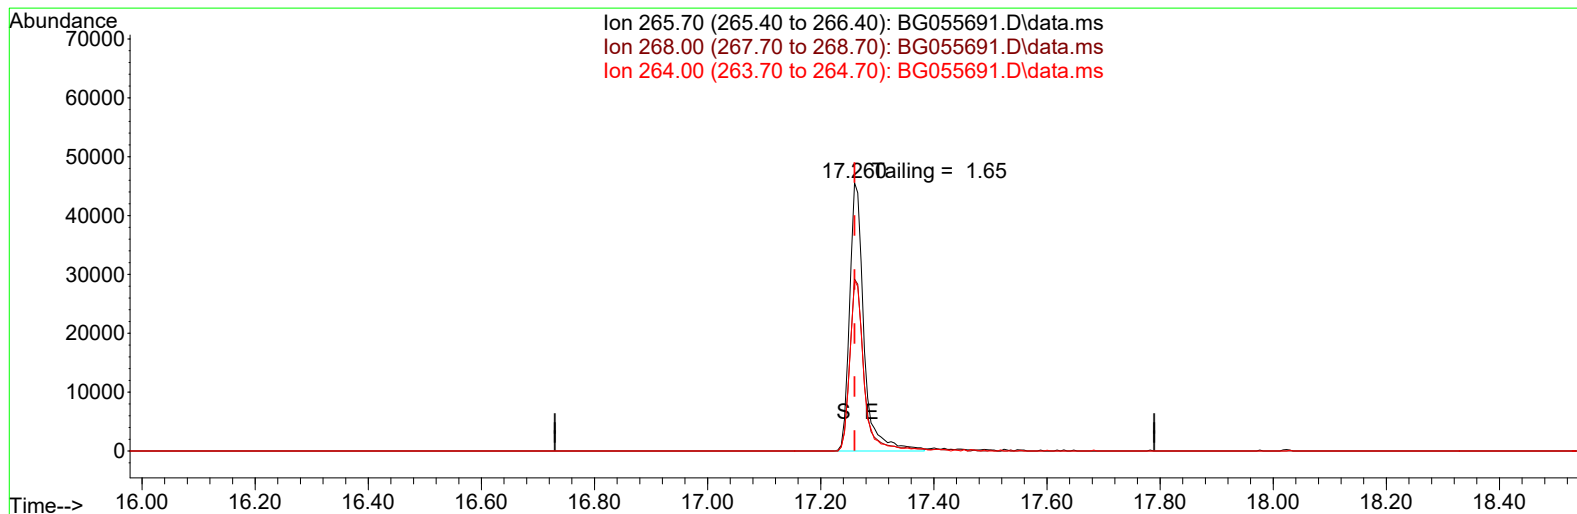

TIC: BG055691.D\data.ms

(70) Pentachlorophenol (C)

17.260min (-0.000) 26251.99 ng




response 80953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.03
264.00	61.90	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG111822\
 Data File : BG055691.D
 Acq On : 18 Nov 2022 15:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Nov 19 04:43:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG111622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 17 02:02:46 2022
 Response via : Initial Calibration

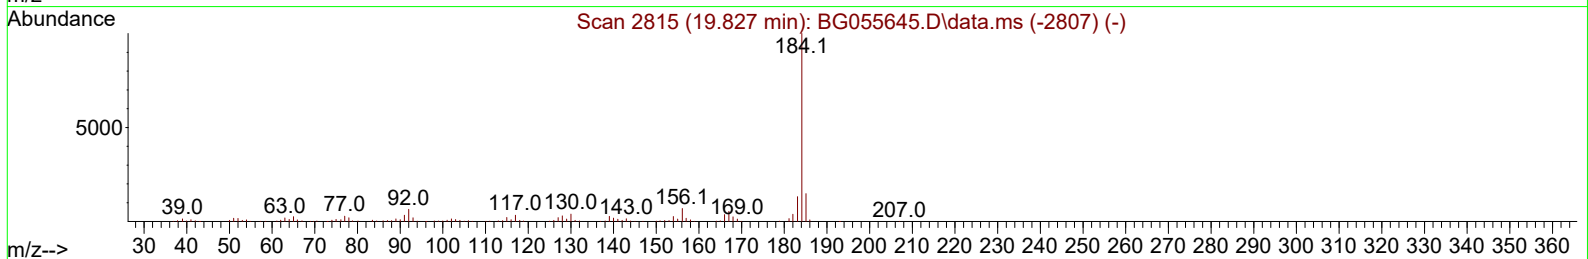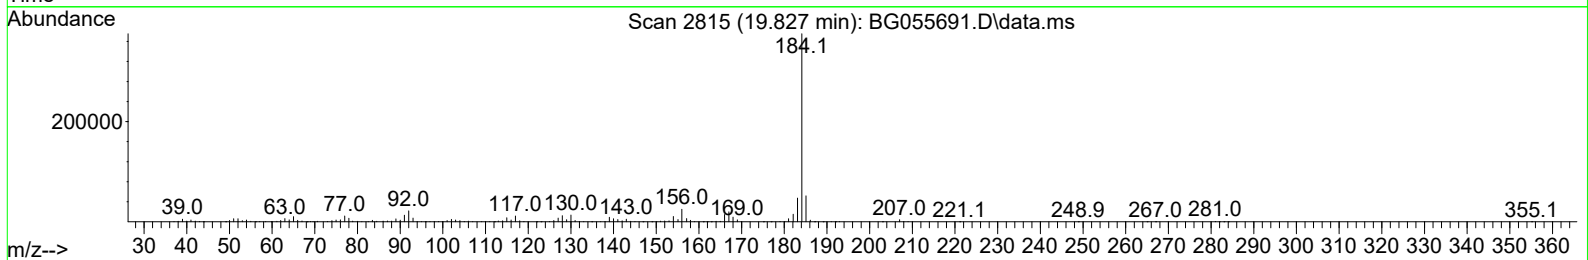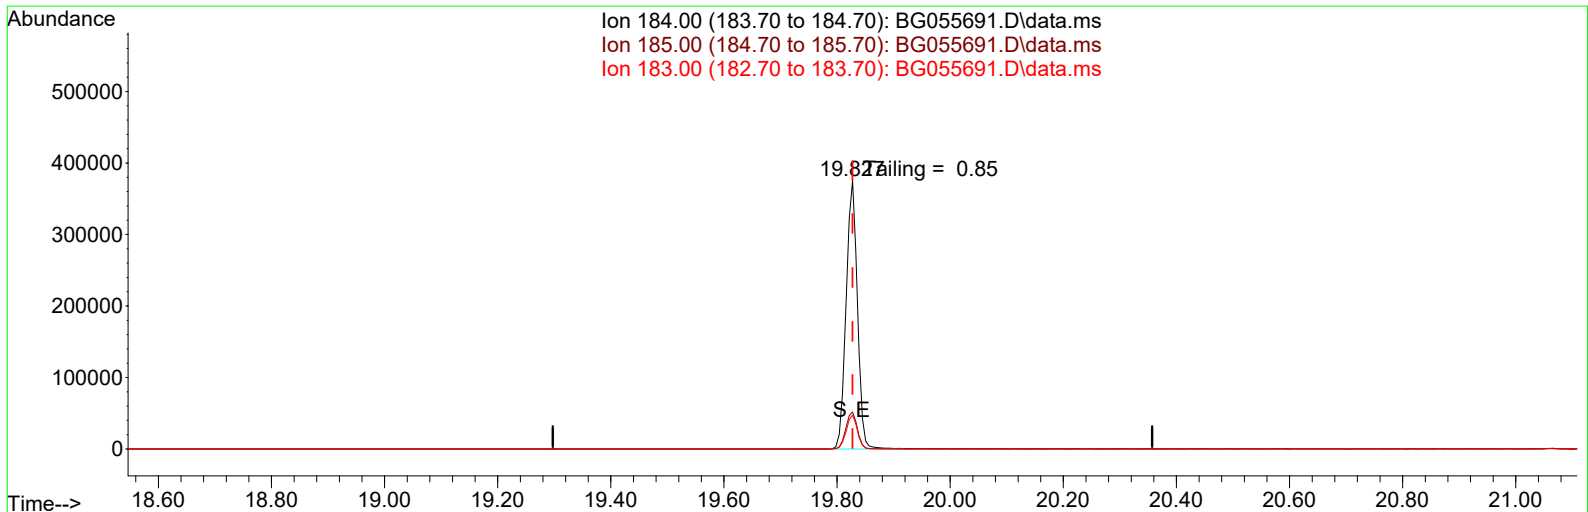

TIC: BG055691.D\data.ms

(77) Benzidine

19.827min (-0.000) 410725.77 ng

response 522606

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.84
183.00	13.20	12.67
0.00	0.00	0.00