

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111915\
 Data File : BG019713.D
 Acq On : 19 Nov 2015 20:10
 Operator : UM/NP
 Sample : G4310-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KN3

Quant Time: Nov 20 01:17:31 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 20 01:13:44 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	27346	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	112718	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.78	164	93971	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.52	188	292128	20.00	ng/ul	0.00
78) Chrysene-d12	21.79	240	396519	20.00	ng/ul	0.00
86) Perylene-d12	25.11	264	380291	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	3035	4.74	ng/uL	0.00
5) Phenol-d5	7.29	99	73229	26.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.46	67	51917	28.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	46709	26.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	61011	26.30	ng/ul	0.00
19) Nitrobenzene-d5	9.32	128	26335	28.46	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	30186	28.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.59	165	60593	26.90	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	74854	35.01	ng/ul	0.00
44) Dimethylphthalate-d6	14.18	166	265352	31.22	ng/ul	0.00
47) Acenaphthylene-d8	14.48	160	273373	29.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.97	143	40132	29.97	ng/ul	0.00
58) Fluorene-d10	15.77	176	231510	30.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.88	200	49858	26.42	ng/ul	0.00
71) Anthracene-d10	17.62	188	419542	29.58	ng/ul	0.00
79) Pyrene-d10	19.90	212	559344	30.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.88	264	627832	31.62	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.23	163	75687	8.98 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG111915\
Data File : BG019713.D
Acq On : 19 Nov 2015 20:10
Operator : UM/NP
Sample : G4310-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KN3

Quant Time: Nov 20 01:17:31 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 20 01:13:44 2015
Response via : Initial Calibration

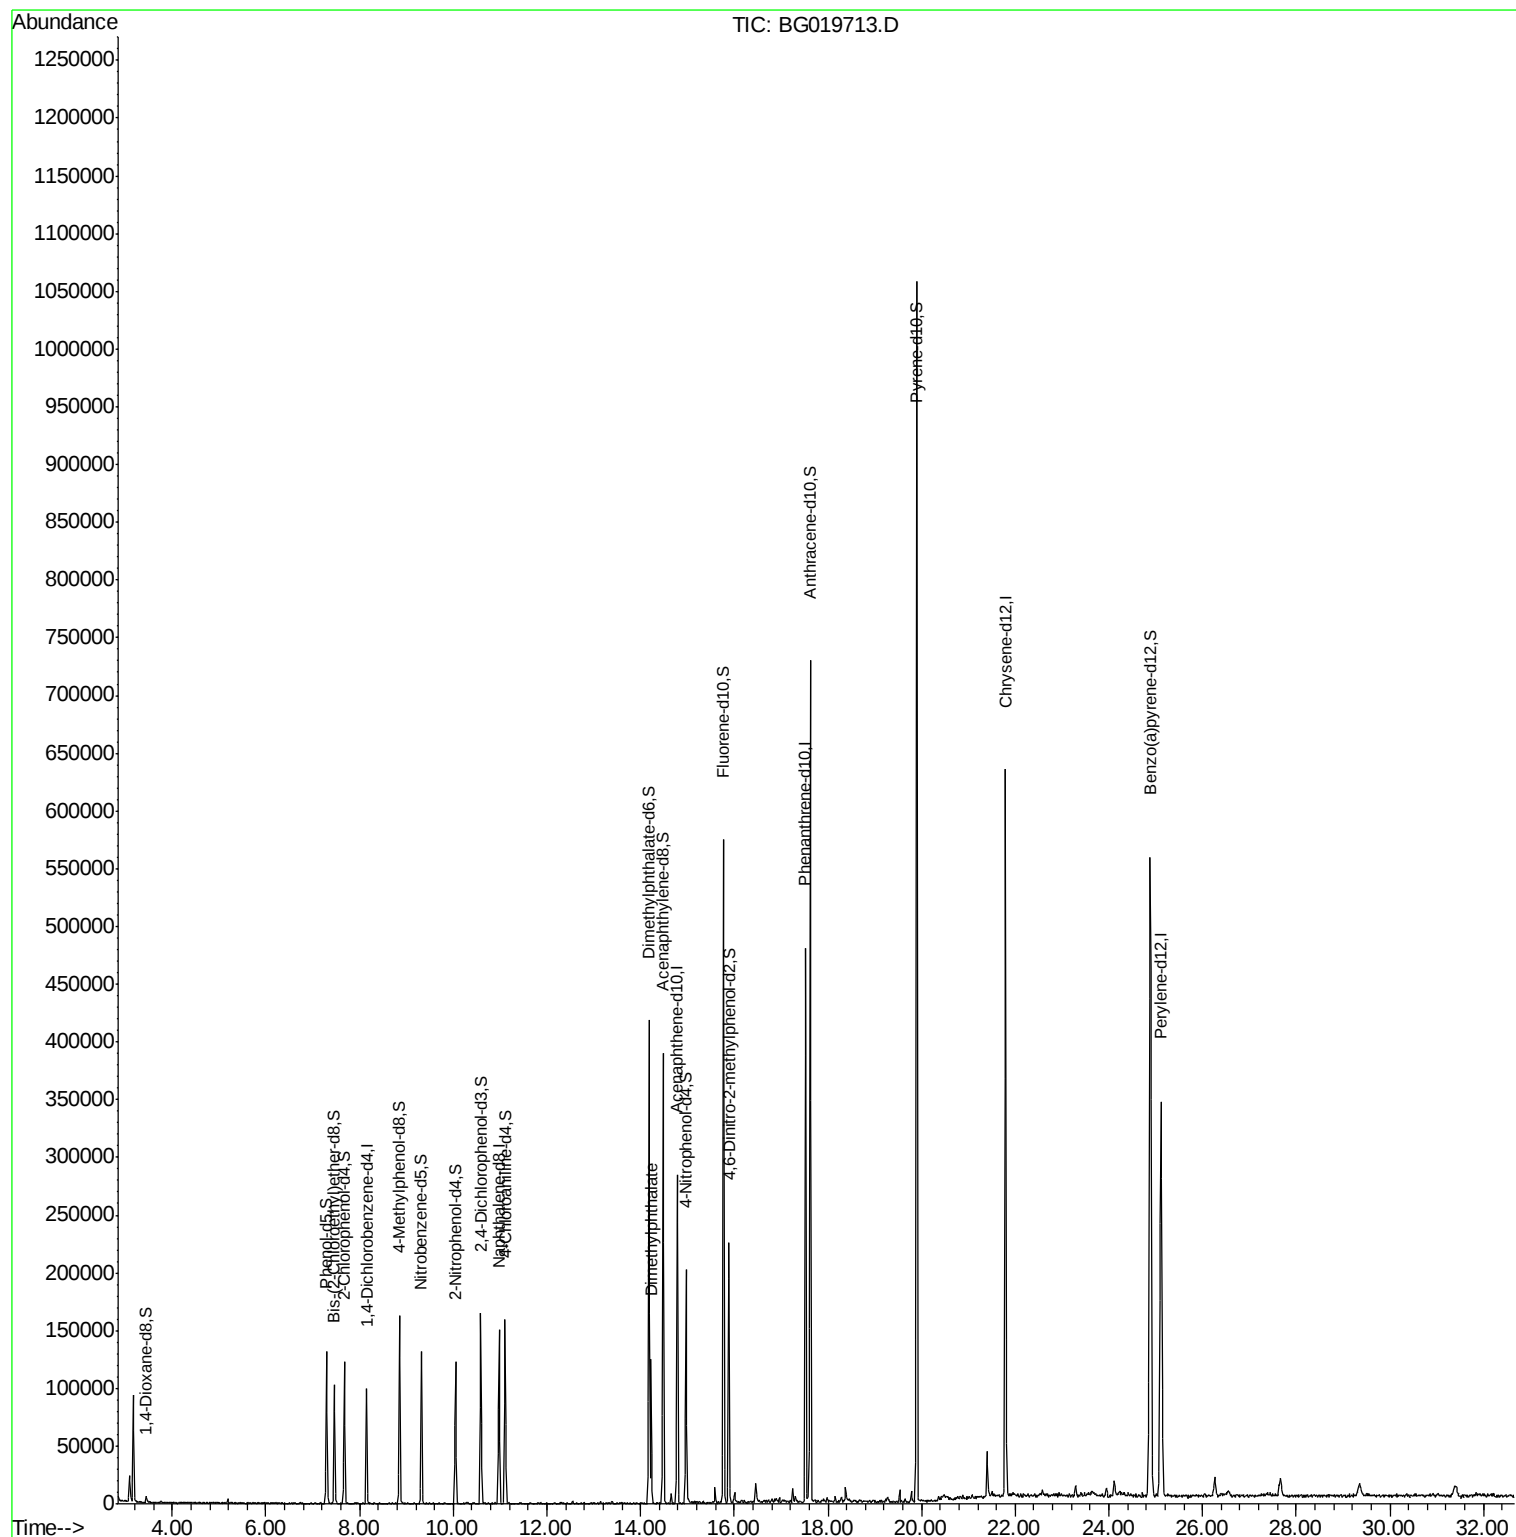

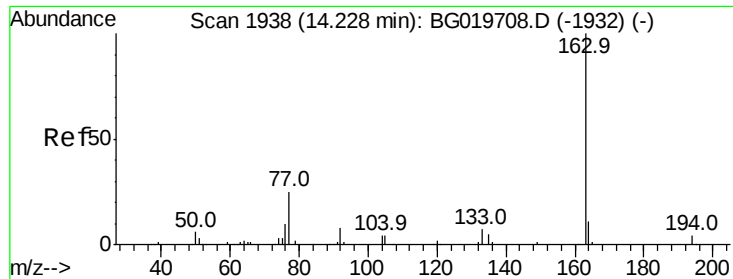

#45

Dimethylphthalate

Concen: 8.98 ng/ul

RT: 14.23 min Scan# 1938

Delta R.T. -0.00 min

Lab File: BG019713.D

Acq: 19 Nov 2015 20:10

Instrument :

BNA_G

ClientSampleId :

D9KN3


Tot Ion:163 Resp: 75687

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 9.6 8.3 12.5

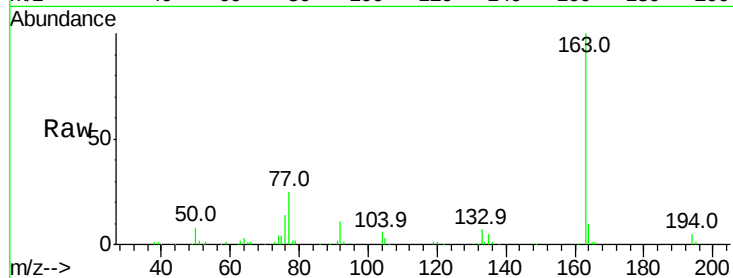

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

