
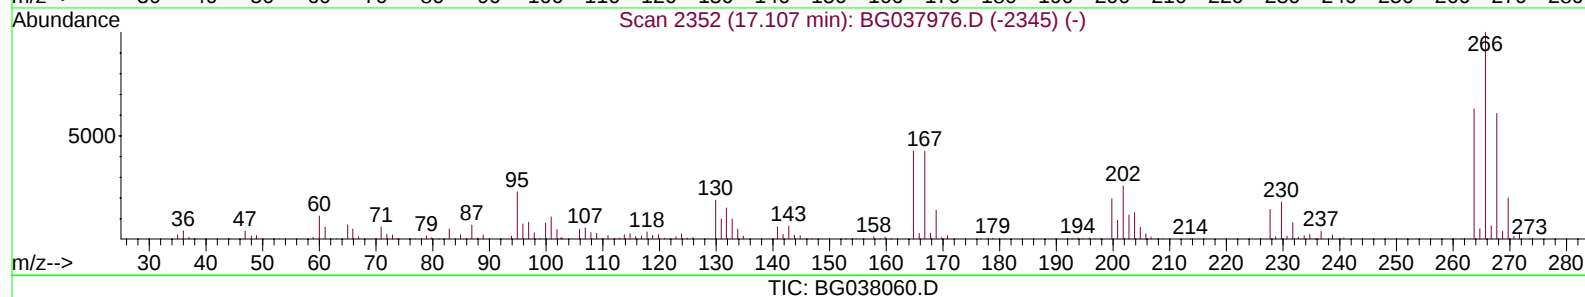
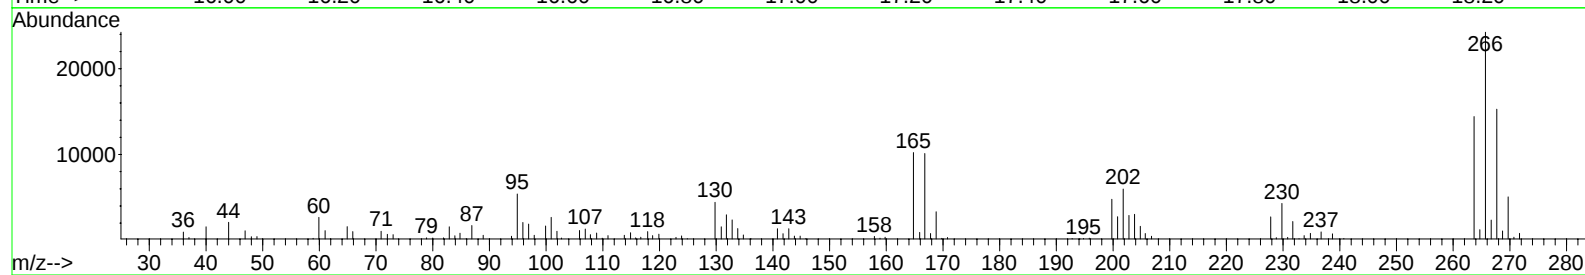


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111918\
Data File : BG038060.D
Acq On : 19 Nov 2018 12:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 17:22:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 16:39:28 2018
Response via : Initial Calibration

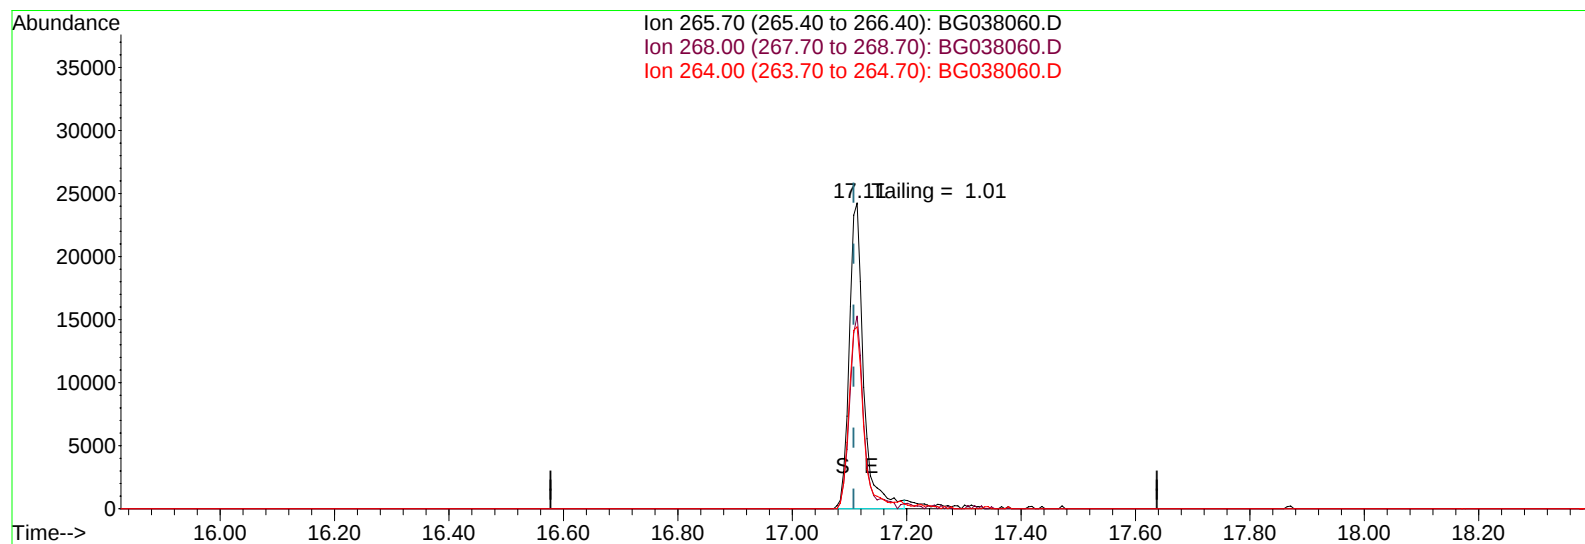

(70) Pentachlorophenol (C)




17.113min (+0.006) 29338.65ng

response 42440

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.48
264.00	73.60	64.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111918\
 Data File : BG038060.D
 Acq On : 19 Nov 2018 12:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 17:22:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG111318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 16:39:28 2018
 Response via : Initial Calibration

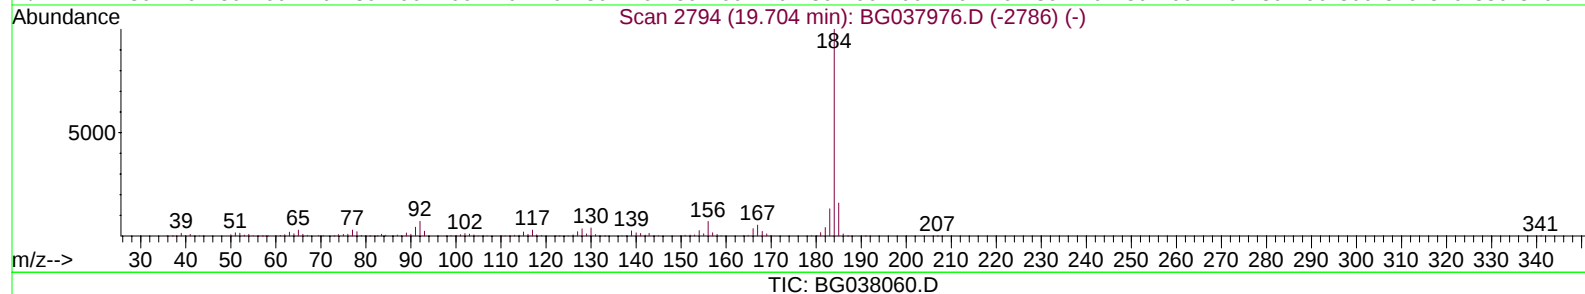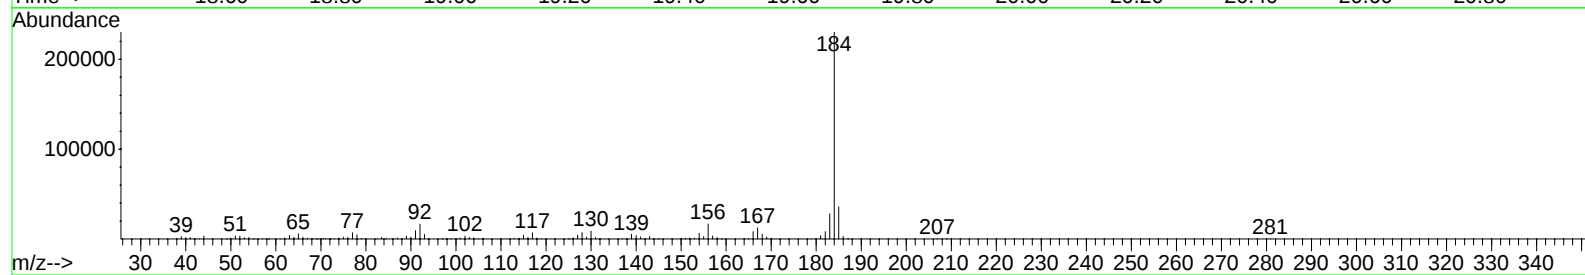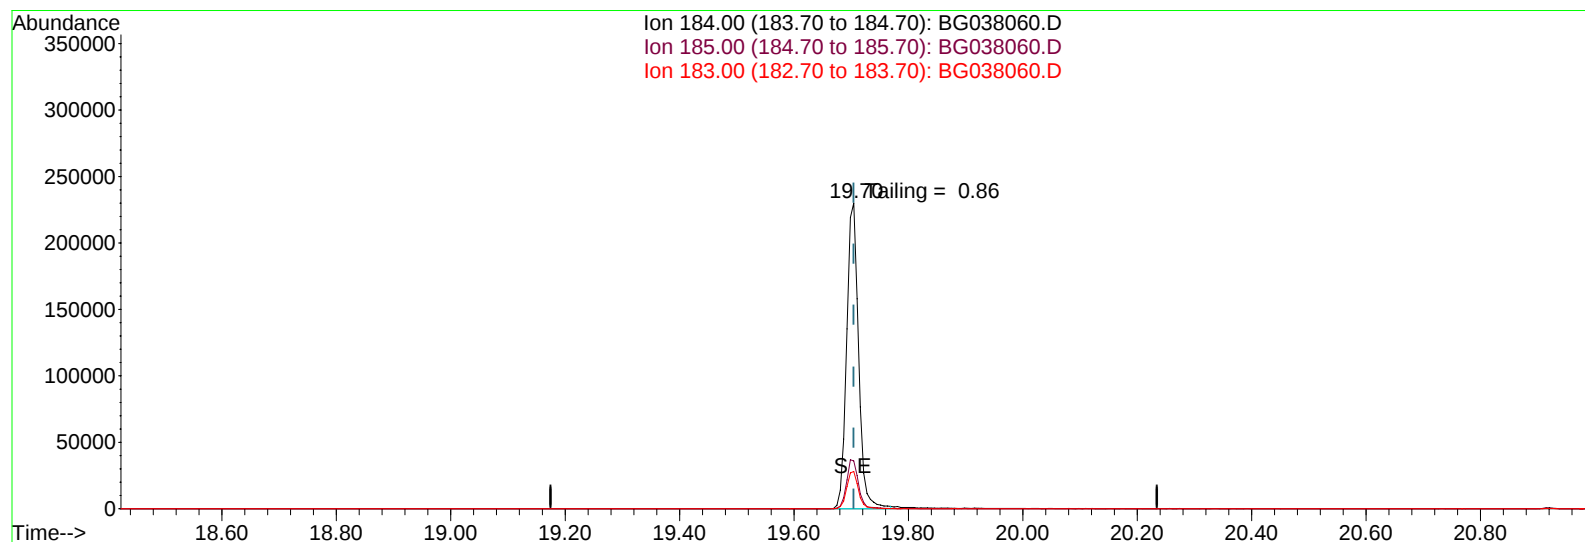

(77) Benzidine

19.704min (+0.000) 0.00ng

response 338363

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.64
183.00	12.70	12.20
0.00	0.00	0.00