


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG111918\
 Data File : BG038060.D
 Acq On : 19 Nov 2018 12:42
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG111318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 16:39:28 2018

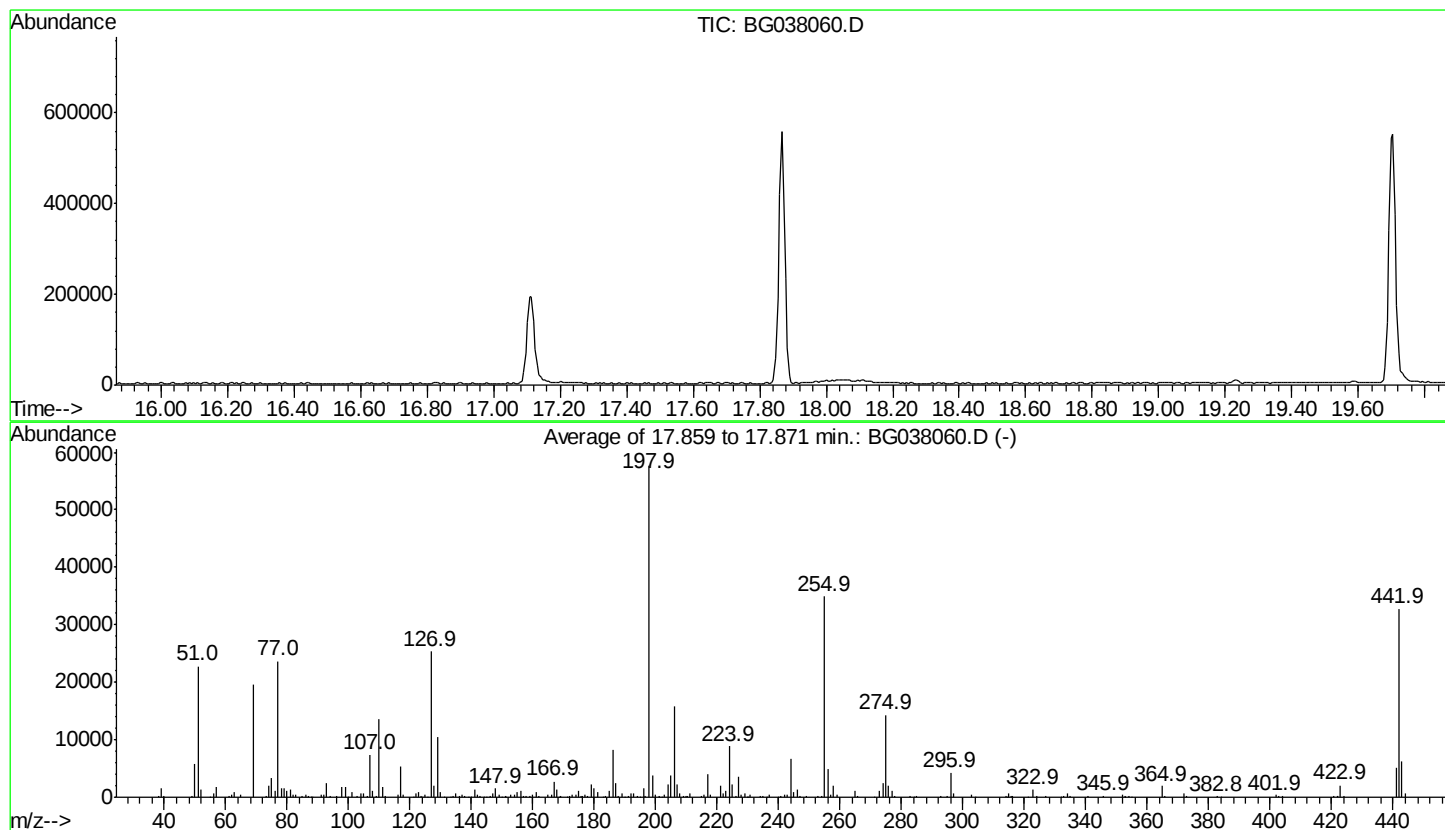

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	22818	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.8	19490	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	25322	PASS
197	198	0.00	2	0.3	167	PASS
198	198	100	100	100.0	57680	PASS
199	198	5	9	6.6	3806	PASS
275	198	10	60	24.8	14303	PASS
365	198	1	100	3.4	1986	PASS
441	198	0.01	100	8.9	5131	PASS
442	198	50	100	56.8	32754	PASS
443	442	15	24	19.0	6224	PASS