

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112015\
 Data File : BG019725.D
 Acq On : 20 Nov 2015 18:38
 Operator : UM/NP
 Sample : G4460-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Nov 21 00:21:59 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 21 00:19:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	24616	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	89265	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.76	164	69619	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.50	188	191276	20.00	ng/ul	0.00
78) Chrysene-d12	21.77	240	256325	20.00	ng/ul	0.00
86) Perylene-d12	25.07	264	246608	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	2262	3.92	ng/uL	0.00
5) Phenol-d5	7.26	99	46984	18.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	30345	18.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	30412	18.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	36397	17.43	ng/ul	0.00
19) Nitrobenzene-d5	9.30	128	15194	20.73	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	17625	21.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	35941	20.15	ng/ul	0.00
29) 4-Chloroaniline-d4	11.08	131	39012	23.04	ng/ul	0.00
44) Dimethylphthalate-d6	14.15	166	137530	21.84	ng/ul	0.00
47) Acenaphthylene-d8	14.45	160	132702	19.44	ng/ul	0.00
52) 4-Nitrophenol-d4	14.95	143	18501	18.65	ng/ul	0.00
58) Fluorene-d10	15.75	176	103036	18.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.86	200	19248	15.58	ng/ul	0.00
71) Anthracene-d10	17.60	188	171510	18.47	ng/ul	0.00
79) Pyrene-d10	19.88	212	199854	17.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.84	264	183789	14.28	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.20	163	76439	12.24	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112015\
Data File : BG019725.D
Acq On : 20 Nov 2015 18:38
Operator : UM/NP
Sample : G4460-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Nov 21 00:21:59 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 21 00:19:56 2015
Response via : Initial Calibration

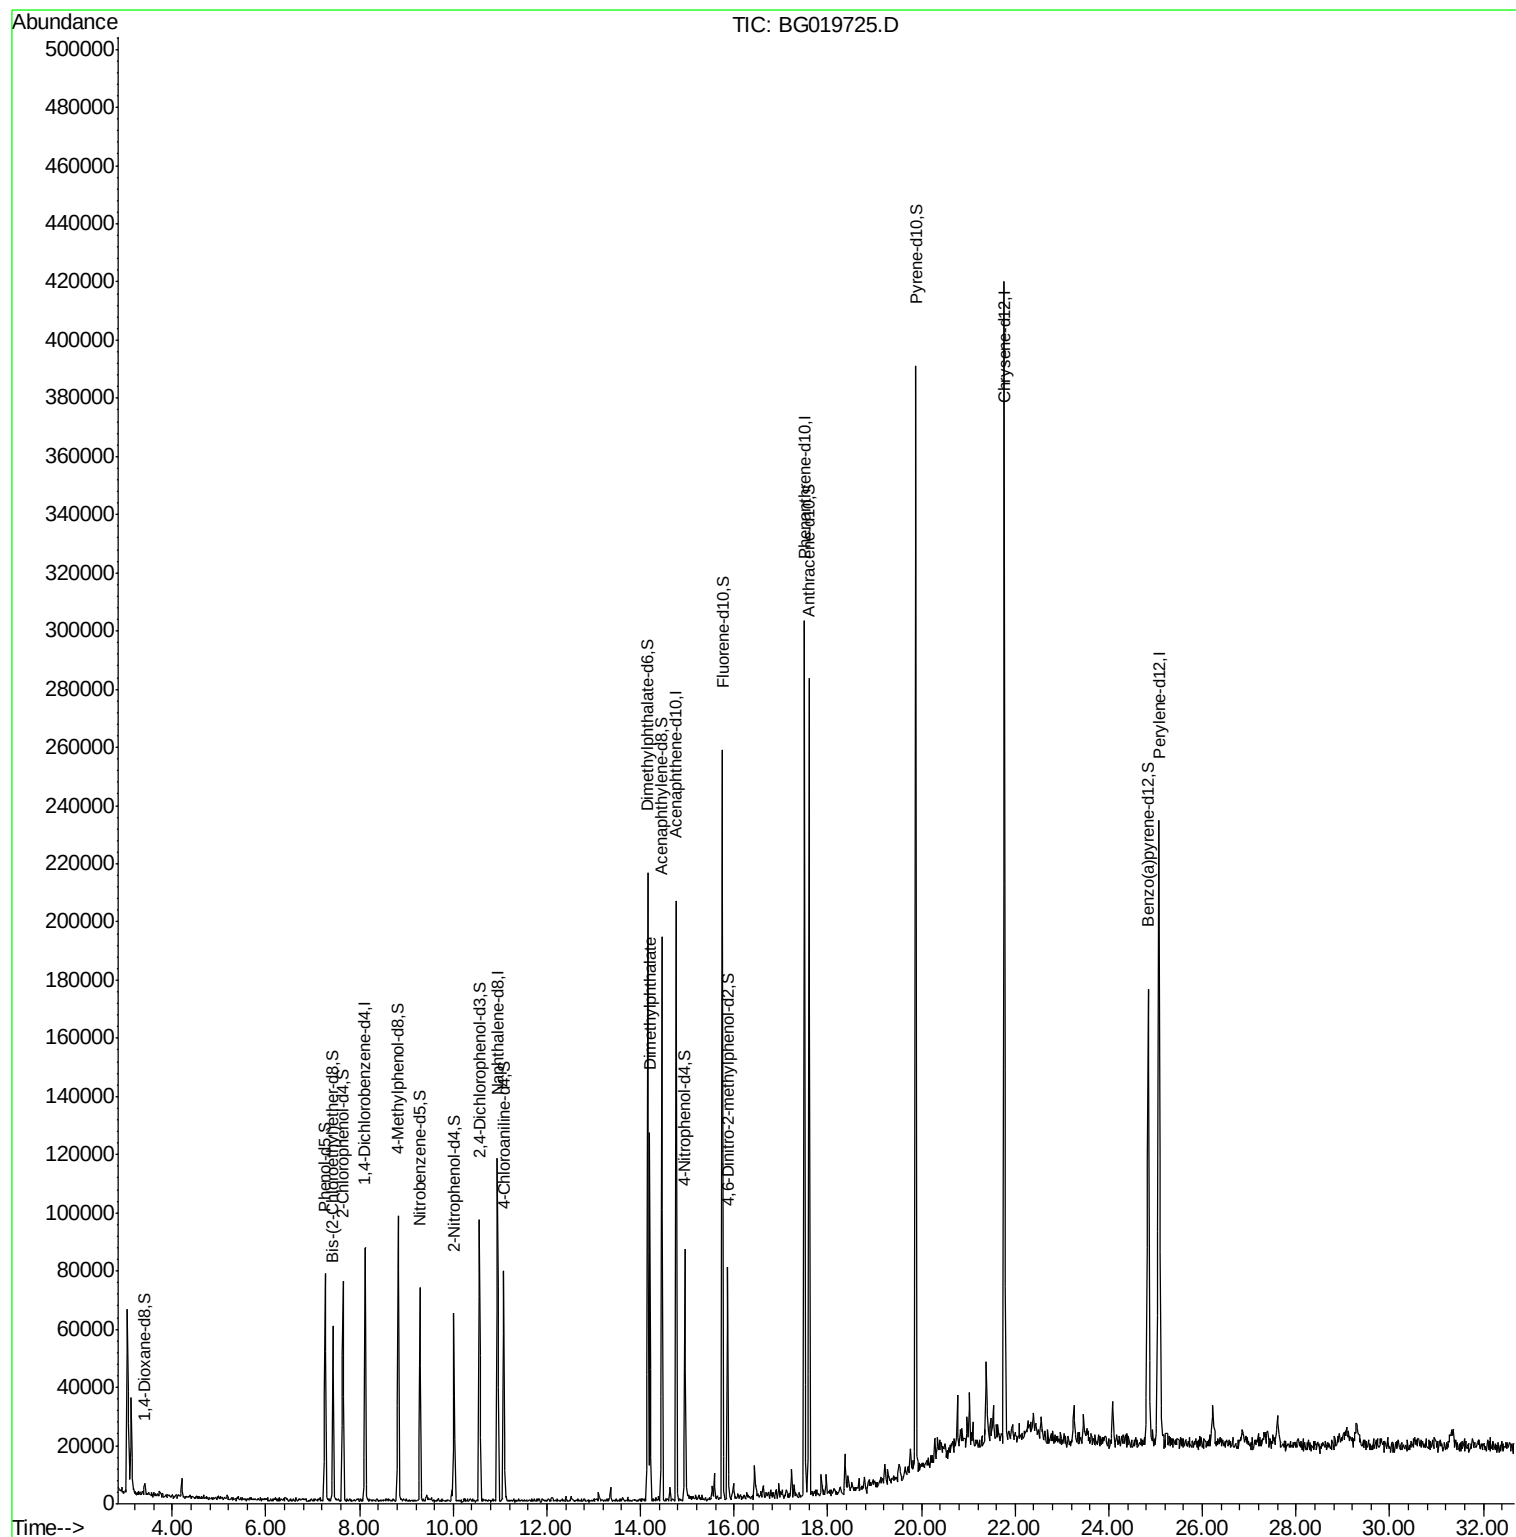

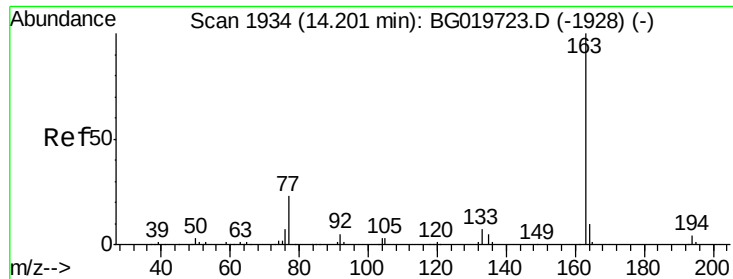

#45

Dimethylphthalate

Concen: 12.24 ng/ul

RT: 14.20 min Scan# 1934

Delta R.T. 0.00 min

Lab File: BG019725.D

Acq: 20 Nov 2015 18:38

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 76439

Ion Ratio Lower Upper

163 100

194 3.7 3.5 5.3

164 9.9 8.3 12.5

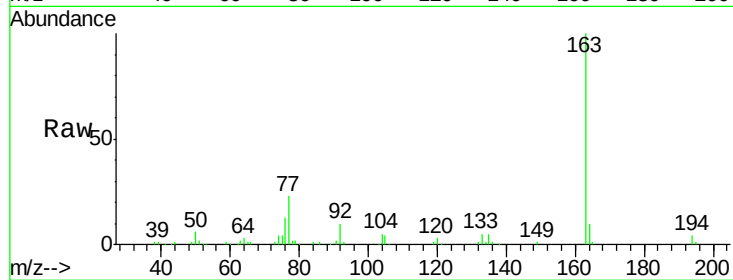

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

