

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG112015\
 Data File : BG019726.D
 Acq On : 20 Nov 2015 19:17
 Operator : UM/NP
 Sample : G4460-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC7D3

Quant Time: Nov 21 00:22:05 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 21 00:19:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	25205	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	92000	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.76	164	71816	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.50	188	200157	20.00	ng/ul	0.00
78) Chrysene-d12	21.77	240	277918	20.00	ng/ul	0.00
86) Perylene-d12	25.07	264	266377	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	2244	3.80	ng/uL	0.00
5) Phenol-d5	7.27	99	43294	16.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	27140	16.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	27539	16.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	33461	15.65	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	14441	19.12	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	16643	19.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	33273	18.10	ng/ul	0.00
29) 4-Chloroaniline-d4	11.08	131	38420	22.02	ng/ul	0.00
44) Dimethylphthalate-d6	14.15	166	137273	21.13	ng/ul	0.00
47) Acenaphthylene-d8	14.45	160	129641	18.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.95	143	18082	17.67	ng/ul	0.00
58) Fluorene-d10	15.75	176	109956	18.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.86	200	20992	16.24	ng/ul	0.00
71) Anthracene-d10	17.60	188	194003	19.96	ng/ul	0.00
79) Pyrene-d10	19.88	212	250848	19.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.84	264	278526	20.03	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.20	163	95555	14.84	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG112015\
Data File : BG019726.D
Acq On : 20 Nov 2015 19:17
Operator : UM/NP
Sample : G4460-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC7D3

Quant Time: Nov 21 00:22:05 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 21 00:19:56 2015
Response via : Initial Calibration

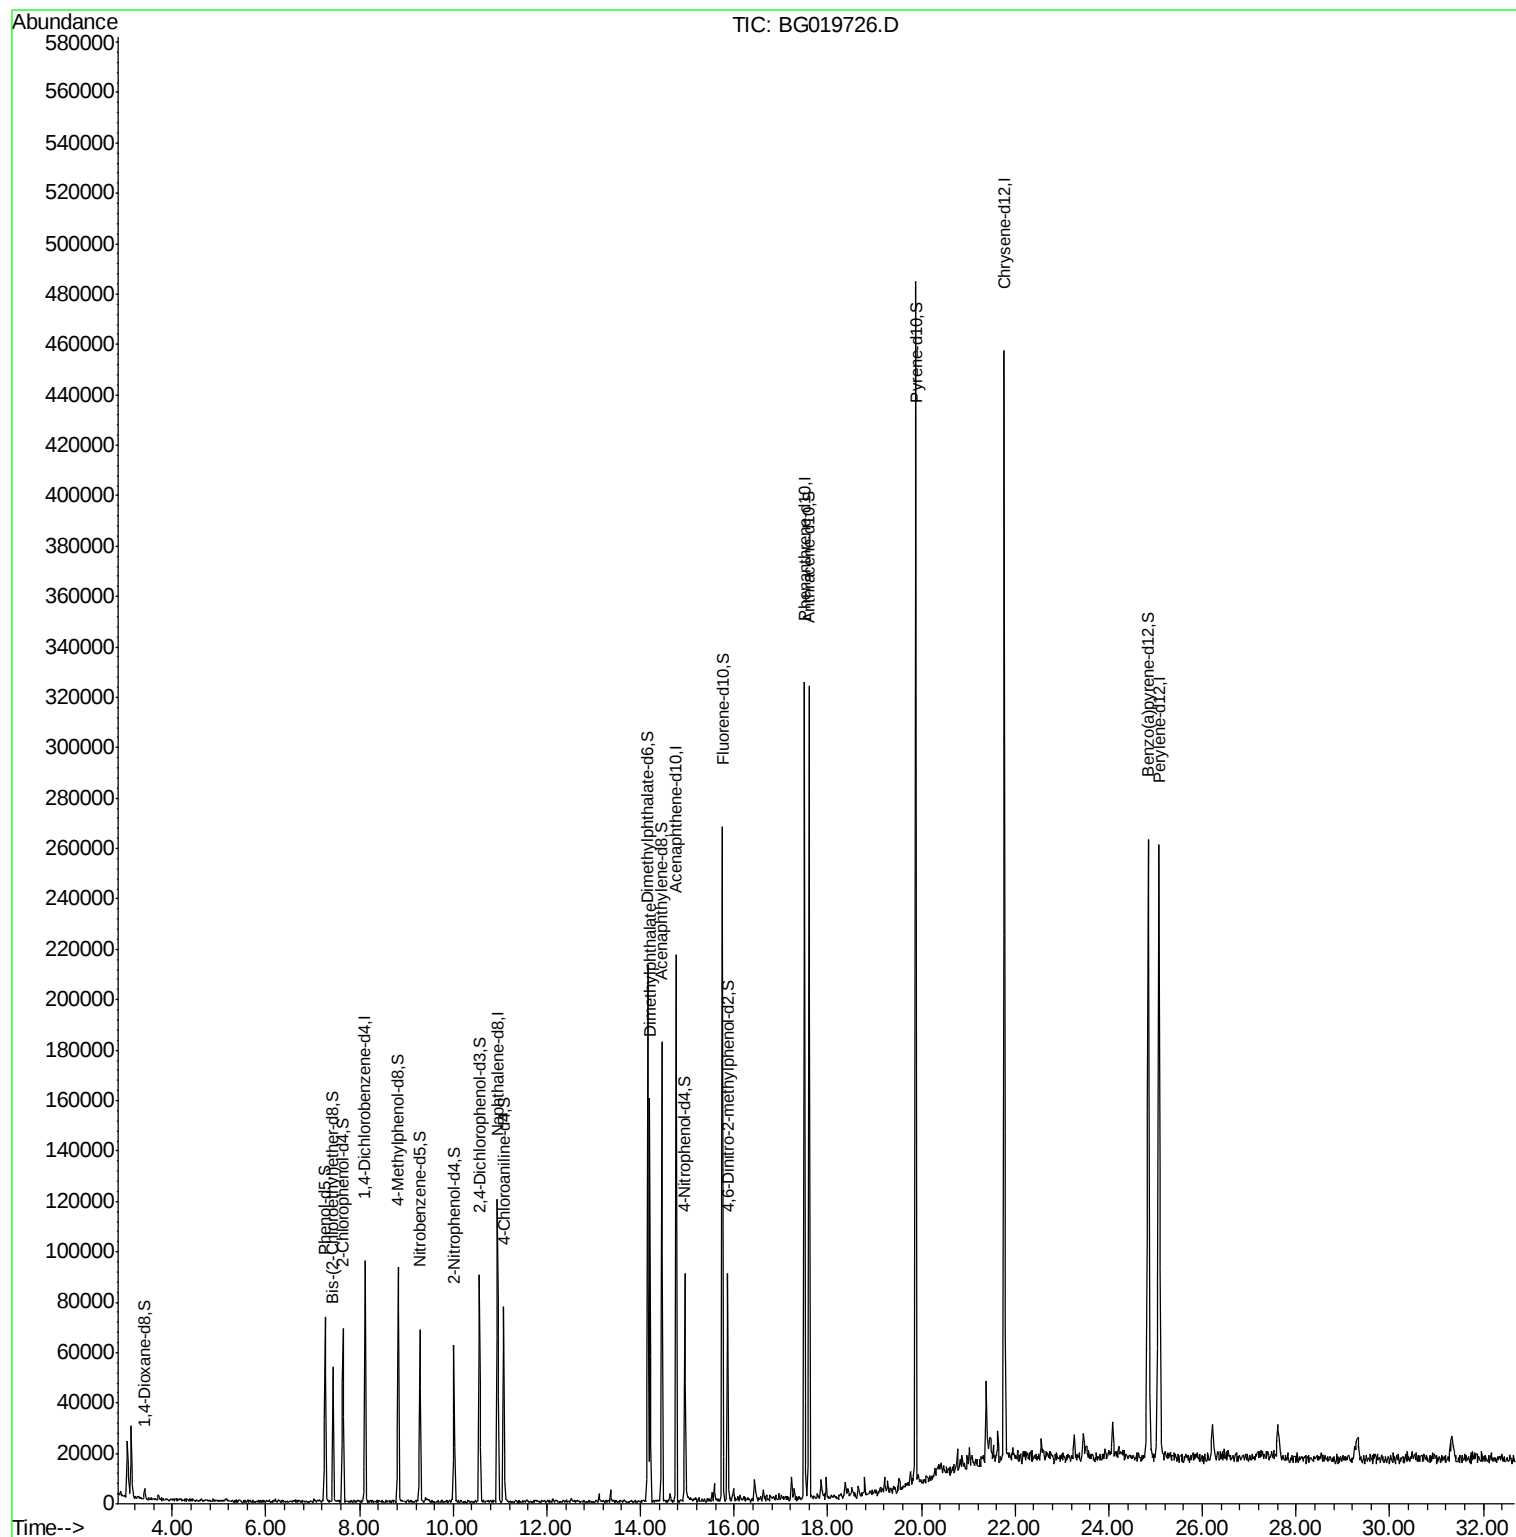

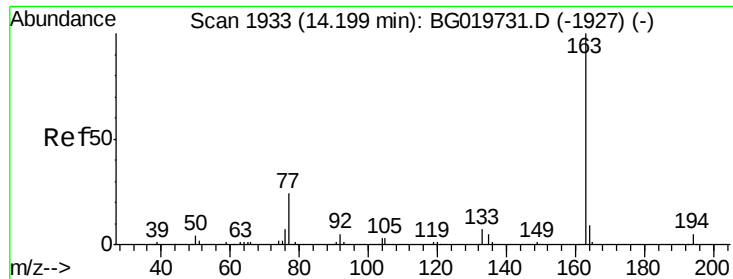

#45

Dimethylphthalate

Concen: 14.84 ng/ul

RT: 14.20 min Scan# 1934

Delta R.T. -0.00 min

Lab File: BG019726.D


Acq: 20 Nov 2015 19:17

Instrument :

BNA_G

ClientSampleId :

BC7D3

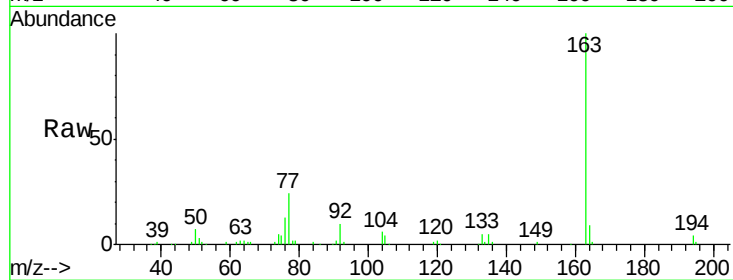


Tgt Ion:163 Resp: 95555

Ion Ratio Lower Upper

163 100

194 3.6 3.5 5.3

164 9.1 8.3 12.5

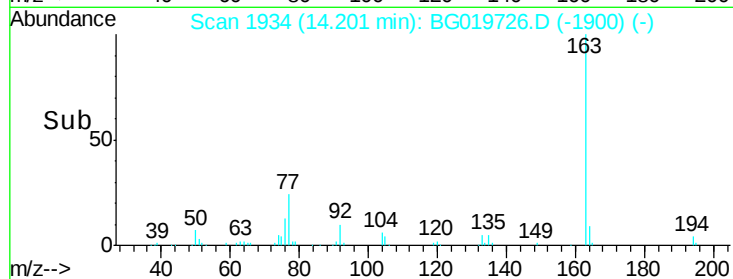

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

