

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112015\
 Data File : BG019743.D
 Acq On : 21 Nov 2015 6:24
 Operator : UM/NP
 Sample : G4428-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC7C0

Quant Time: Nov 22 00:19:07 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 21 01:06:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	24742	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	99024	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.75	164	83375	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.50	188	248052	20.00	ng/ul	0.00
78) Chrysene-d12	21.76	240	327855	20.00	ng/ul	0.00
86) Perylene-d12	25.06	264	314708	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	2278	3.93	ng/uL	0.00
5) Phenol-d5	7.26	99	53455	21.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	36004	21.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	34408	21.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	43638	20.79	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	17351	21.34	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	20606	22.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	41581	21.02	ng/ul	0.00
29) 4-Chloroaniline-d4	11.08	131	48467	25.80	ng/ul	0.00
44) Dimethylphthalate-d6	14.15	166	154859	20.54	ng/ul	0.00
47) Acenaphthylene-d8	14.45	160	155416	19.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.94	143	21471	18.07	ng/ul	0.00
58) Fluorene-d10	15.74	176	125183	18.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.86	200	18926	11.81	ng/ul	0.00
71) Anthracene-d10	17.59	188	224067	18.60	ng/ul	0.00
79) Pyrene-d10	19.87	212	270633	18.12	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.83	264	296334	18.04	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.20	163	125384	16.77	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112015\
Data File : BG019743.D
Acq On : 21 Nov 2015 6:24
Operator : UM/NP
Sample : G4428-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC7C0

Quant Time: Nov 22 00:19:07 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 21 01:06:32 2015
Response via : Initial Calibration

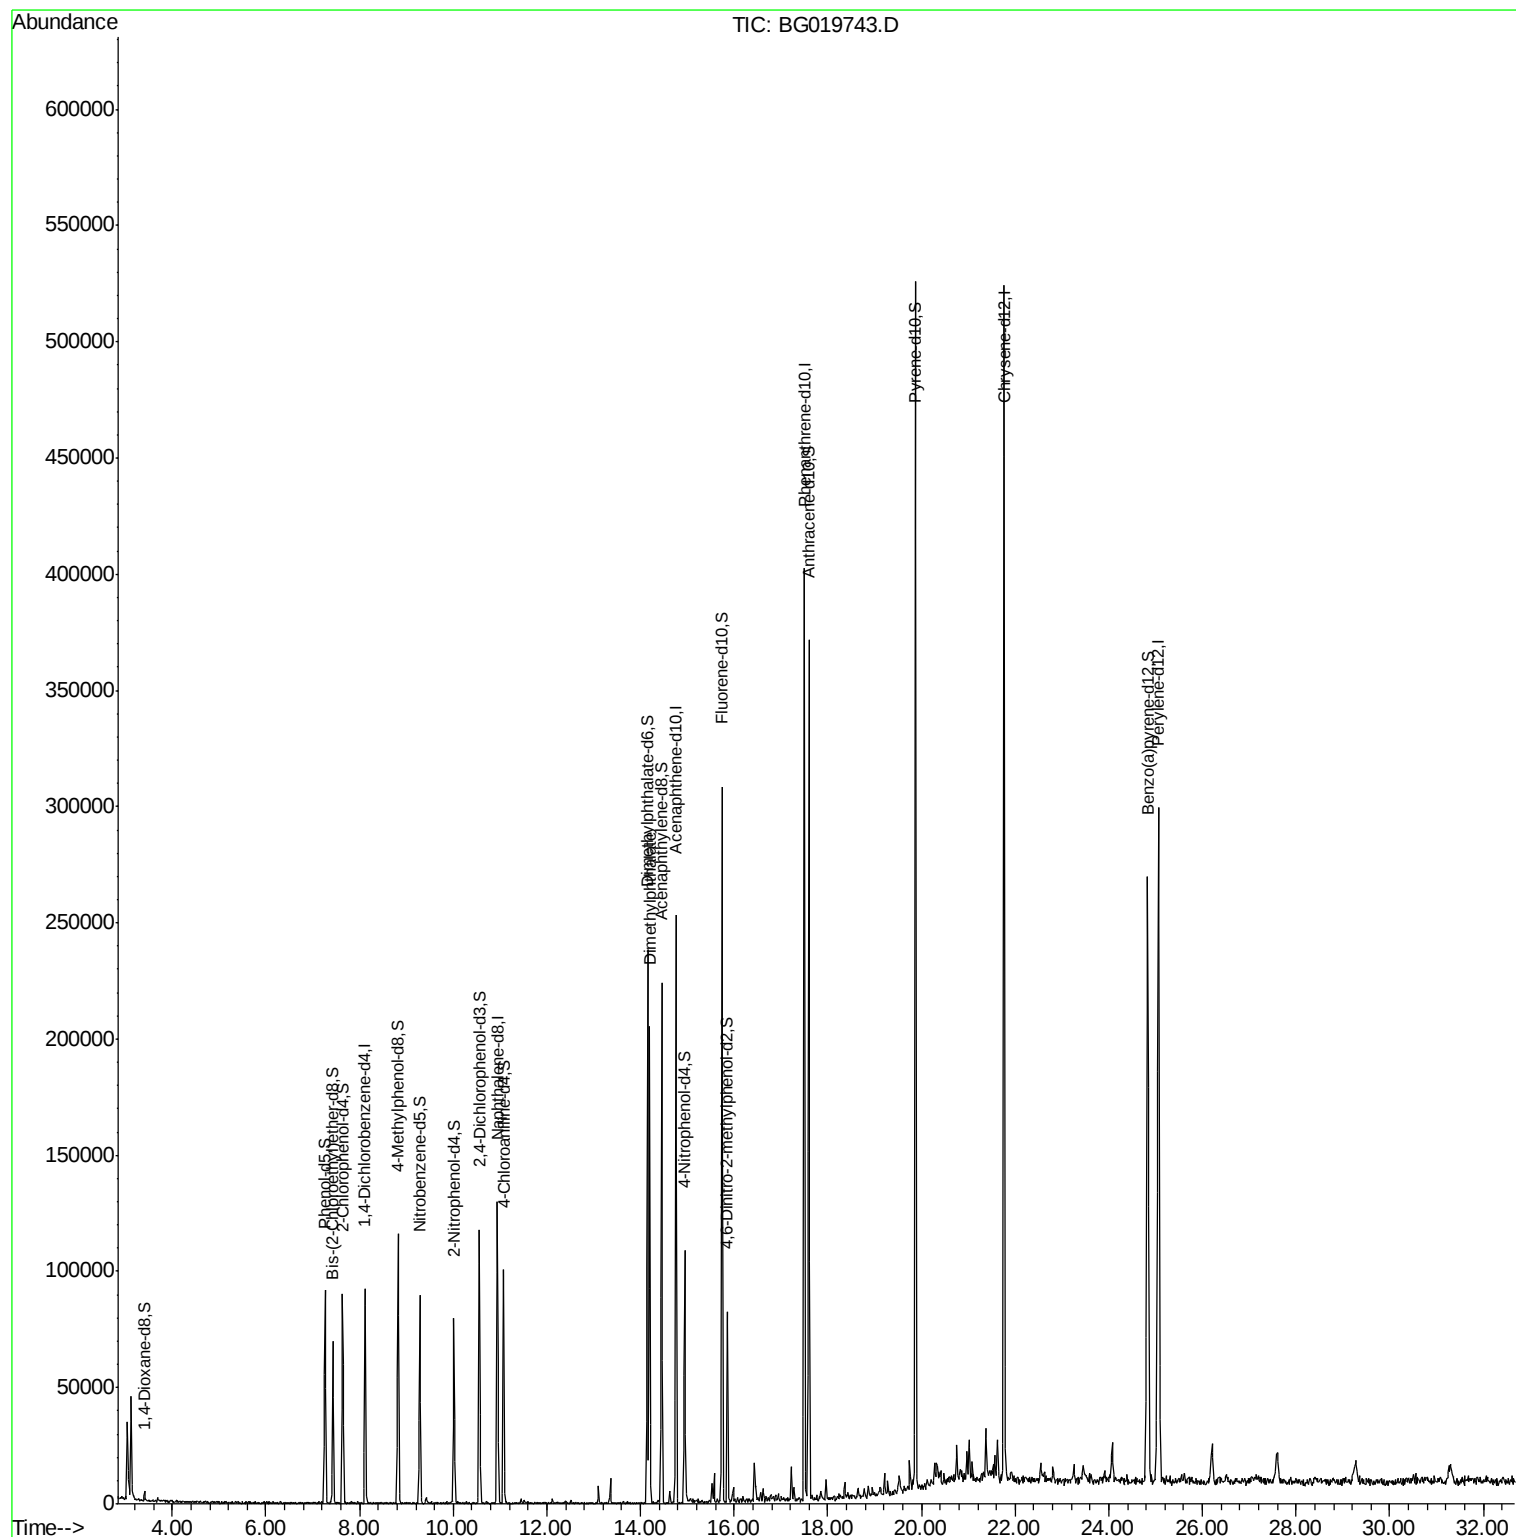

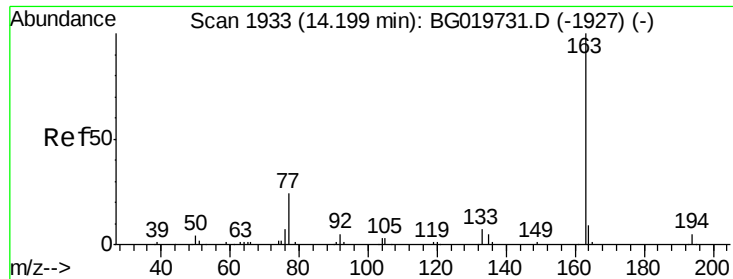

#45

Dimethylphthalate

Concen: 16.77 ng/ul

RT: 14.20 min Scan# 1933

Delta R.T. -0.00 min

Lab File: BG019743.D

Acq: 21 Nov 2015 6:24

Instrument :

BNA_G

ClientSampleId :

BC7C0


Tot Ion:163 Resp: 125384

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.1 8.3 12.5

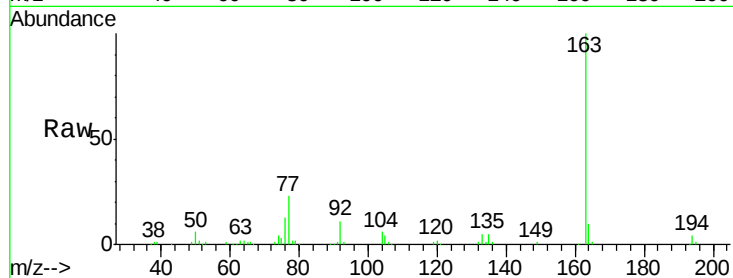

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

