

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112015\
 Data File : BG019751.D
 Acq On : 21 Nov 2015 12:50
 Operator : UM/NP
 Sample : G4428-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC7C6

Quant Time: Nov 21 14:14:44 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 21 01:06:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	22585	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	87975	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.76	164	68280	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.49	188	199857	20.00	ng/ul	0.00
78) Chrysene-d12	21.76	240	265920	20.00	ng/ul	-0.01
86) Perylene-d12	25.06	264	258619	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.40	96	2049	3.87	ng/uL	0.00
5) Phenol-d5	7.26	99	44678	19.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	28863	19.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	29356	19.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	37510	19.58	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	14415	19.96	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	16858	20.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	37481	21.32	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	37004	22.18	ng/ul	0.00
44) Dimethylphthalate-d6	14.15	166	131717	21.33	ng/ul	0.00
47) Acenaphthylene-d8	14.45	160	136136	20.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.94	143	22075	22.69	ng/ul	-0.01
58) Fluorene-d10	15.74	176	115330	20.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.85	200	22986	17.80	ng/ul	0.00
71) Anthracene-d10	17.59	188	219870	22.66	ng/ul	0.00
79) Pyrene-d10	19.87	212	268580	22.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.83	264	303630	22.49	ng/ul	0.00


Target Compounds						Ovalue
45) Dimethylphthalate	14.20	163	86446	14.12	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG112015\
Data File : BG019751.D
Acq On : 21 Nov 2015 12:50
Operator : UM/NP
Sample : G4428-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC7C6

Quant Time: Nov 21 14:14:44 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 21 01:06:32 2015
Response via : Initial Calibration

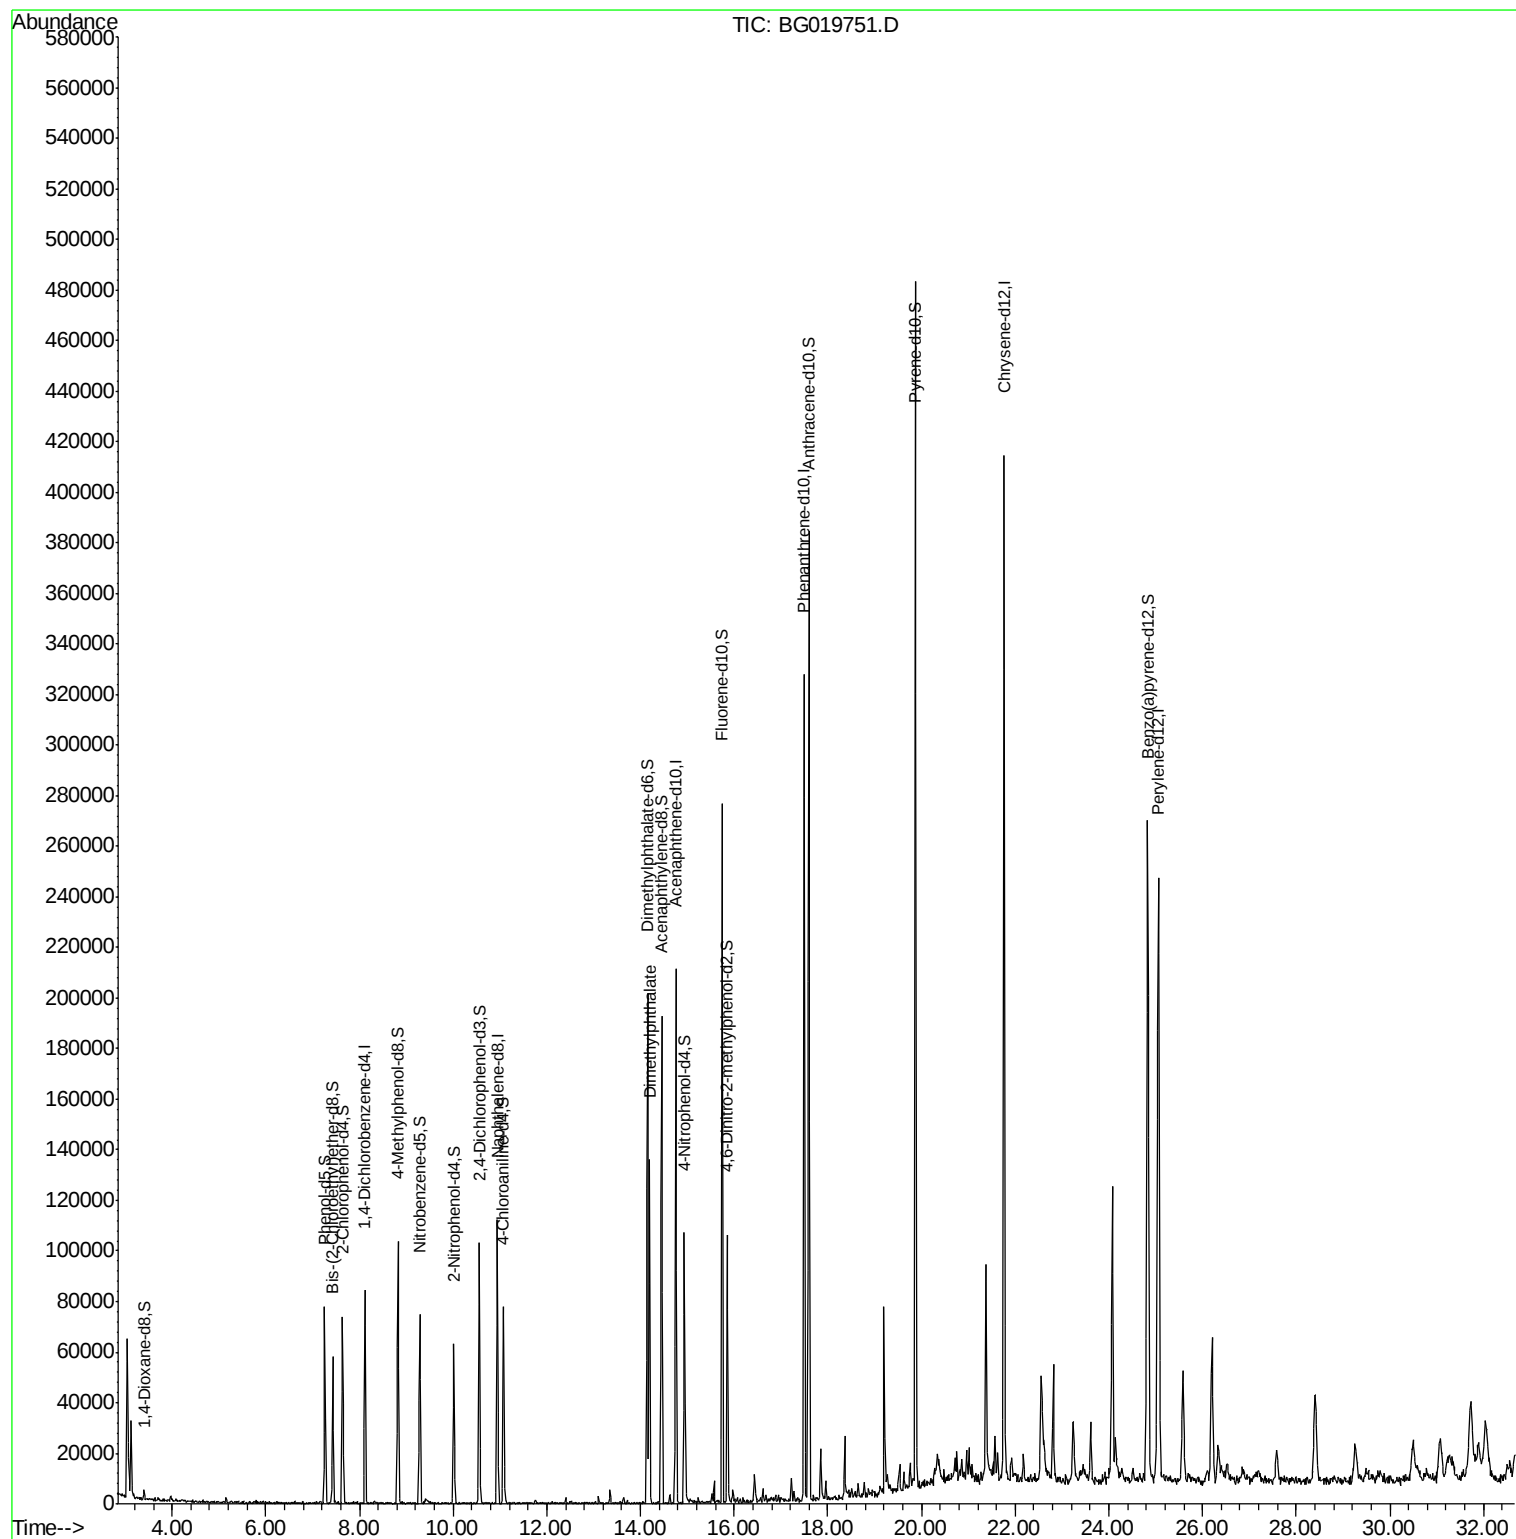

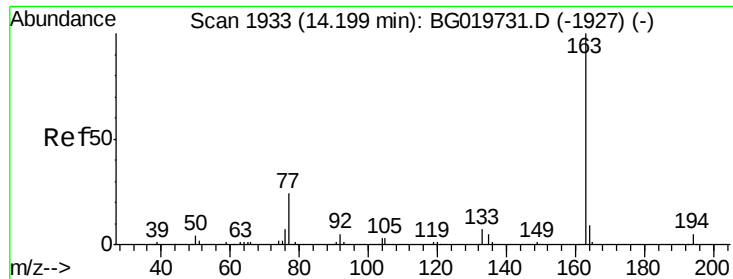

#45

Dimethylphthalate

Concen: 14.12 ng/ul

RT: 14.20 min Scan# 1933

Delta R.T. -0.00 min

Lab File: BG019751.D

Acq: 21 Nov 2015 12:50

Instrument :

BNA_G

ClientSampleId :

BC7C6


Tot Ion:163 Resp: 86446

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 8.6 8.3 12.5

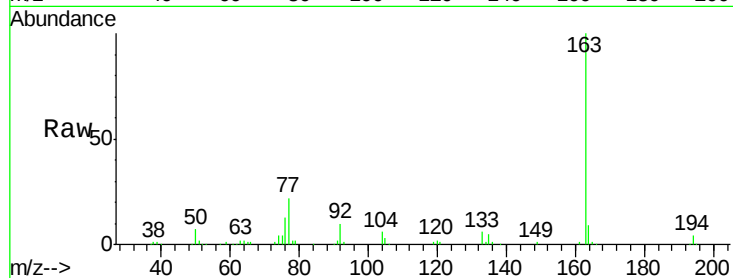

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

