

Data Path : V:\HPCHEM1\BNA G\DATA\BG112015\
 Data File : BG019767.D
 Acq On : 21 Nov 2015 23:20
 Operator : UM/NP
 Sample : G4310-19
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 D9KN8

Quant Time: Nov 22 07:33:26 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Nov 22 07:06:07 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	19319	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	76024	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.75	164	59352	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.50	188	171806	20.00	ng/ul	0.00
78) Chrysene-d12	21.76	240	236223	20.00	ng/ul	0.00
86) Perylene-d12	25.06	264	225175	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	2767	6.12	ng/uL	0.00
5) Phenol-d5	7.26	99	61113	30.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	44260	34.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	43037	33.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	49784	30.38	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	21684	34.74	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	25420	36.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	51169	33.69	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	61536	42.67	ng/ul	0.00
44) Dimethylphthalate-d6	14.15	166	186376	34.72	ng/ul	0.00
47) Acenaphthylene-d8	14.45	160	207334	35.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.94	143	24100	28.50	ng/ul	0.00
58) Fluorene-d10	15.74	176	168530	35.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.86	200	29748	26.80	ng/ul	0.00
71) Anthracene-d10	17.59	188	310339	37.20	ng/ul	0.00
79) Pyrene-d10	19.87	212	399956	37.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.84	264	454301	38.65	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.19	163	38072	7.15	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : V:\HPCHEM1\BNA G\DATA\BG112015\
Data File : BG019767.D
Acq On : 21 Nov 2015 23:20
Operator : UM/NP
Sample : G4310-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
D9KN8

Quant Time: Nov 22 07:33:26 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG111615.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Nov 22 07:06:07 2015
Response via : Initial Calibration

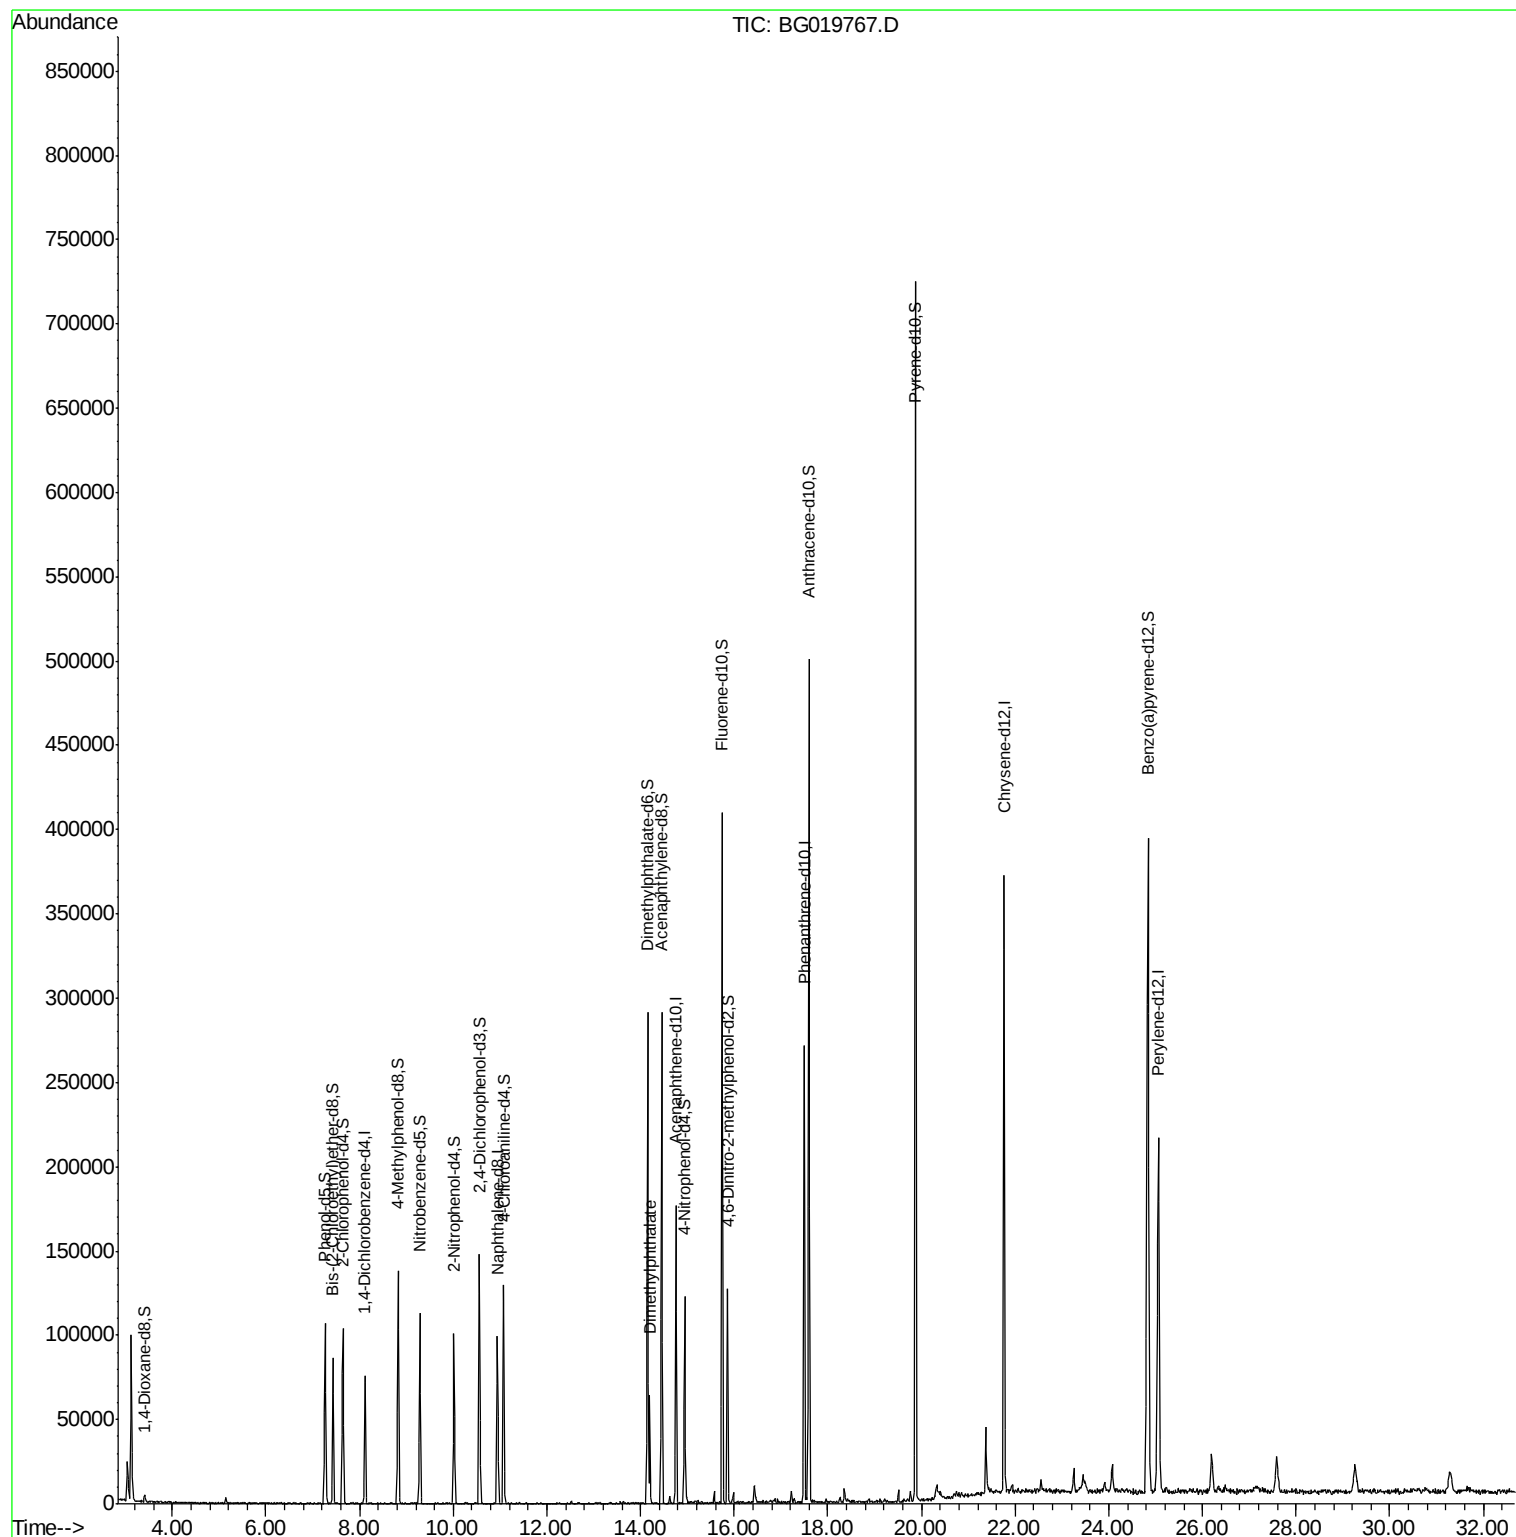

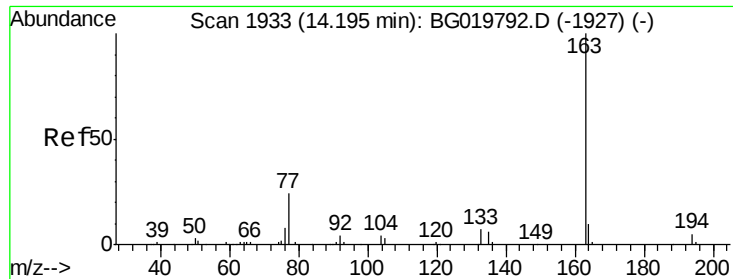

#45

Dimethylphthalate

Concen: 7.15 ng/ul

RT: 14.19 min Scan# 1933

Delta R.T. -0.00 min

Lab File: BG019767.D

Acq: 21 Nov 2015 23:20

Instrument :

BNA_G

ClientSampleId :

D9KN8


Tot Ion:163 Resp: 38072

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 10.2 8.3 12.5

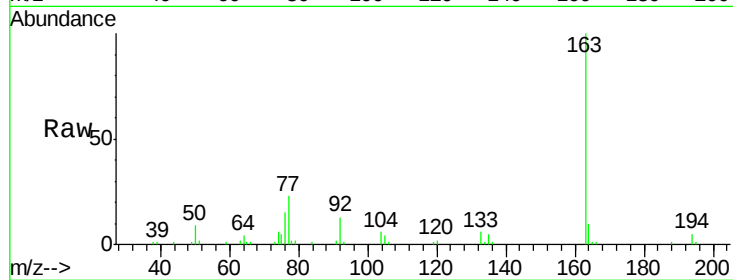

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

