

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112020\
 Data File : BG047380.D
 Acq On : 20 Nov 2020 18:19
 Operator : CG/JU
 Sample : PB133083BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK83

Quant Time: Nov 21 01:29:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 21 01:27:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	40015	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	157362	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	117766	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.71	188	562849	20.00	ng/ul	0.10
78) Chrysene-d12	21.90	240	275900	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	280390	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.62	96	6982	6.34	ng/uL	0.00
5) Phenol-d5	7.40	99	147896	36.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	83568	36.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	101896	37.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	112273	36.41	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	51739	39.80	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	57845	40.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	118917	36.62	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	143887	43.82	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	385882	38.17	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	452849	38.76	ng/ul	0.00
52) 4-Nitrophenol-d4	15.03	143	60533	39.24	ng/ul	0.00
58) Fluorene-d10	15.87	176	336523	36.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	57081	17.82	ng/ul	0.00
71) Anthracene-d10	17.71	188	562303	20.14	ng/ul	0.00
79) Pyrene-d10	19.98	212	633306	39.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	640995	39.72	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.96	70	3345	1.167	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112020\
Data File : BG047380.D
Acq On : 20 Nov 2020 18:19
Operator : CG/JU
Sample : PB133083BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK83

Quant Time: Nov 21 01:29:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 21 01:27:02 2020
Response via : Initial Calibration

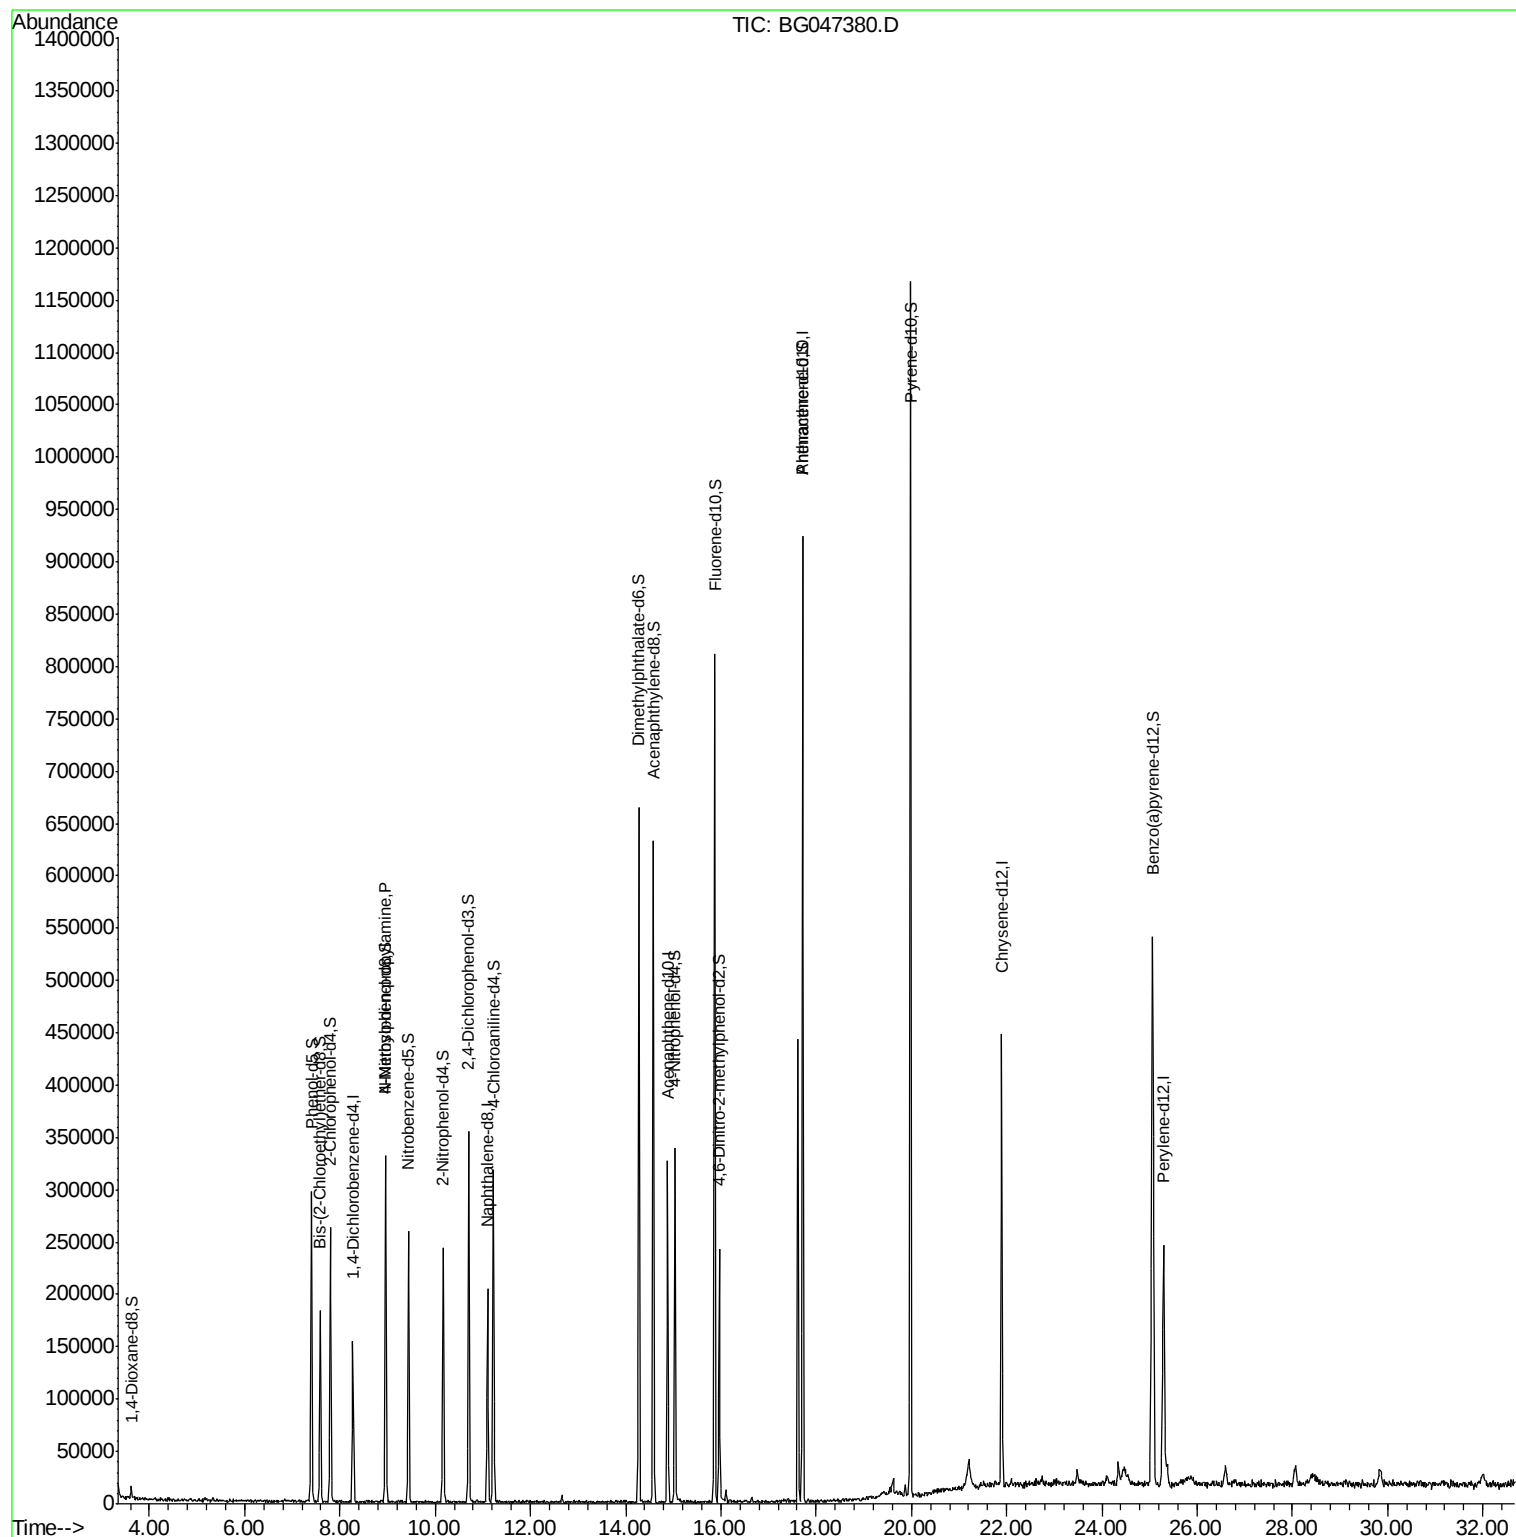

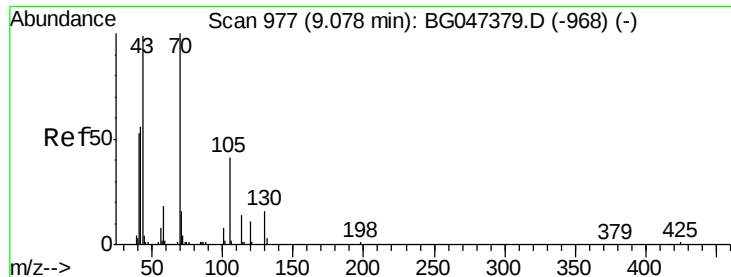

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.167 ng/ul
 RT: 8.96 min Scan# 957
 Delta R.T. -0.12 min
 Lab File: BG047380.D
 Acq: 20 Nov 2020 18:19

Instrument :
 BNA_G
 ClientSampleId :
 SBLK83

Tot Ion: 70 Resp: 3345
 Ion Ratio Lower Upper
 70 100
 42 317.7 44.2 66.2#
 101 0.0 9.0 13.6#
 130 0.0 15.1 22.7#

