

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112020\
 Data File : BG047381.D
 Acq On : 20 Nov 2020 18:59
 Operator : CG/JU
 Sample : L4711-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B51

Manual Integrations
 APPROVED

mohammad
 11/23/2020 1:29:45 PM

Quant Time: Nov 21 05:20:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Nov 21 01:27:02 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	36922	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	152653	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	118428	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	278372	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	260648	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	276282	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.63	96	1062m	1.05	ng/uL	0.01
5) Phenol-d5	7.40	99	28299	7.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.59	67	16850	7.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	20238	8.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	23331	8.20	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	10480	8.31	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	11483	8.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	24954	7.92	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	22241	6.98	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	81174	7.98	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	98235	8.36	ng/ul	0.00
52) 4-Nitrophenol-d4	15.04	143	10116	6.52	ng/ul	0.00
58) Fluorene-d10	15.86	176	75677	8.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.96	200	11260m	7.11	ng/ul	-0.01
71) Anthracene-d10	17.72	188	120770m	8.75	ng/ul	0.00
79) Pyrene-d10	19.98	212	131367	8.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	131292	8.26	ng/ul	0.00

Target Compounds

					Ovalue	
45) Dimethylphthalate	14.32	163	36647	3.534	ng/ul#	97
77) Fluoranthene	19.64	202	38104	2.007	ng/ul#	93
80) Pyrene	20.01	202	32500	1.760	ng/ul	98
83) Benzo(a)anthracene	21.88	228	19795m	1.067	ng/ul	
84) Bis(2-ethylhexyl)phthalate	21.77	149	25966	2.873	ng/ul	94
85) Chrysene	21.95	228	22020	1.248	ng/ul	97
88) Benzo(b)fluoranthene	24.21	252	25353	1.300	ng/ul#	92
91) Benzo(a)pyrene	25.13	252	19992m	1.150	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112020\
Data File : BG047381.D
Acq On : 20 Nov 2020 18:59
Operator : CG/JU
Sample : L4711-09
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0B51

Manual Integrations
APPROVED

mohammad
11/23/2020 1:29:45 PM

Quant Time: Nov 21 05:20:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Nov 21 01:27:02 2020
Response via : Initial Calibration

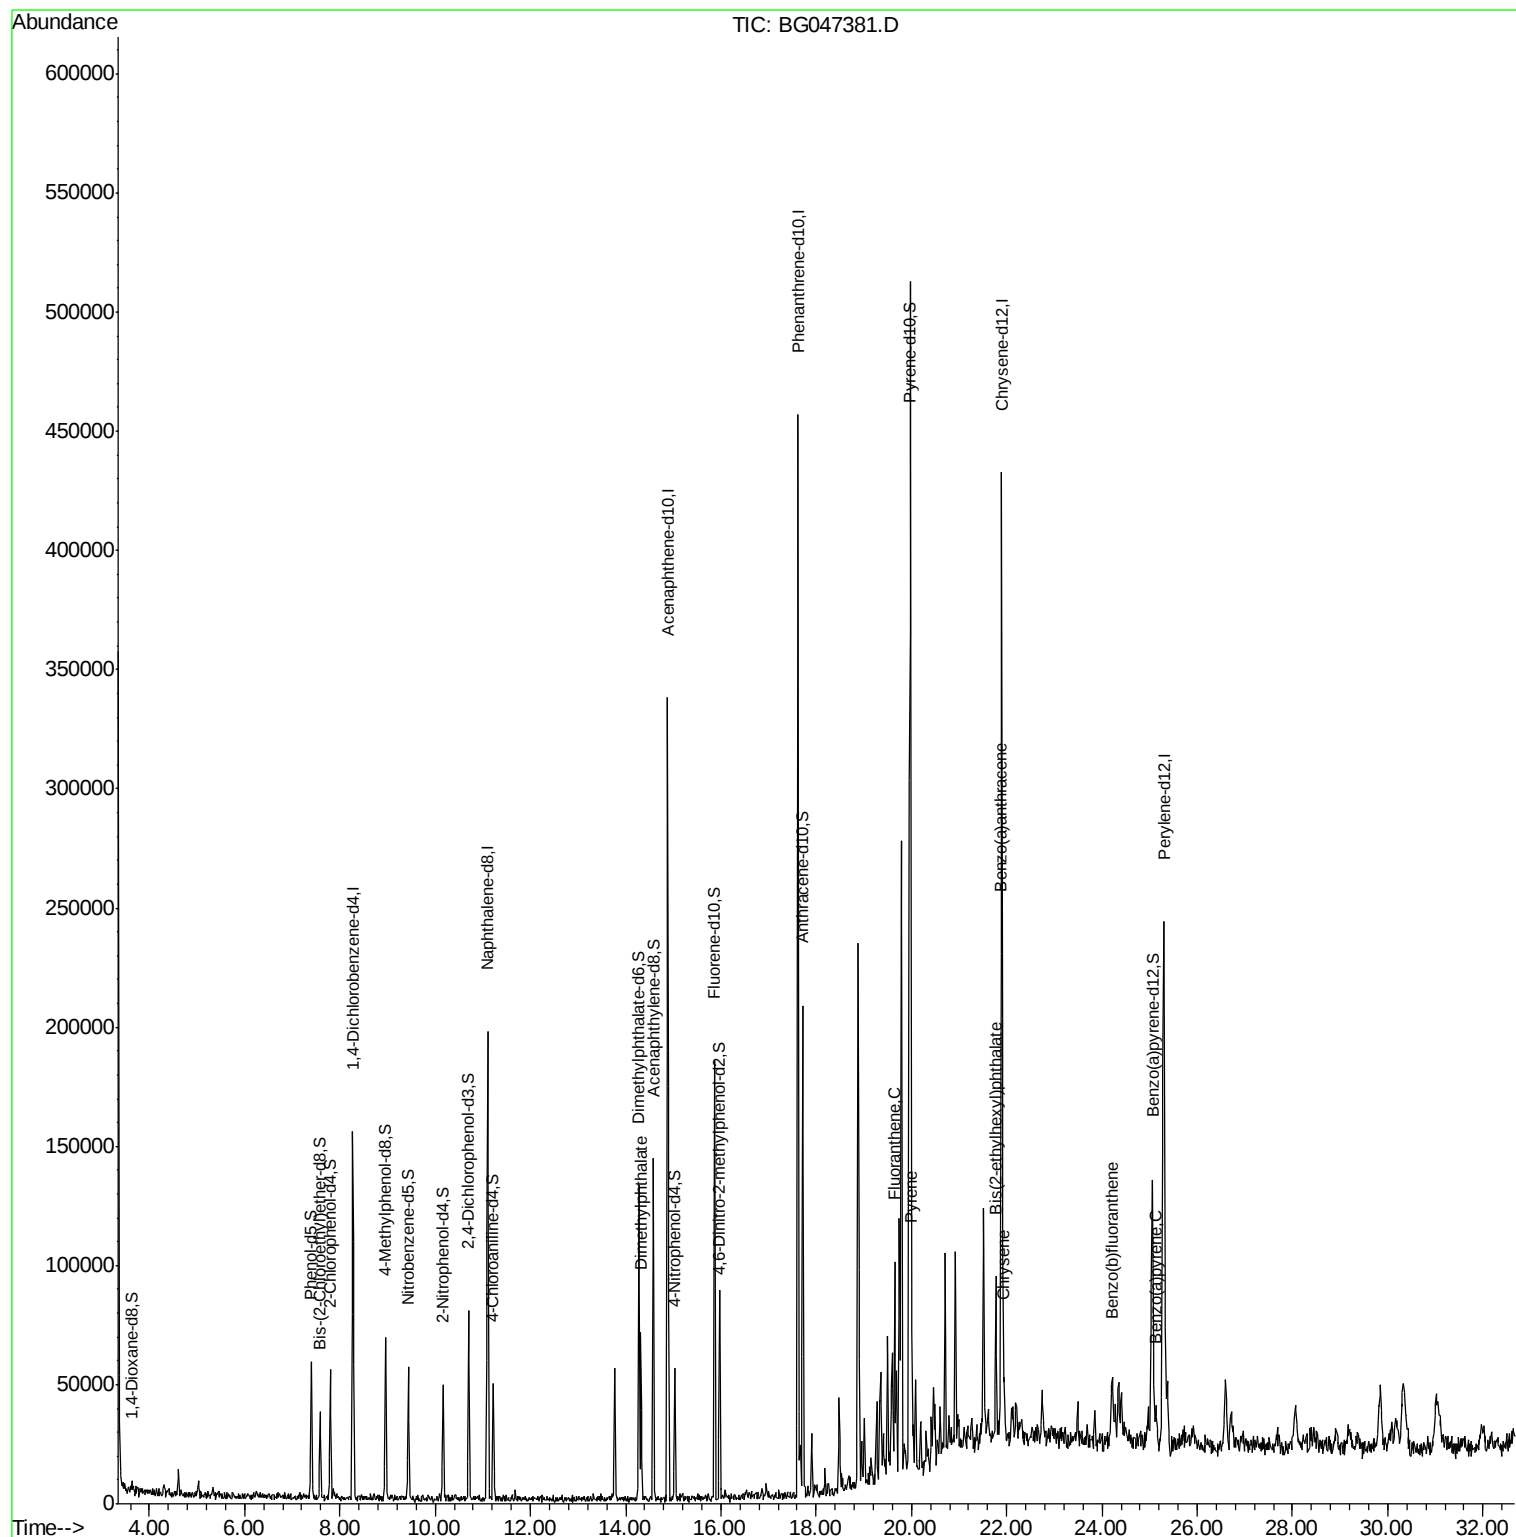

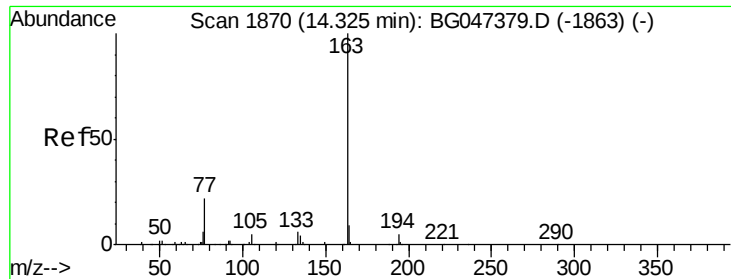

#45

Dimethylphthalate

Concen: 3.534 ng/ul

RT: 14.32 min Scan# 1869

Delta R.T. -0.01 min

Lab File: BG047381.D

Acq: 20 Nov 2020 18:59

Instrument :

BNA_G





ClientSampleId :

C0B51

Tot Ion:	163	Resp:	36647
Ion Ratio	Lower	Upper	
163	100		
194	3.4	3.4	5.2#
164	12.4	8.8	13.2

Manual Integrations
APPROVED

mohammad
11/23/2020 1:29:45 PM

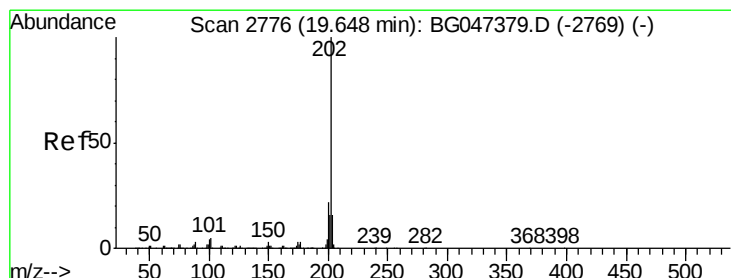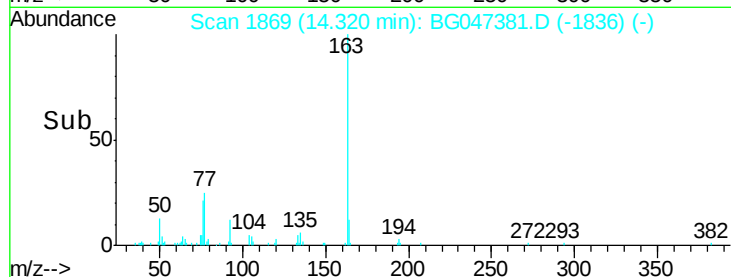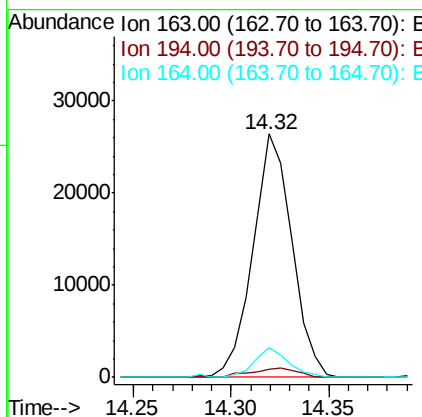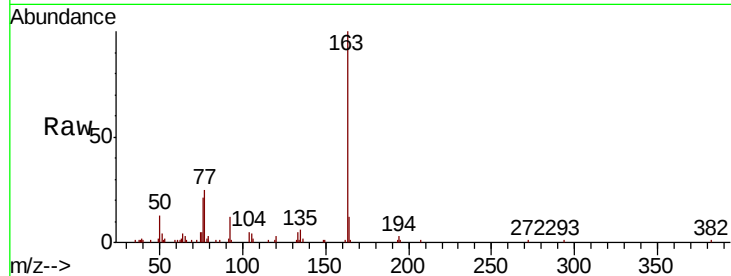

#77

Fluoranthene

Concen: 2.007 ng/ul




RT: 19.64 min Scan# 2775


Delta R.T. -0.01 min

Lab File: BG047381.D

Acq: 20 Nov 2020 18:59

Tgt Ion:	202	Resp:	38104
Ion Ratio	Lower	Upper	
202	100		
101	4.7	3.3	4.9
100	7.9	3.4	5.0#

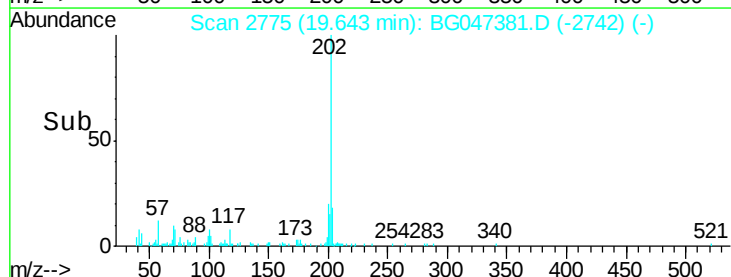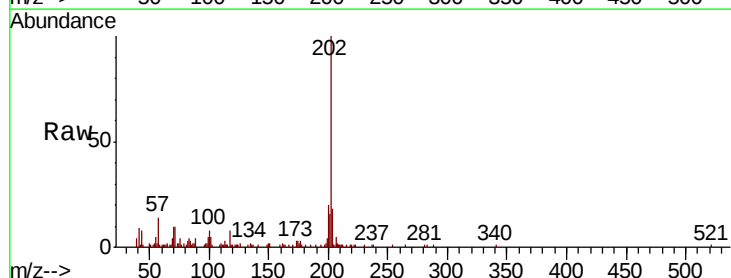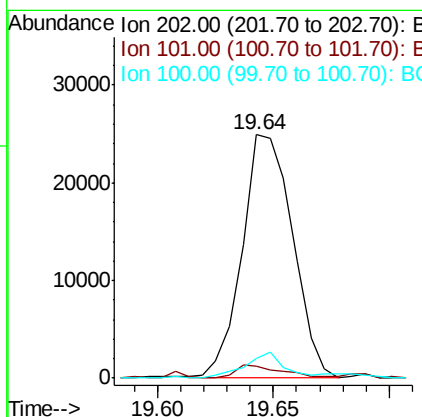

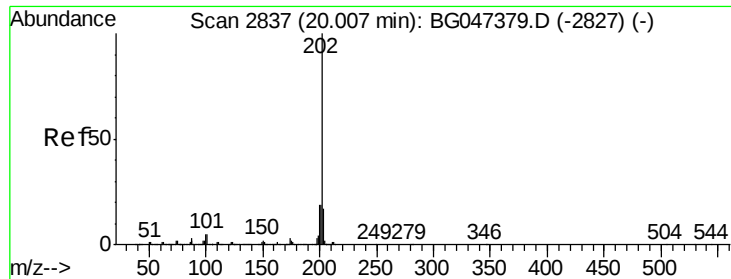





#80
Pvrene
Concen: 1.760 ng/ul
RT: 20.01 min Scan# 2837
Delta R.T. -0.00 min
Lab File: BG047381.D
Acq: 20 Nov 2020 18:59

Instrument :
BNA_G
ClientSampleId :
C0B51

Tot Ion	Ratio	Lower	Upper
202	100		
101	5.0	5.0	7.4
100	6.2	4.6	7.0




Manual Integrations
APPROVED


mohammad
11/23/2020 1:29:45 PM

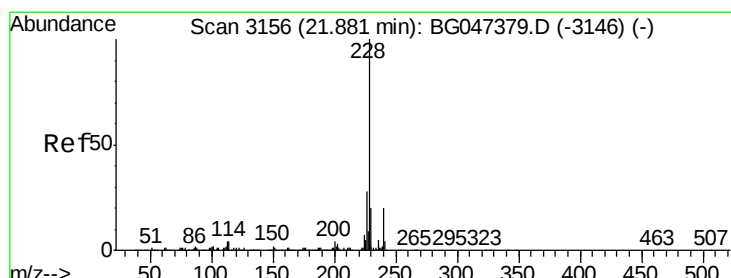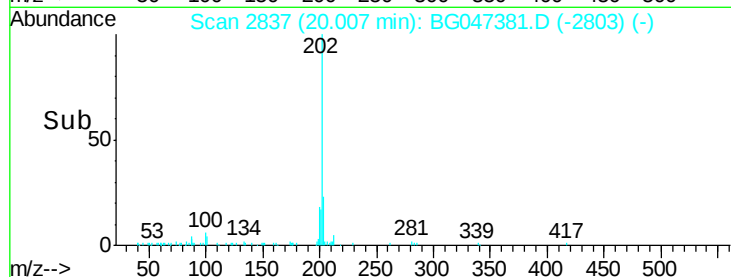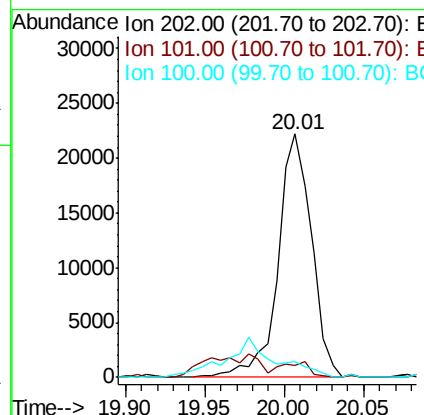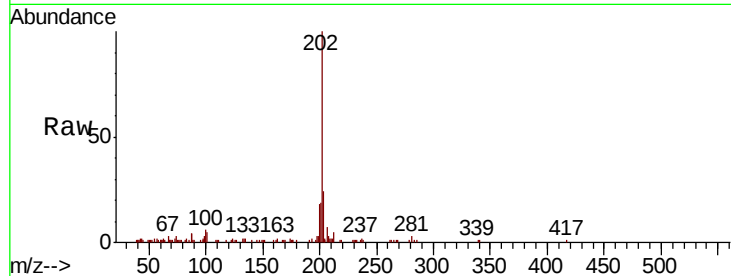

#83
Benzo(a)anthracene
Concen: 1.067 ng/ul m
RT: 21.88 min Scan# 3155
Delta R.T. -0.01 min
Lab File: BG047381.D
Acq: 20 Nov 2020 18:59

Tgt Ion	Ratio	Lower	Upper
228	100		
229	16.5	16.2	24.2
226	20.9	23.3	34.9#

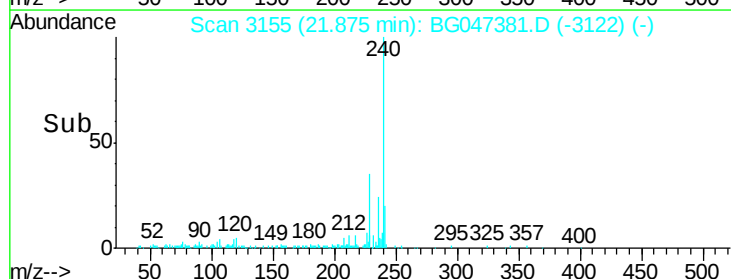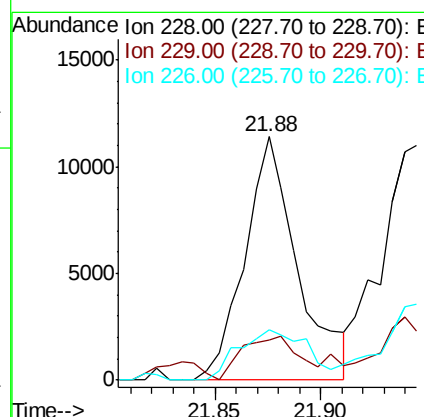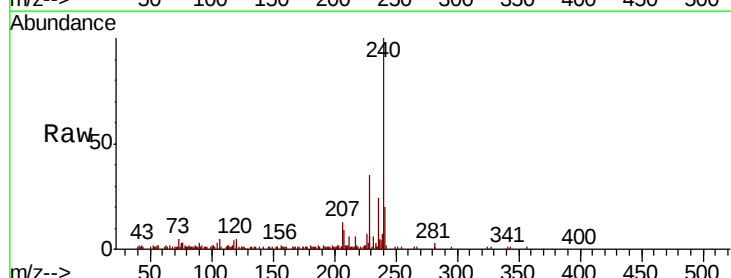

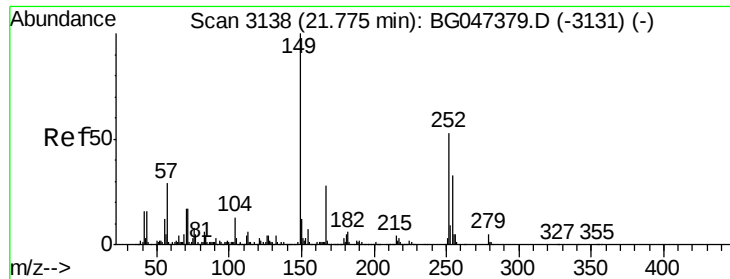

#84

Bis(2-ethylhexyl)phthalate

Concen: 2.873 ng/ul

RT: 21.77 min Scan# 3137

Delta R.T. -0.01 min

Lab File: BG047381.D

Acq: 20 Nov 2020 18:59

Instrument :

BNA_G


ClientSampled :

C0B51




Tot Ion:	149	Resp:	25966
Ion Ratio	Lower	Upper	
149	100		
167	31.1	21.8	32.8
279	5.5	4.2	6.2

Manual Integrations
APPROVED

mohammad
11/23/2020 1:29:45 PM

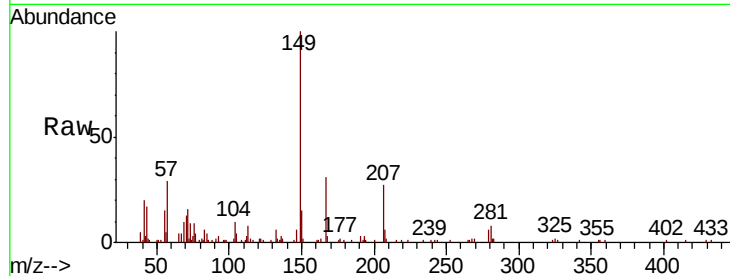

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

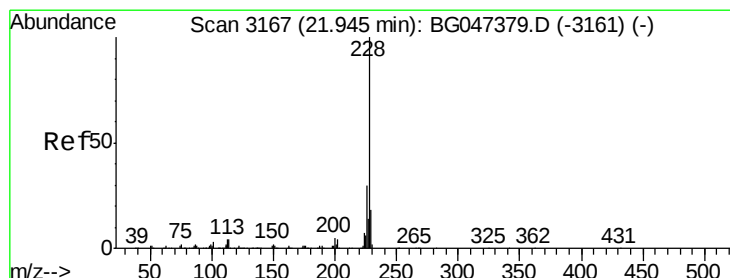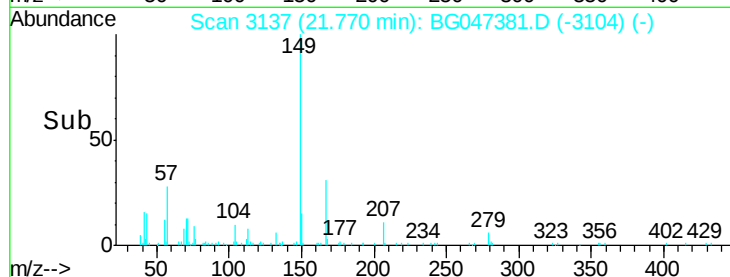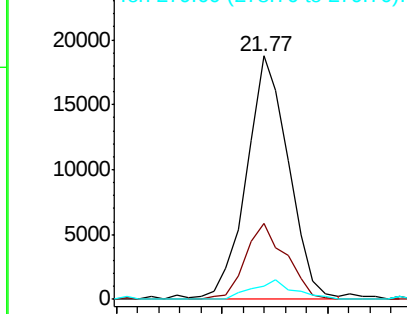

#85

Chrysene

Concen: 1.248 ng/ul


RT: 21.95 min Scan# 3167

Delta R.T. -0.00 min



Lab File: BG047381.D


Acq: 20 Nov 2020 18:59

Tgt Ion:	228	Resp:	22020
Ion Ratio	Lower	Upper	
228	100		
226	32.6	23.8	35.6
229	20.2	16.3	24.5

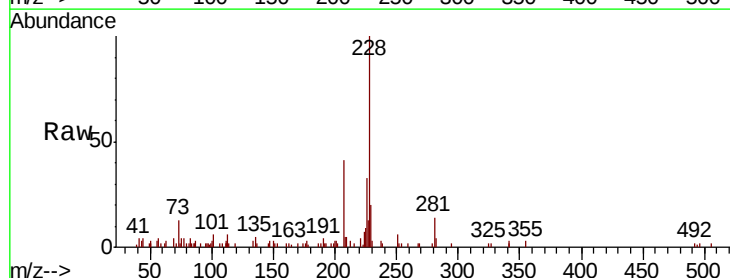

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

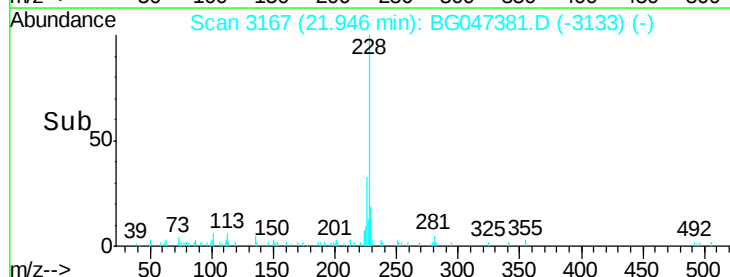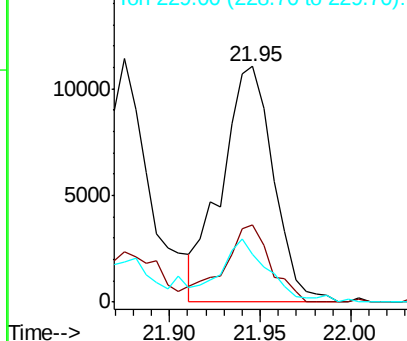

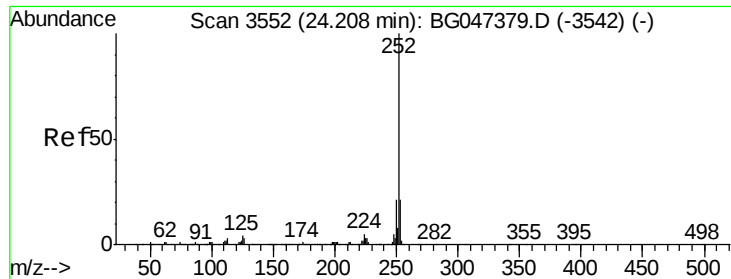

#88

Benzo(b)fluoranthene

Concen: 1.300 ng/uL

RT: 24.21 min Scan# 3552

Delta R.T. -0.00 min

Lab File: BG047381.D

Acq: 20 Nov 2020 18:59

Instrument :

BNA_G


ClientSampled :

C0B51




Tot Ion:	252	Resp:	25353
Ion Ratio	Lower	Upper	
252	100		
253	26.8	18.4	27.6
125	5.6	2.5	3.7#

Manual Integrations
APPROVED

mohammad
11/23/2020 1:29:45 PM

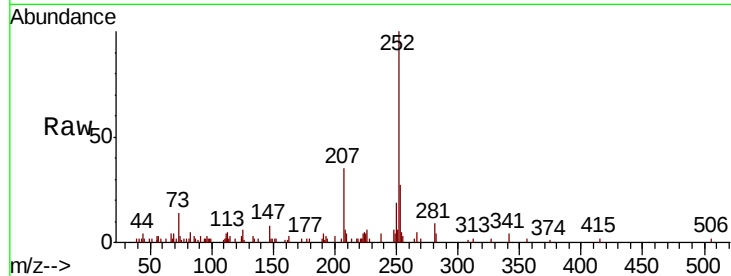

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

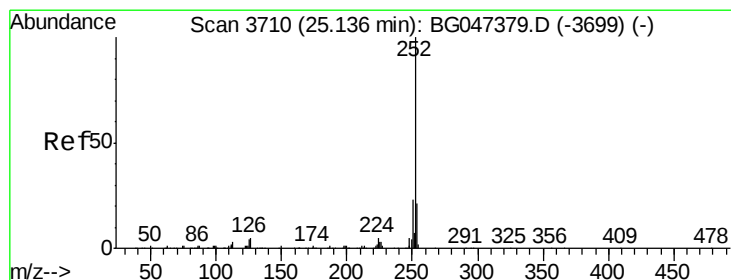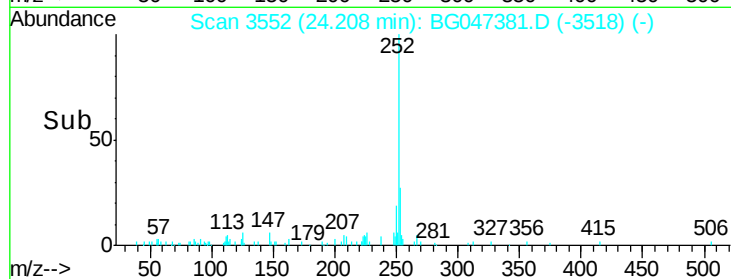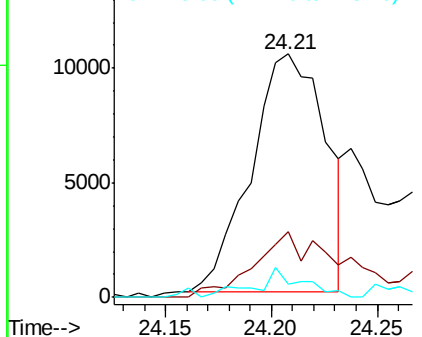

#91

Benzo(a)pyrene

Concen: 1.150 ng/uL m

RT: 25.13 min Scan# 3709

Delta R.T. -0.01 min

Lab File: BG047381.D

Acq: 20 Nov 2020 18:59

Tgt Ion:	252	Resp:	19992
Ion Ratio	Lower	Upper	
252	100		
253	25.3	17.5	26.3
125	0.0	3.1	4.7#

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

