
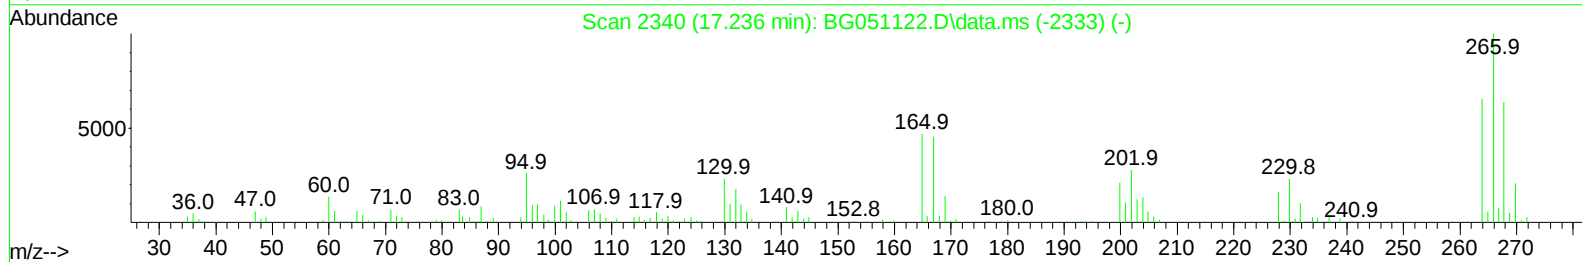
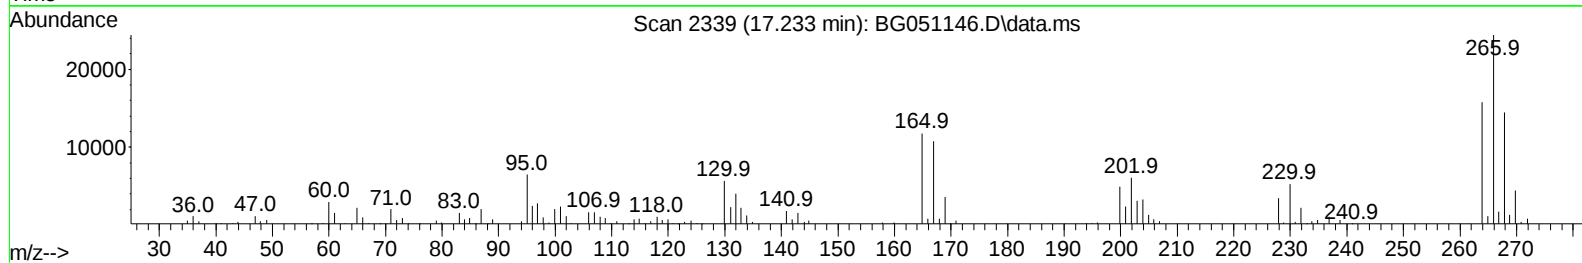


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
Data File : BG051146.D
Acq On : 20 Nov 2021 13:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 02:57:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

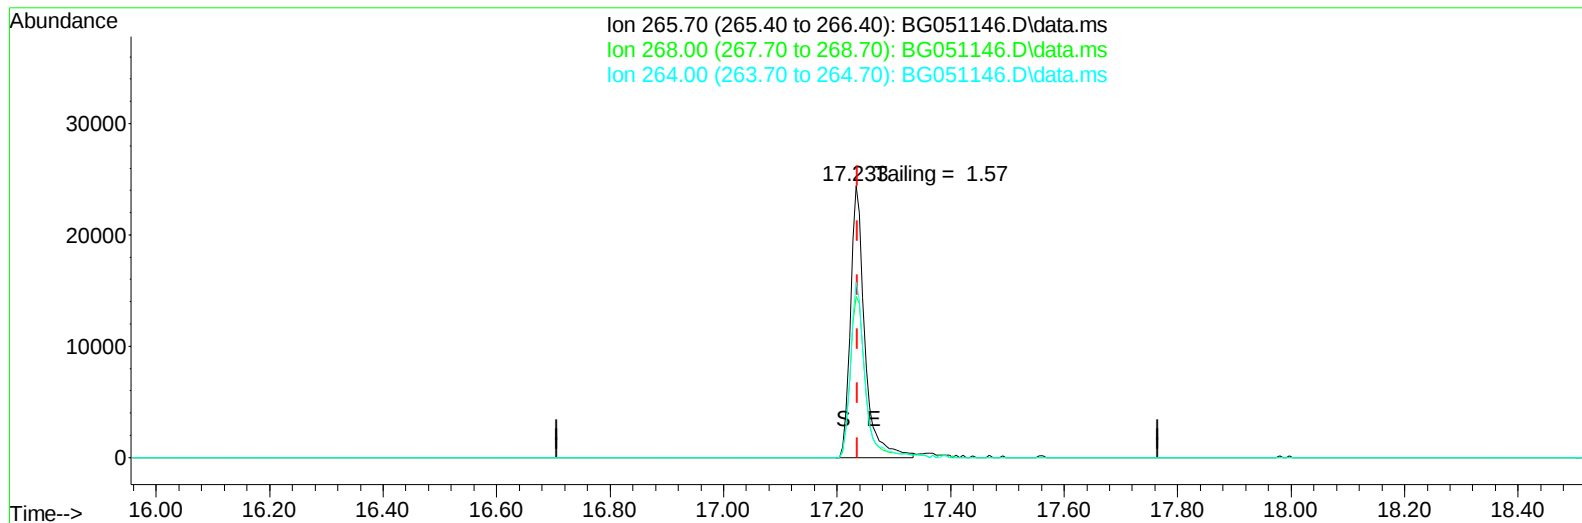

TIC: BG051146.D\data.ms

(70) Pentachlorophenol (C)




17.233min (-0.002) 5643.56 ng

response 43040

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	59.29
264.00	61.30	64.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112021\
Data File : BG051146.D
Acq On : 20 Nov 2021 13:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 02:57:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG11921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 16:26:22 2021
Response via : Initial Calibration

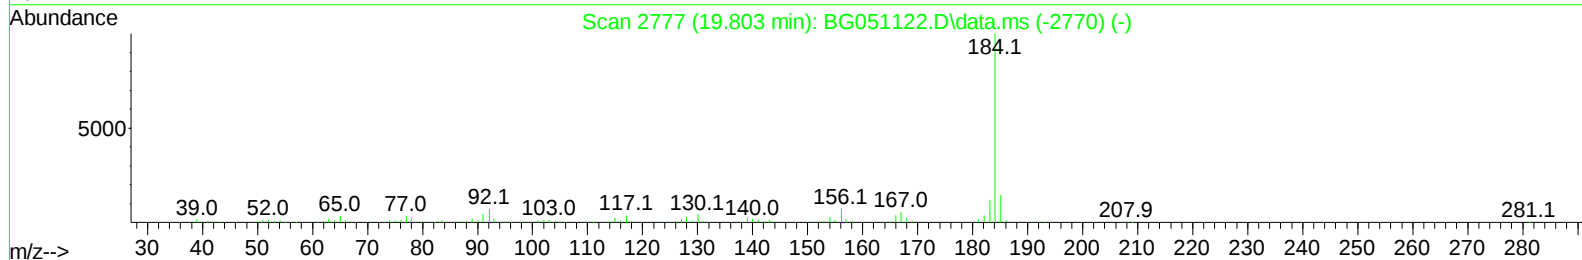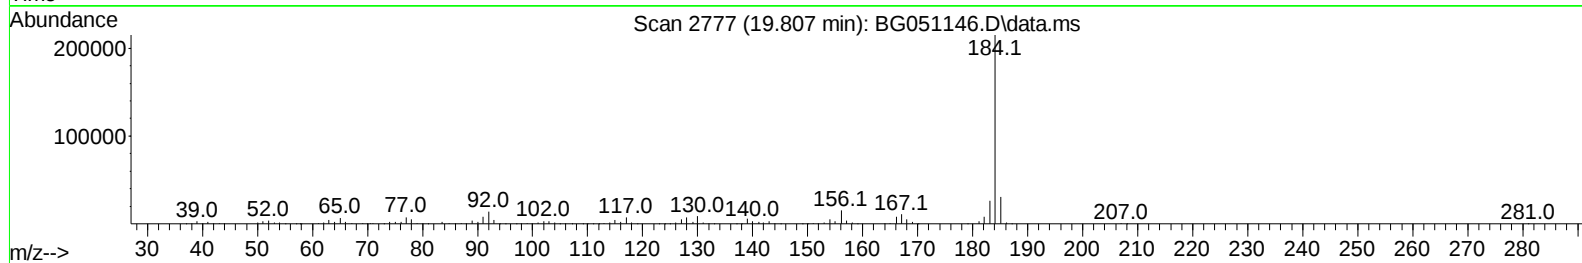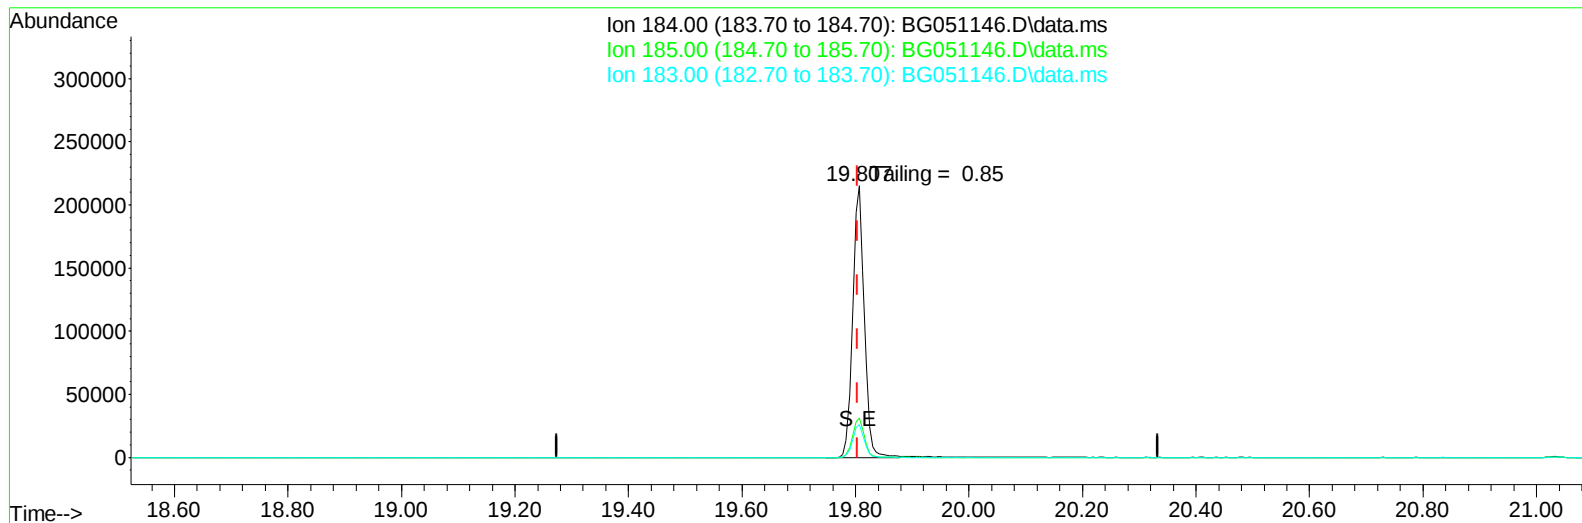

TIC: BG051146.D\data.ms

(77) Benzidine**19.807min (+ 0.004) 51022.59 ng****response 306635**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.42
183.00	11.70	12.18
0.00	0.00	0.00